

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111022\
 Data File : FF011624.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2022 00:54
 Operator : YP\AJ
 Sample : N5531-14MS
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WC-28MS

Integration File: Sample.e
 Quant Time: Nov 11 05:36:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.055	1435016	12.095 ug/ml
Target Compounds			
2) N-DECANE	4.616	2307399	17.482 ug/ml
3) N-DODECANE	6.776	2418422	17.994 ug/ml
4) N-TETRADECANE	8.601	2489644	18.397 ug/ml
5) N-HEXADECANE	10.207	2577782	18.751 ug/ml
6) N-OCTADECANE	11.649	2551094	18.443 ug/ml
7) N-EICOSANE	12.958	2444389	17.675 ug/ml
8) N-DOCOSANE	14.157	2386741	17.683 ug/ml
10) N-TETRACOSANE	15.260	2371069	17.484 ug/ml
11) N-HEXACOSANE	16.281	2291199	17.149 ug/ml
12) N-OCTACOSANE	17.231	2256549	17.033 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111022\
Data File : FF011624.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2022 00:54
Operator : YP\AJ
Sample : N5531-14MS
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-28MS

Integration File: Sample.e
Quant Time: Nov 11 05:36:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

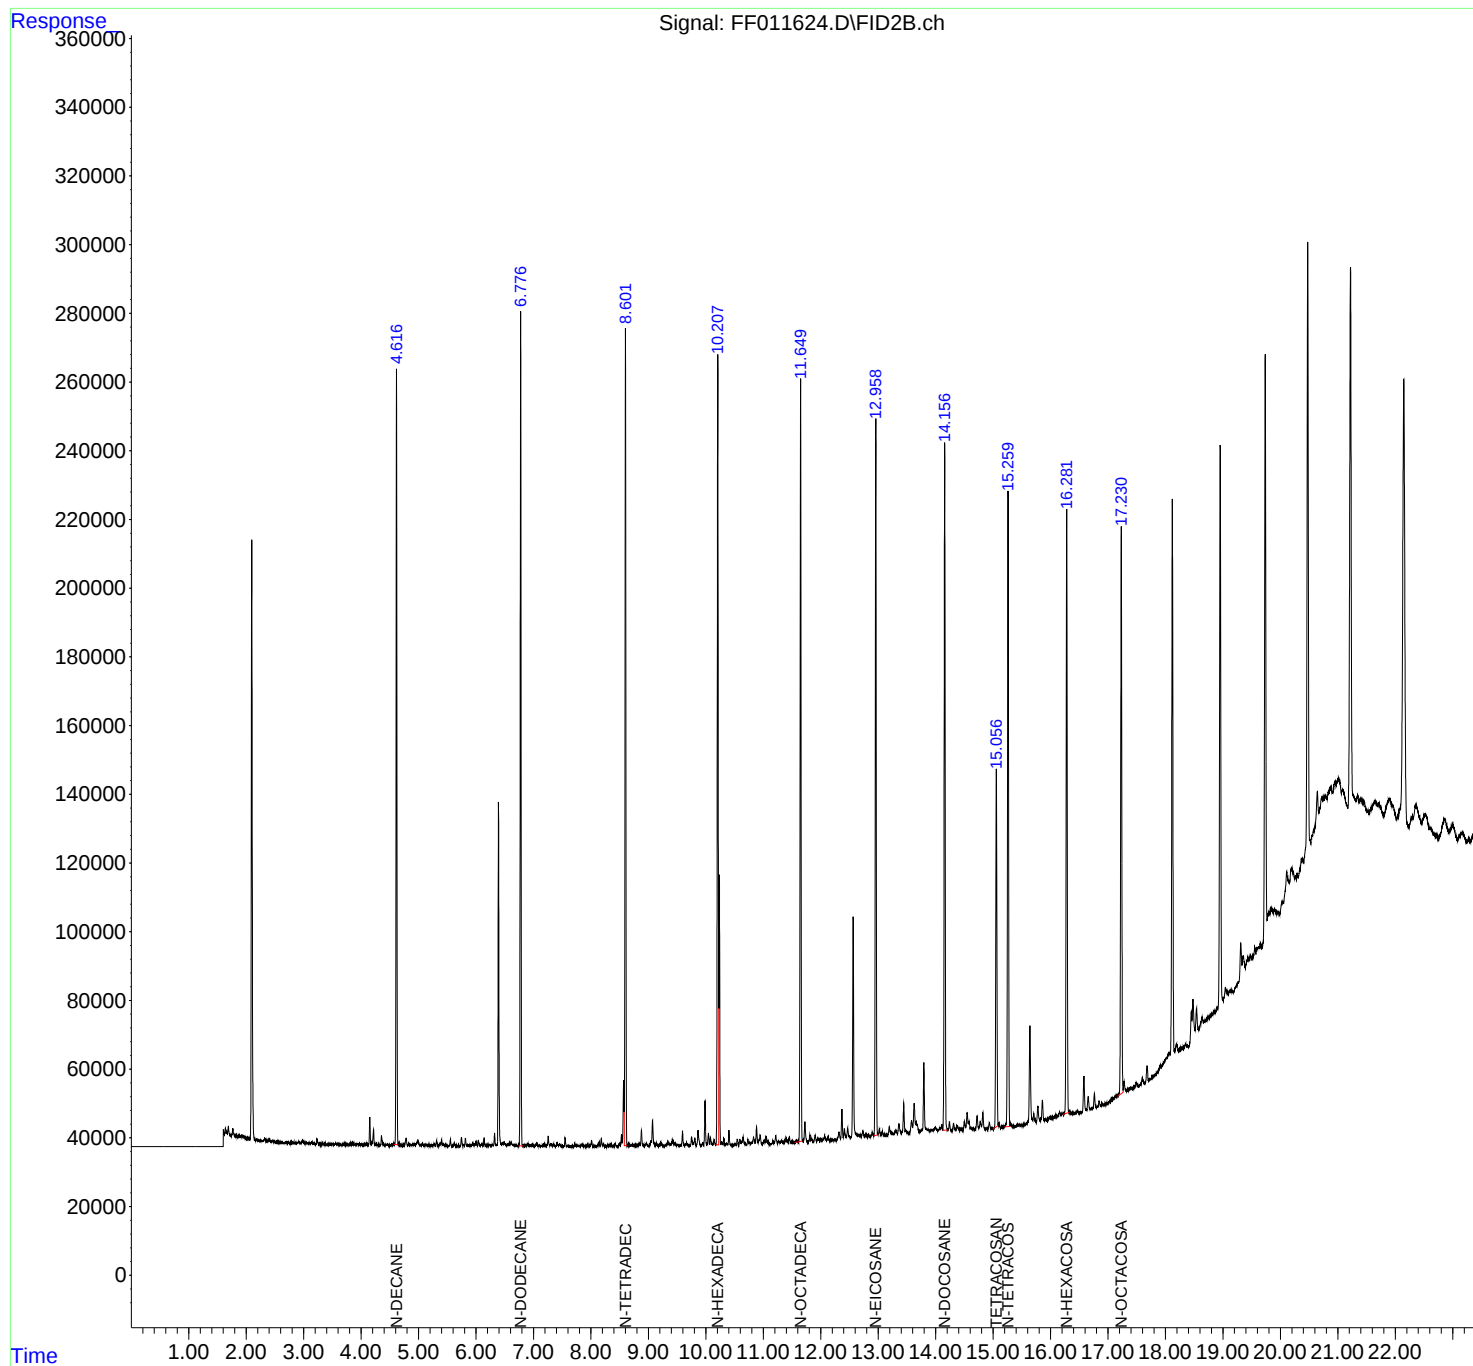


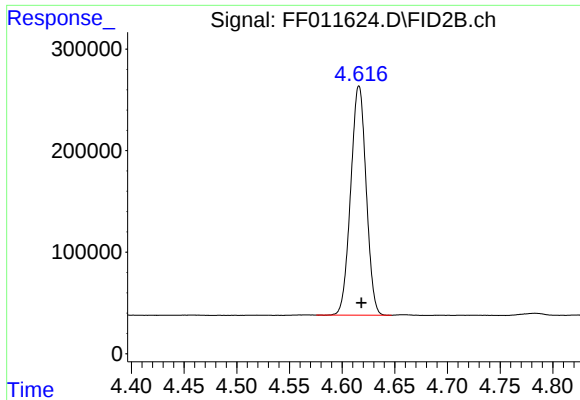

#2 N-DECANE


R.T.: 4.616 min
Delta R.T.: -0.002 min
Response: 2307399
Conc: 17.48 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-28MS

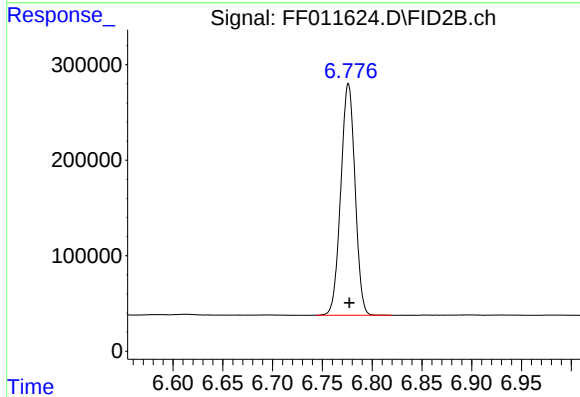


#3 N-DODECANE

R.T.: 6.776 min
Delta R.T.: -0.001 min
Response: 2418422
Conc: 17.99 ug/ml

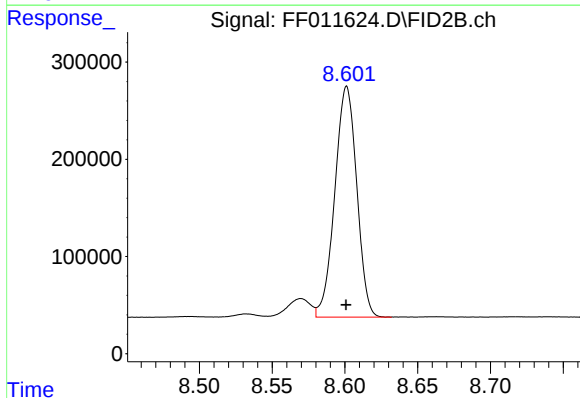


#4 N-TETRADECANE

R.T.: 8.601 min
Delta R.T.: 0.000 min
Response: 2489644
Conc: 18.40 ug/ml

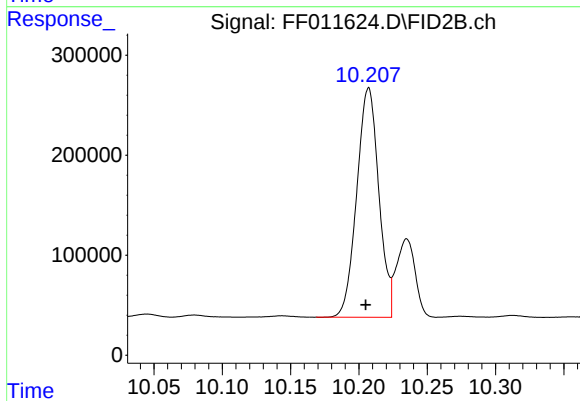

#5 N-HEXADECANE


R.T.: 10.207 min
Delta R.T.: 0.002 min
Response: 2577782
Conc: 18.75 ug/ml

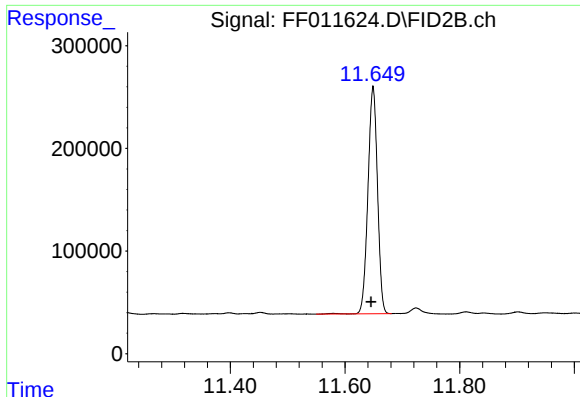

#6 N-OCTADECANE


R.T.: 11.649 min
Delta R.T.: 0.004 min
Response: 2551094
Conc: 18.44 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-28MS

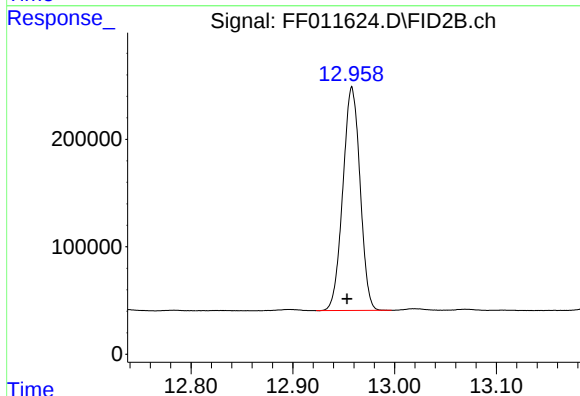


#7 N-EICOSANE

R.T.: 12.958 min
Delta R.T.: 0.005 min
Response: 2444389
Conc: 17.67 ug/ml

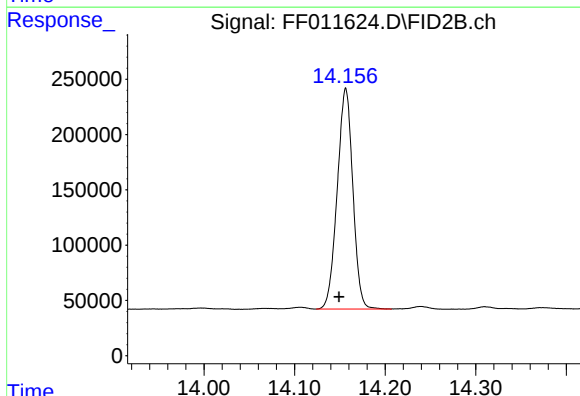


#8 N-DOCOSANE

R.T.: 14.157 min
Delta R.T.: 0.007 min
Response: 2386741
Conc: 17.68 ug/ml

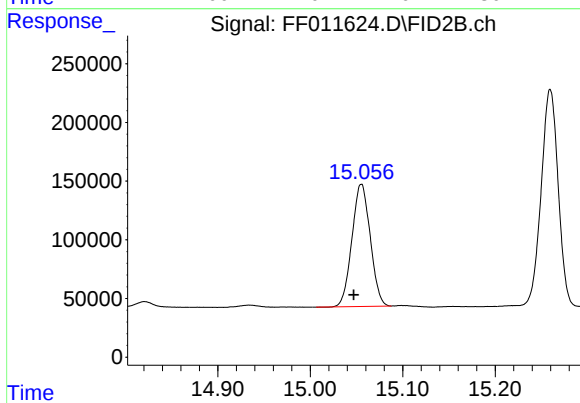

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.055 min
Delta R.T.: 0.008 min
Response: 1435016
Conc: 12.10 ug/ml

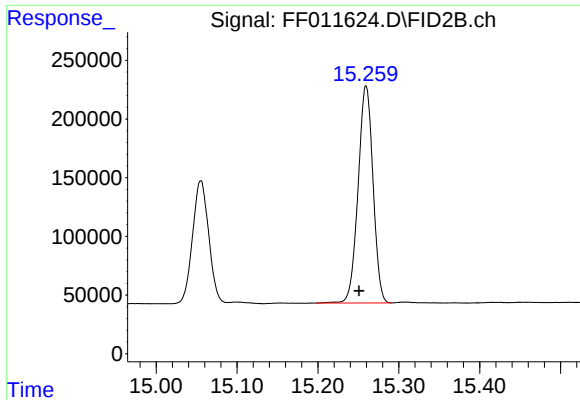

#10 N-TETRACOSANE


R.T.: 15.260 min
Delta R.T.: 0.009 min
Response: 2371069
Conc: 17.48 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-28MS

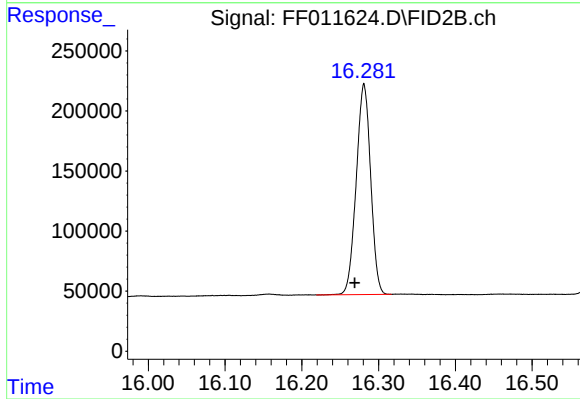

#11 N-HEXACOSANE

R.T.: 16.281 min
Delta R.T.: 0.012 min
Response: 2291199
Conc: 17.15 ug/ml

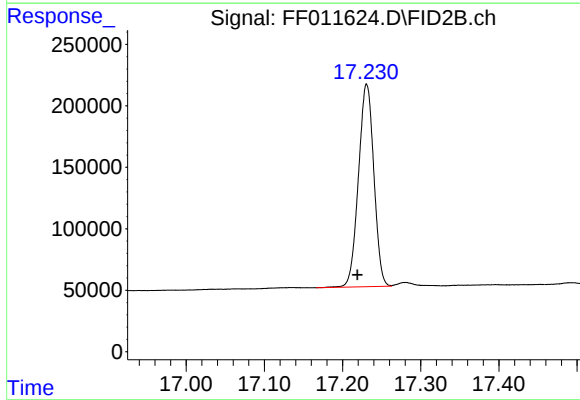

#12 N-OCTACOSANE

R.T.: 17.231 min
Delta R.T.: 0.012 min
Response: 2256549
Conc: 17.03 ug/ml