

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
 Data File : FF007854.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2020 14:05
 Operator : DD\AJ
 Sample : L4680-05
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 12 01:57:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.714	2216764	17.354 ug/ml
Target Compounds			
4) N-TETRADECANE	8.318f	1237143	8.761 ug/ml
7) N-EICOSANE	12.681f	1016979	6.861 ug/ml
10) N-TETRACOSANE	14.906	453862	3.138 ug/ml
12) N-OCTACOSANE	16.915	148606	1.096 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007854.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 14:05
Operator : DD\AJ
Sample : L4680-05
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 01:57:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

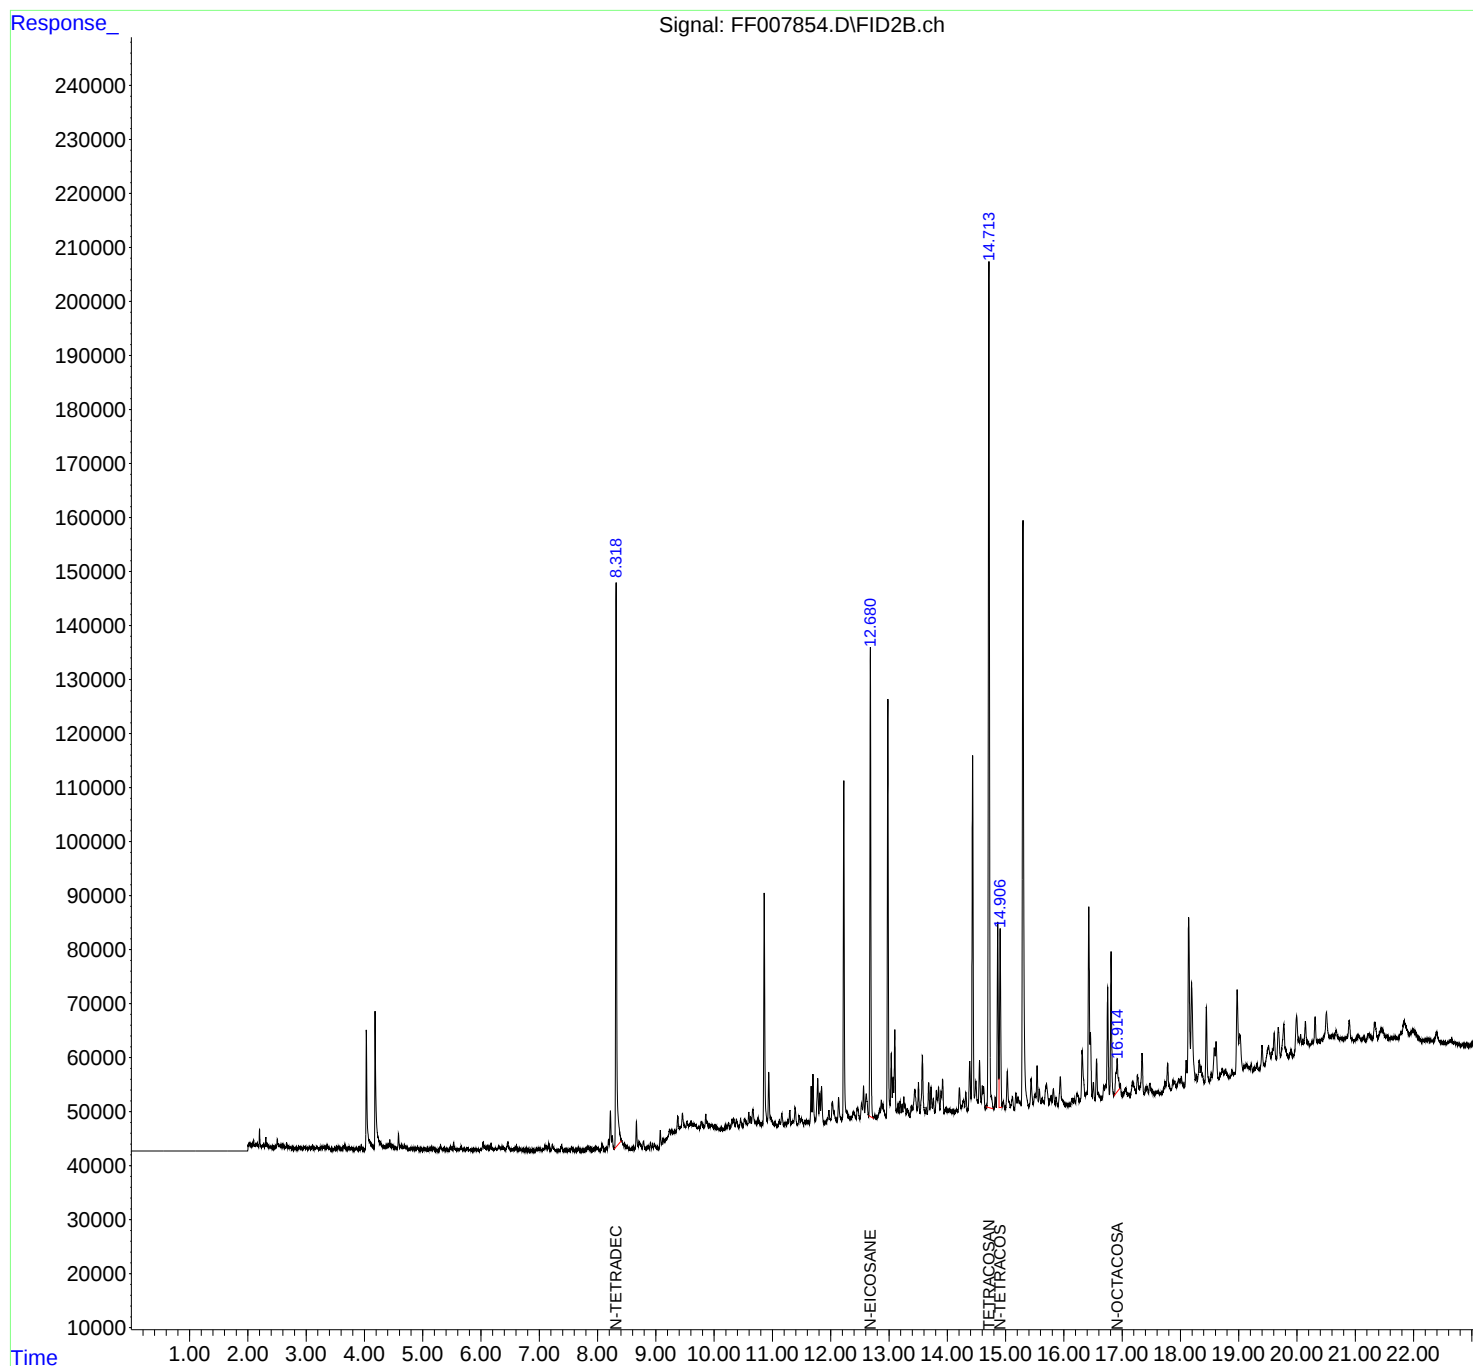


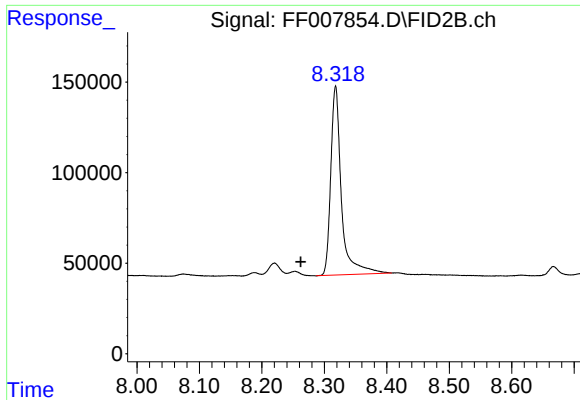

#4 N-TETRADECANE


R.T.: 8.318 min
Delta R.T.: 0.056 min
Response: 1237143
Conc: 8.76 ug/ml

Instrument :
FID_F
ClientSampleId :

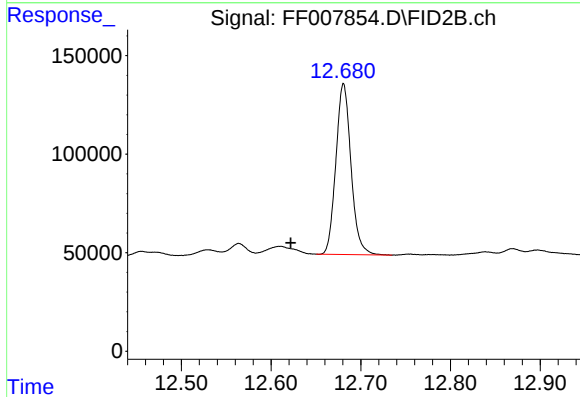


#7 N-EICOSANE

R.T.: 12.681 min
Delta R.T.: 0.059 min
Response: 1016979
Conc: 6.86 ug/ml

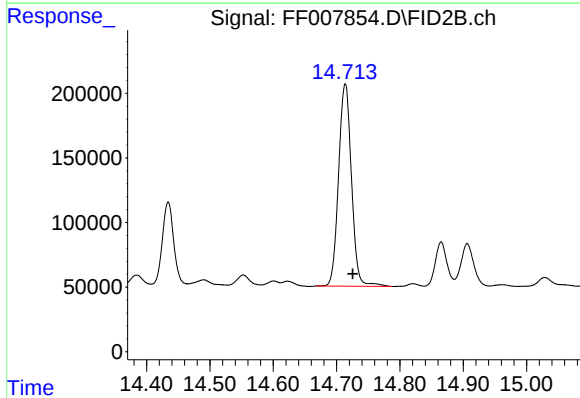


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.714 min
Delta R.T.: -0.012 min
Response: 2216764
Conc: 17.35 ug/ml

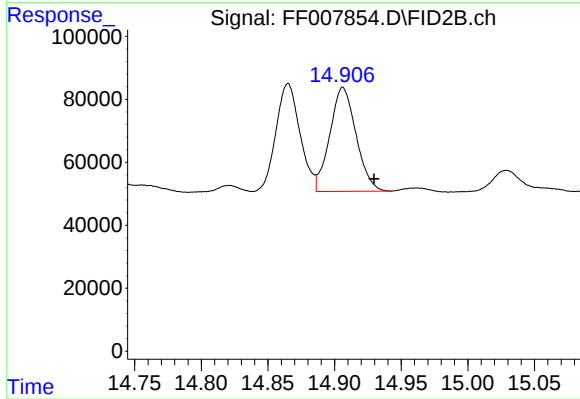

#10 N-TETRACOSANE

R.T.: 14.906 min
Delta R.T.: -0.023 min
Response: 453862
Conc: 3.14 ug/ml

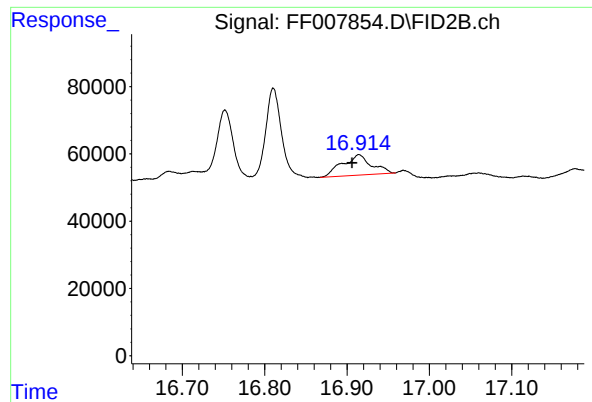

#12 N-OCTACOSANE

R.T.: 16.915 min
Delta R.T.: 0.008 min
Response: 148606
Conc: 1.10 ug/ml

Instrument :
FID_F
ClientSampleId :