

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
 Data File : FF007857.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2020 15:39
 Operator : DD\AJ
 Sample : L4622-03 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 12 01:58:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	197274	1.544 ug/ml
Target Compounds			
7) N-EICOSANE	12.685f	819181	5.527 ug/ml
10) N-TETRACOSANE	14.913	279352	1.932 ug/ml
12) N-OCTACOSANE	16.923	237083	1.748 ug/ml
14) N-DOTRIACONTANE	18.621	175190	1.511 ug/ml
15) N-TETRATRIACONTANE	19.417	211599	2.253 ug/ml
16) N-HEXATRIACONTANE	20.203	825194	10.864 ug/ml
17) N-OCTATRIACONTANE	20.845f	263191	4.236 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007857.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 15:39
Operator : DD\AJ
Sample : L4622-03 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 01:58:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

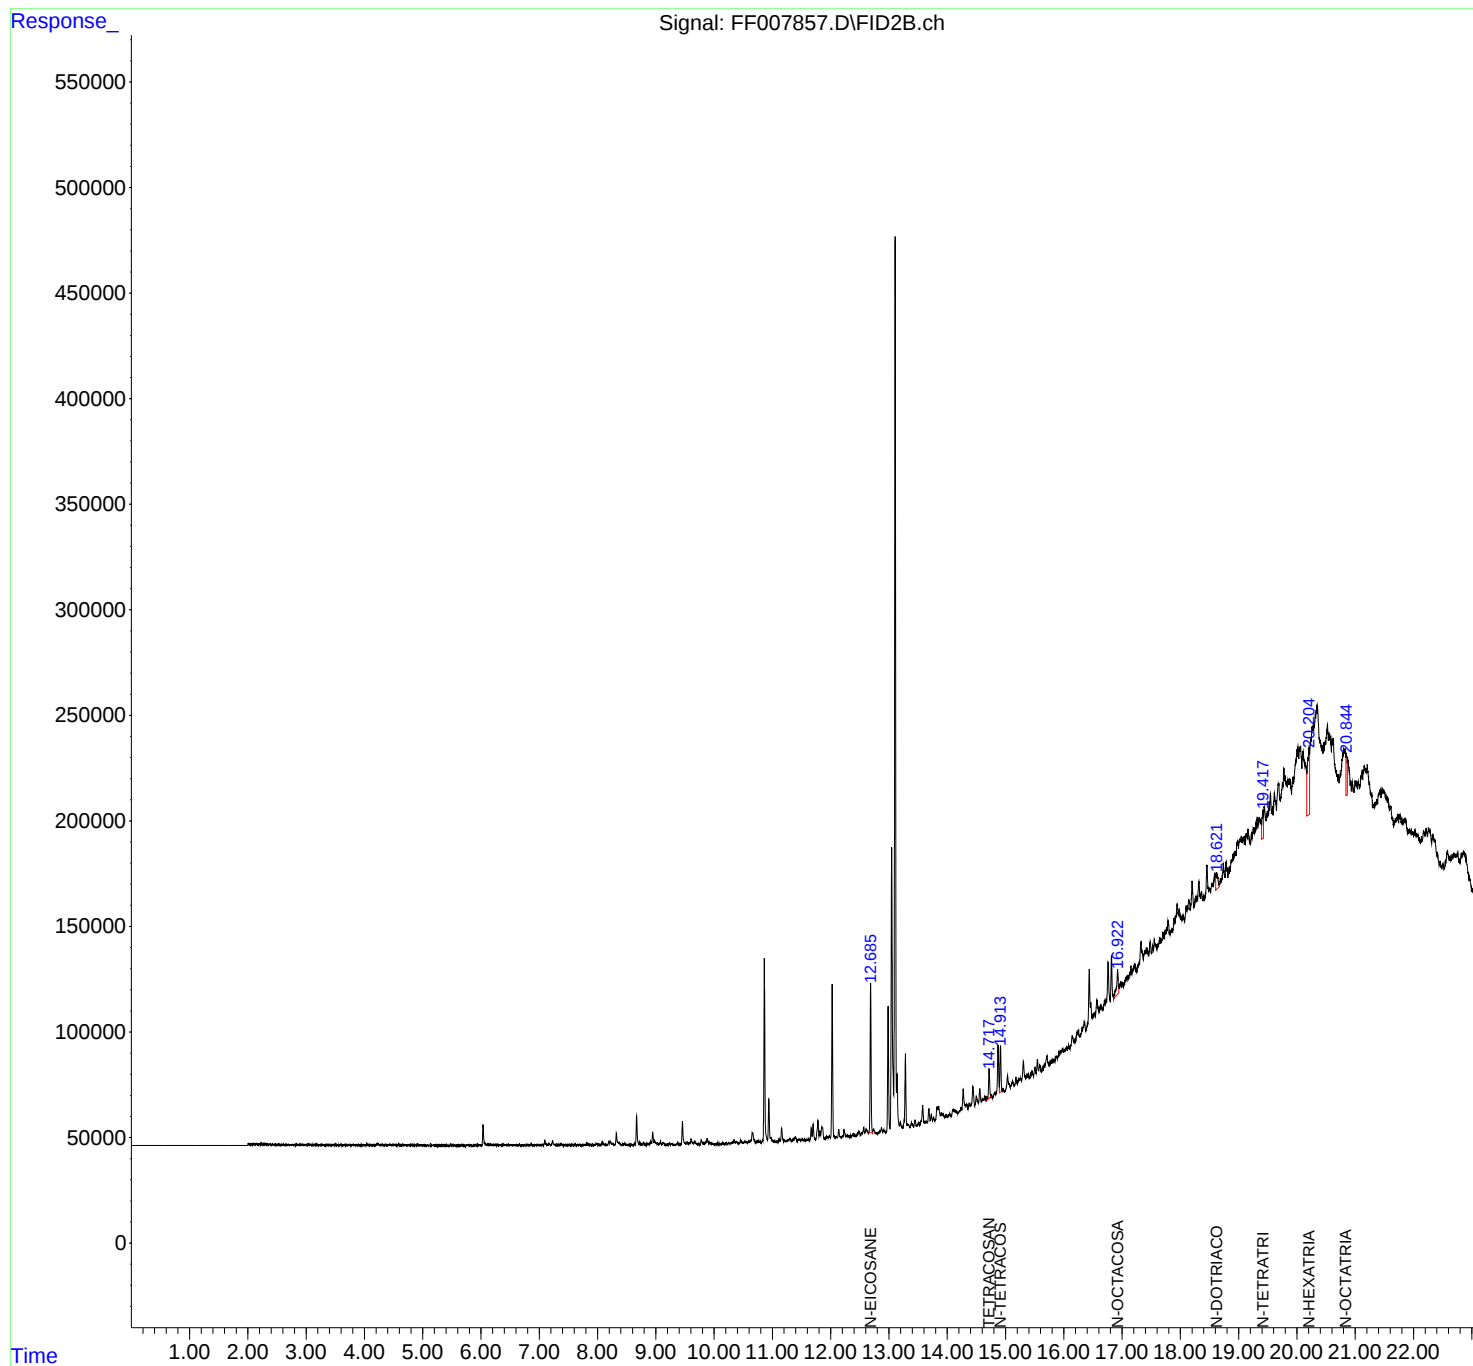


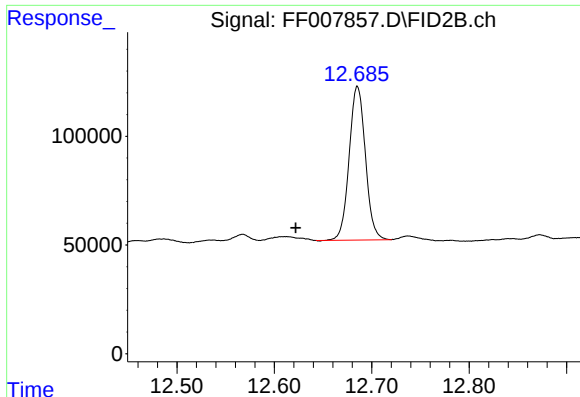

#7 N-EICOSANE


R.T.: 12.685 min
Delta R.T.: 0.063 min
Response: 819181
Conc: 5.53 ug/ml

Instrument :
FID_F
ClientSampleId :

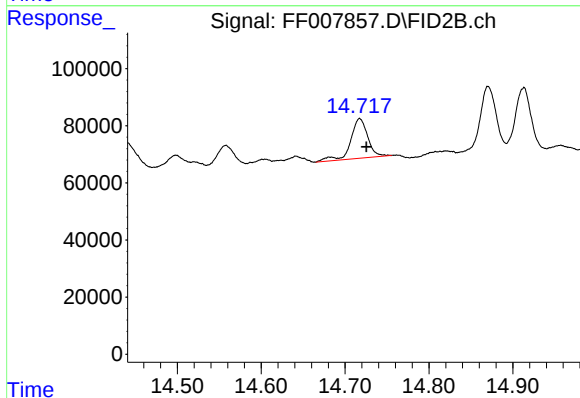


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.717 min
Delta R.T.: -0.008 min
Response: 197274
Conc: 1.54 ug/ml

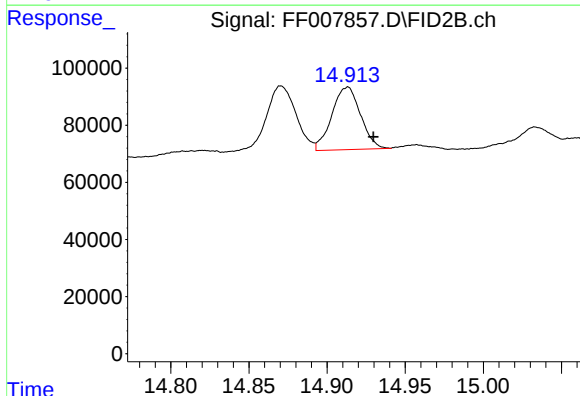


#10 N-TETRACOSANE

R.T.: 14.913 min
Delta R.T.: -0.017 min
Response: 279352
Conc: 1.93 ug/ml

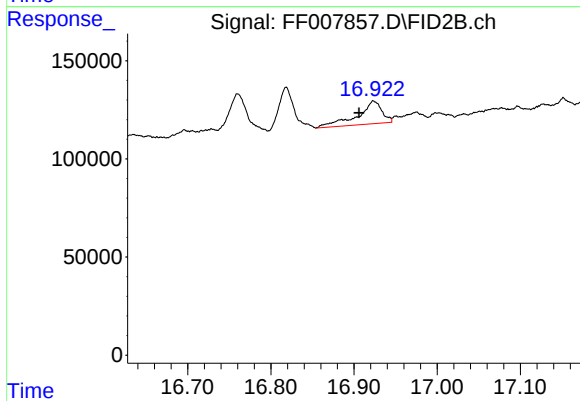

#12 N-OCTACOSANE


R.T.: 16.923 min
Delta R.T.: 0.017 min
Response: 237083
Conc: 1.75 ug/ml

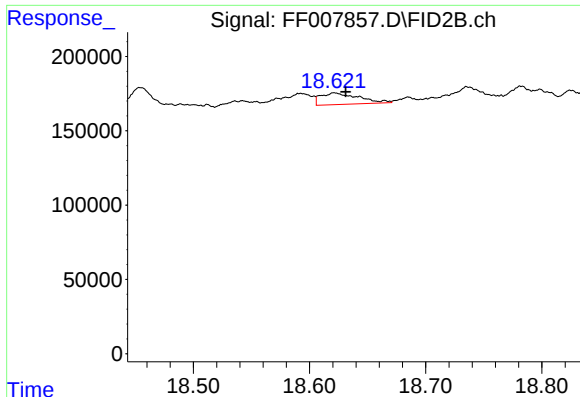

#14 N-DOTRIACONTANE


R.T.: 18.621 min
Delta R.T.: -0.010 min
Response: 175190
Conc: 1.51 ug/ml

Instrument :
FID_F
ClientSampleId :

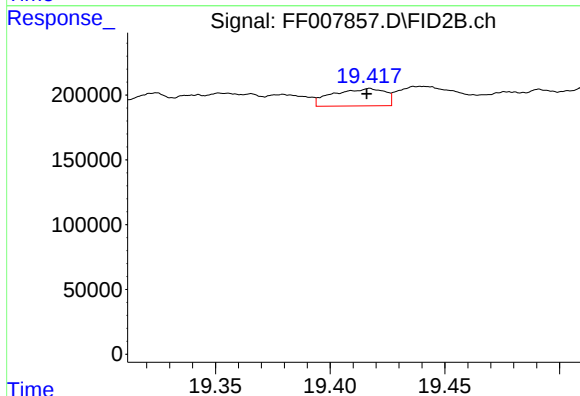


#15 N-TETRATRIACONTANE

R.T.: 19.417 min
Delta R.T.: 0.001 min
Response: 211599
Conc: 2.25 ug/ml

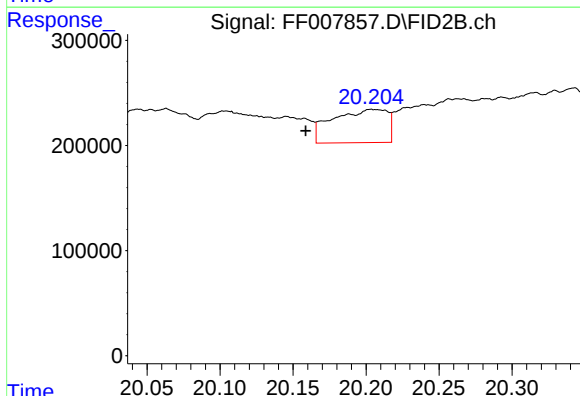

#16 N-HEXATRIACONTANE

R.T.: 20.203 min
Delta R.T.: 0.045 min
Response: 825194
Conc: 10.86 ug/ml

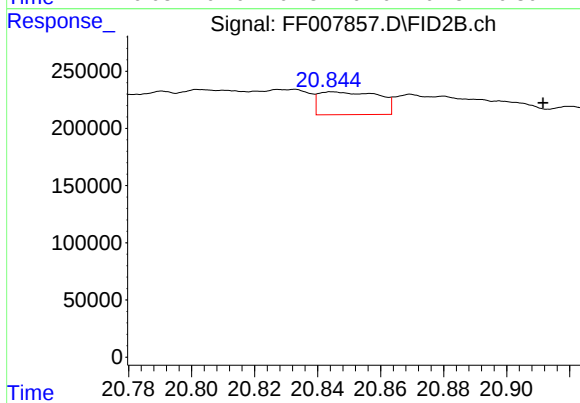

#17 N-OCTATRIACONTANE

R.T.: 20.845 min
Delta R.T.: -0.067 min
Response: 263191
Conc: 4.24 ug/ml