

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
 Data File : FF007858.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2020 16:10
 Operator : DD\AJ
 Sample : L4622-05 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 12 01:58:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	212143	1.661 ug/ml
Target Compounds			
3) N-DODECANE	6.460	84531	0.611 ug/ml
7) N-EICOSANE	12.669	164720	1.111 ug/ml
8) N-DOCOSANE	13.861	334704	2.297 ug/ml
10) N-TETRACOSANE	14.915	398228	2.754 ug/ml
12) N-OCTACOSANE	16.900	89669	0.661 ug/ml
13) N-TRIACONTANE	17.792	242641	1.875 ug/ml
14) N-DOTRIACONTANE	18.625	243938	2.104 ug/ml
15) N-TETRATRIACONTANE	19.409	202115	2.152 ug/ml
16) N-HEXATRIACONTANE	20.162	64933	0.855 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007858.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 16:10
Operator : DD\AJ
Sample : L4622-05 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 01:58:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

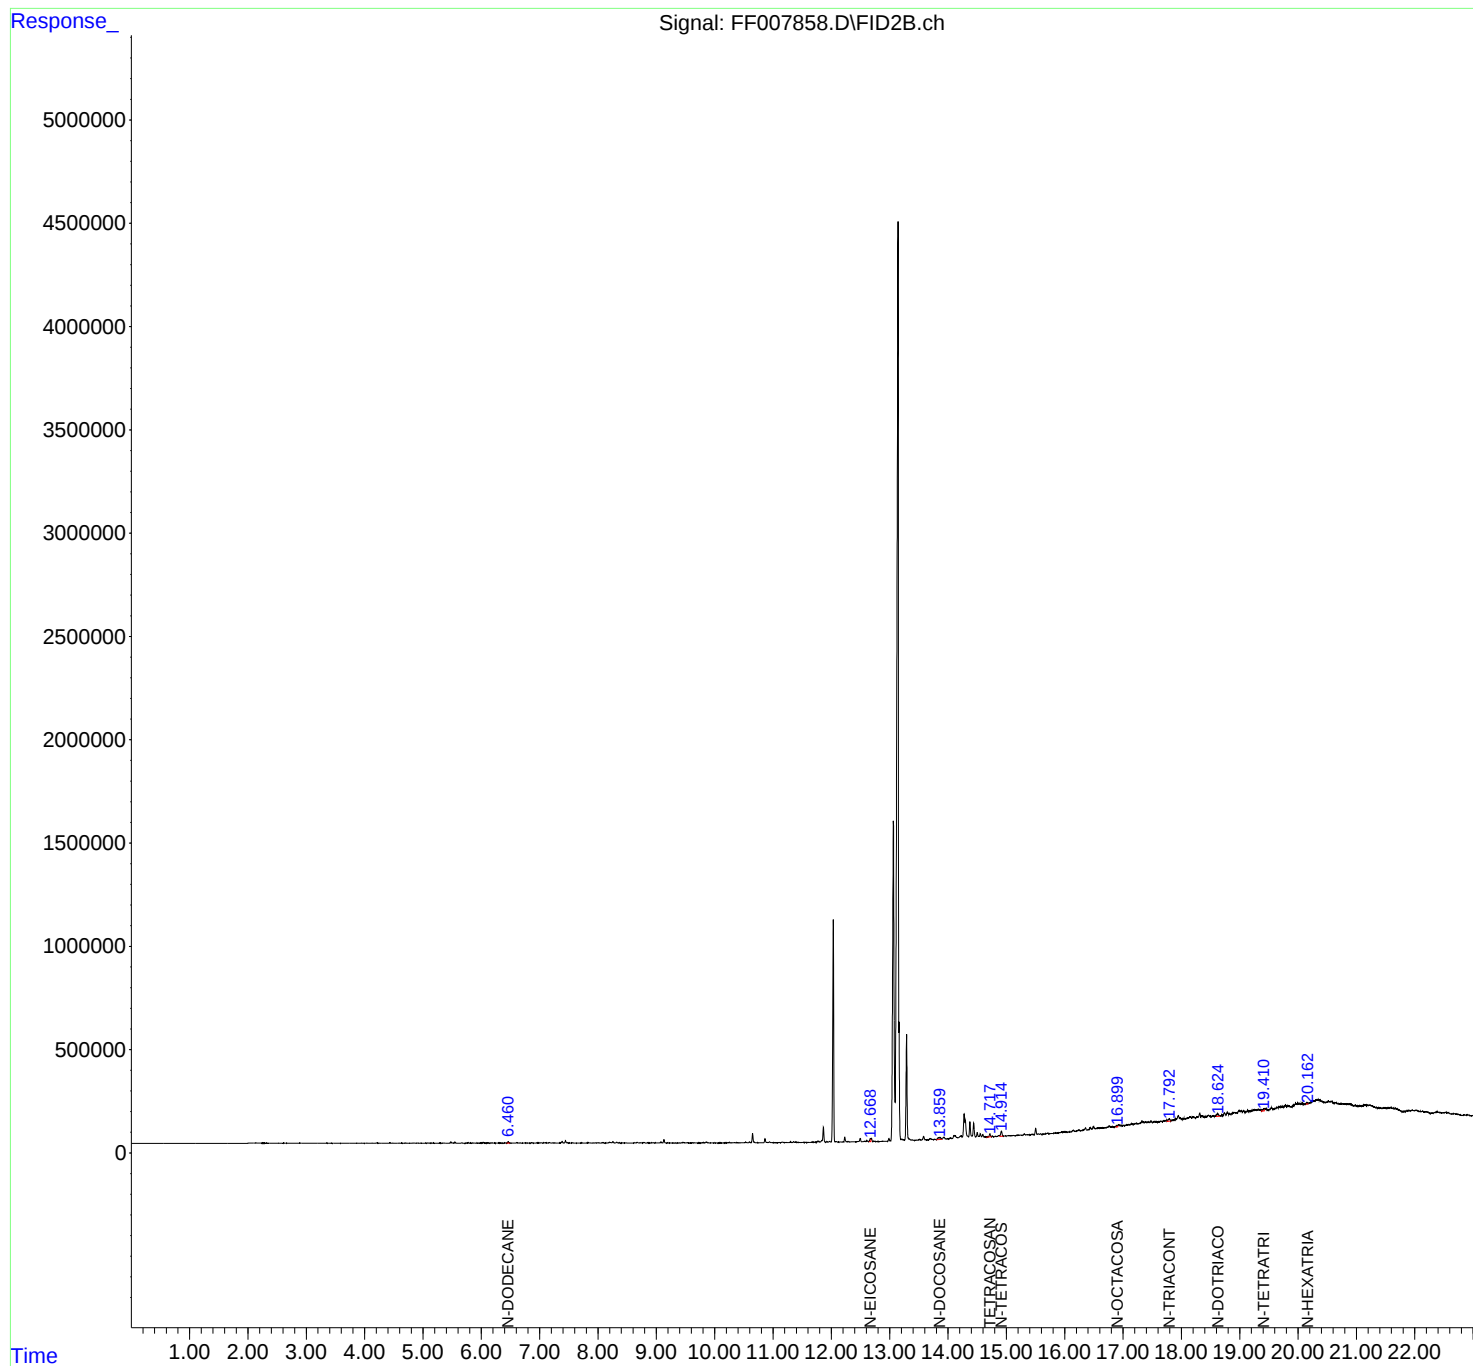


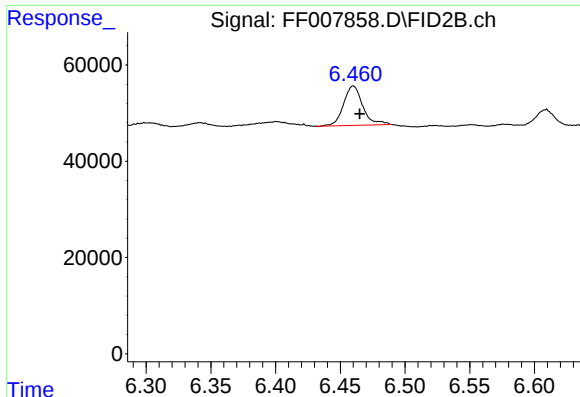

#3 N-DODECANE


R.T.: 6.460 min
Delta R.T.: -0.005 min
Response: 84531
Conc: 0.61 ug/ml

Instrument :
FID_F
ClientSampleId :

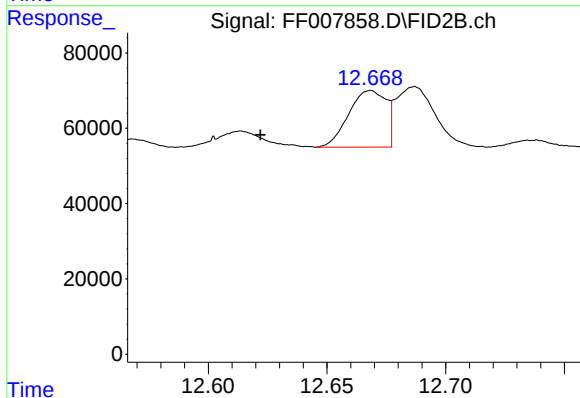


#7 N-EICOSANE

R.T.: 12.669 min
Delta R.T.: 0.047 min
Response: 164720
Conc: 1.11 ug/ml

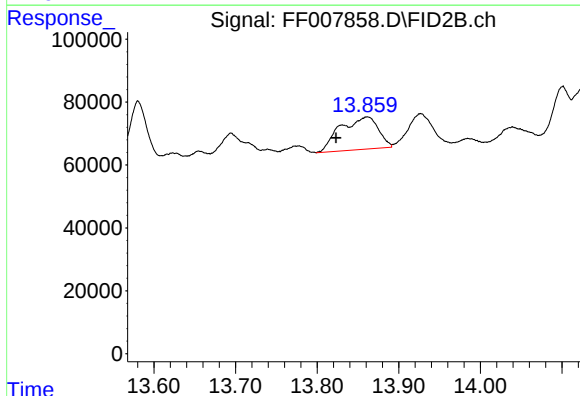


#8 N-DOCOSANE

R.T.: 13.861 min
Delta R.T.: 0.038 min
Response: 334704
Conc: 2.30 ug/ml

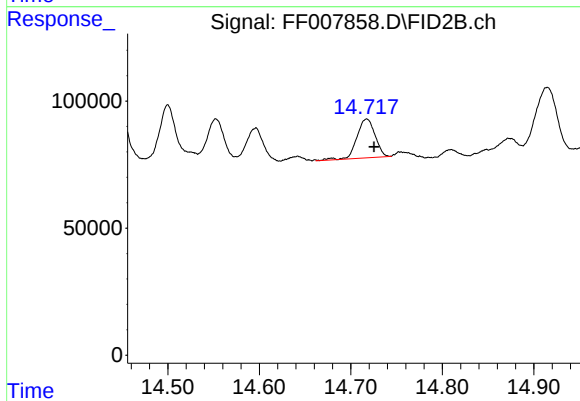

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.717 min
Delta R.T.: -0.008 min
Response: 212143
Conc: 1.66 ug/ml

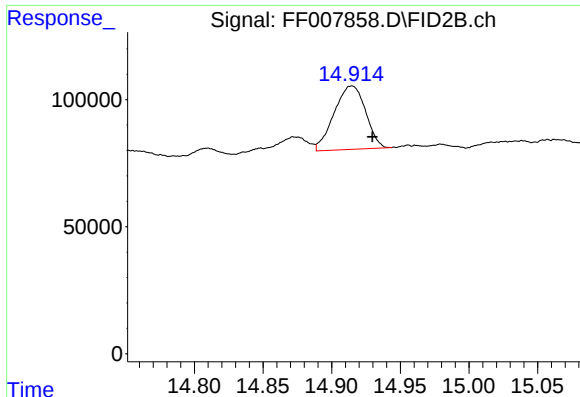

#10 N-TETRACOSANE


R.T.: 14.915 min
Delta R.T.: -0.015 min
Response: 398228
Conc: 2.75 ug/ml

Instrument :
FID_F
ClientSampleId :

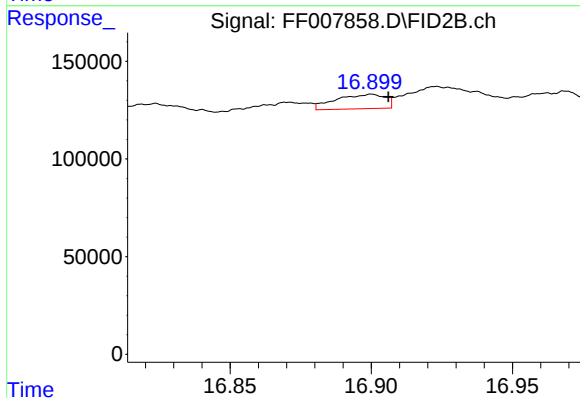


#12 N-OCTACOSANE

R.T.: 16.900 min
Delta R.T.: -0.006 min
Response: 89669
Conc: 0.66 ug/ml

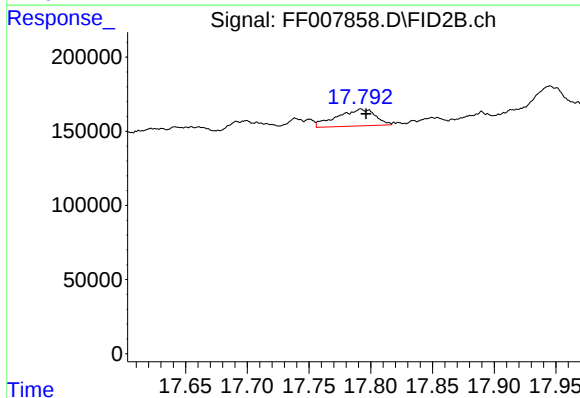


#13 N-TRIACONTANE

R.T.: 17.792 min
Delta R.T.: -0.004 min
Response: 242641
Conc: 1.88 ug/ml

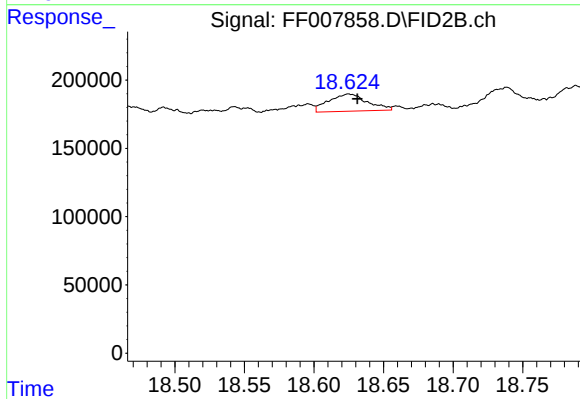

#14 N-DOTRIACONTANE


R.T.: 18.625 min
Delta R.T.: -0.006 min
Response: 243938
Conc: 2.10 ug/ml

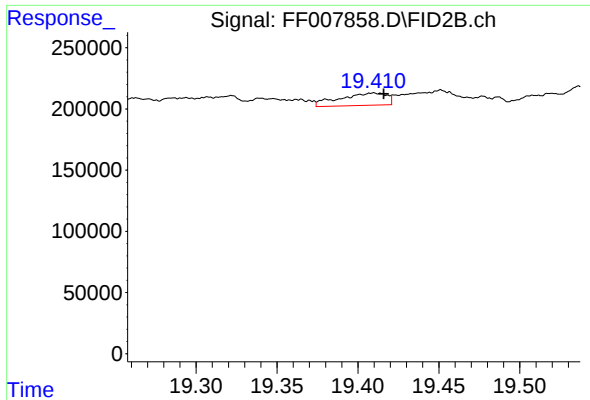

#15 N-TETRATRIACONTANE

R.T.: 19.409 min
Delta R.T.: -0.007 min
Response: 202115
Conc: 2.15 ug/ml

Instrument :
FID_F
ClientSampleId :

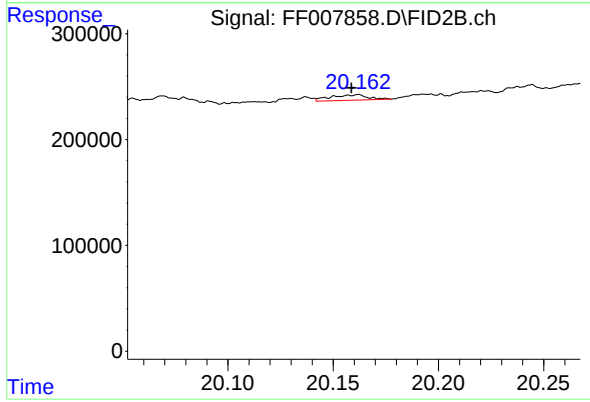

#16 N-HEXATRIACONTANE

R.T.: 20.162 min
Delta R.T.: 0.003 min
Response: 64933
Conc: 0.85 ug/ml