

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
 Data File : FF007859.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2020 16:41
 Operator : DD\AJ
 Sample : L4631-03 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 12 01:59:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	192553	1.507 ug/ml
Target Compounds			
7) N-EICOSANE	12.687f	153570	1.036 ug/ml
13) N-TRIACONTANE	17.791	117384	0.907 ug/ml
14) N-DOTRIACONTANE	18.624	129144	1.114 ug/ml
16) N-HEXATRIACONTANE	20.119	51334	0.676 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007859.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 16:41
Operator : DD\AJ
Sample : L4631-03 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 01:59:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

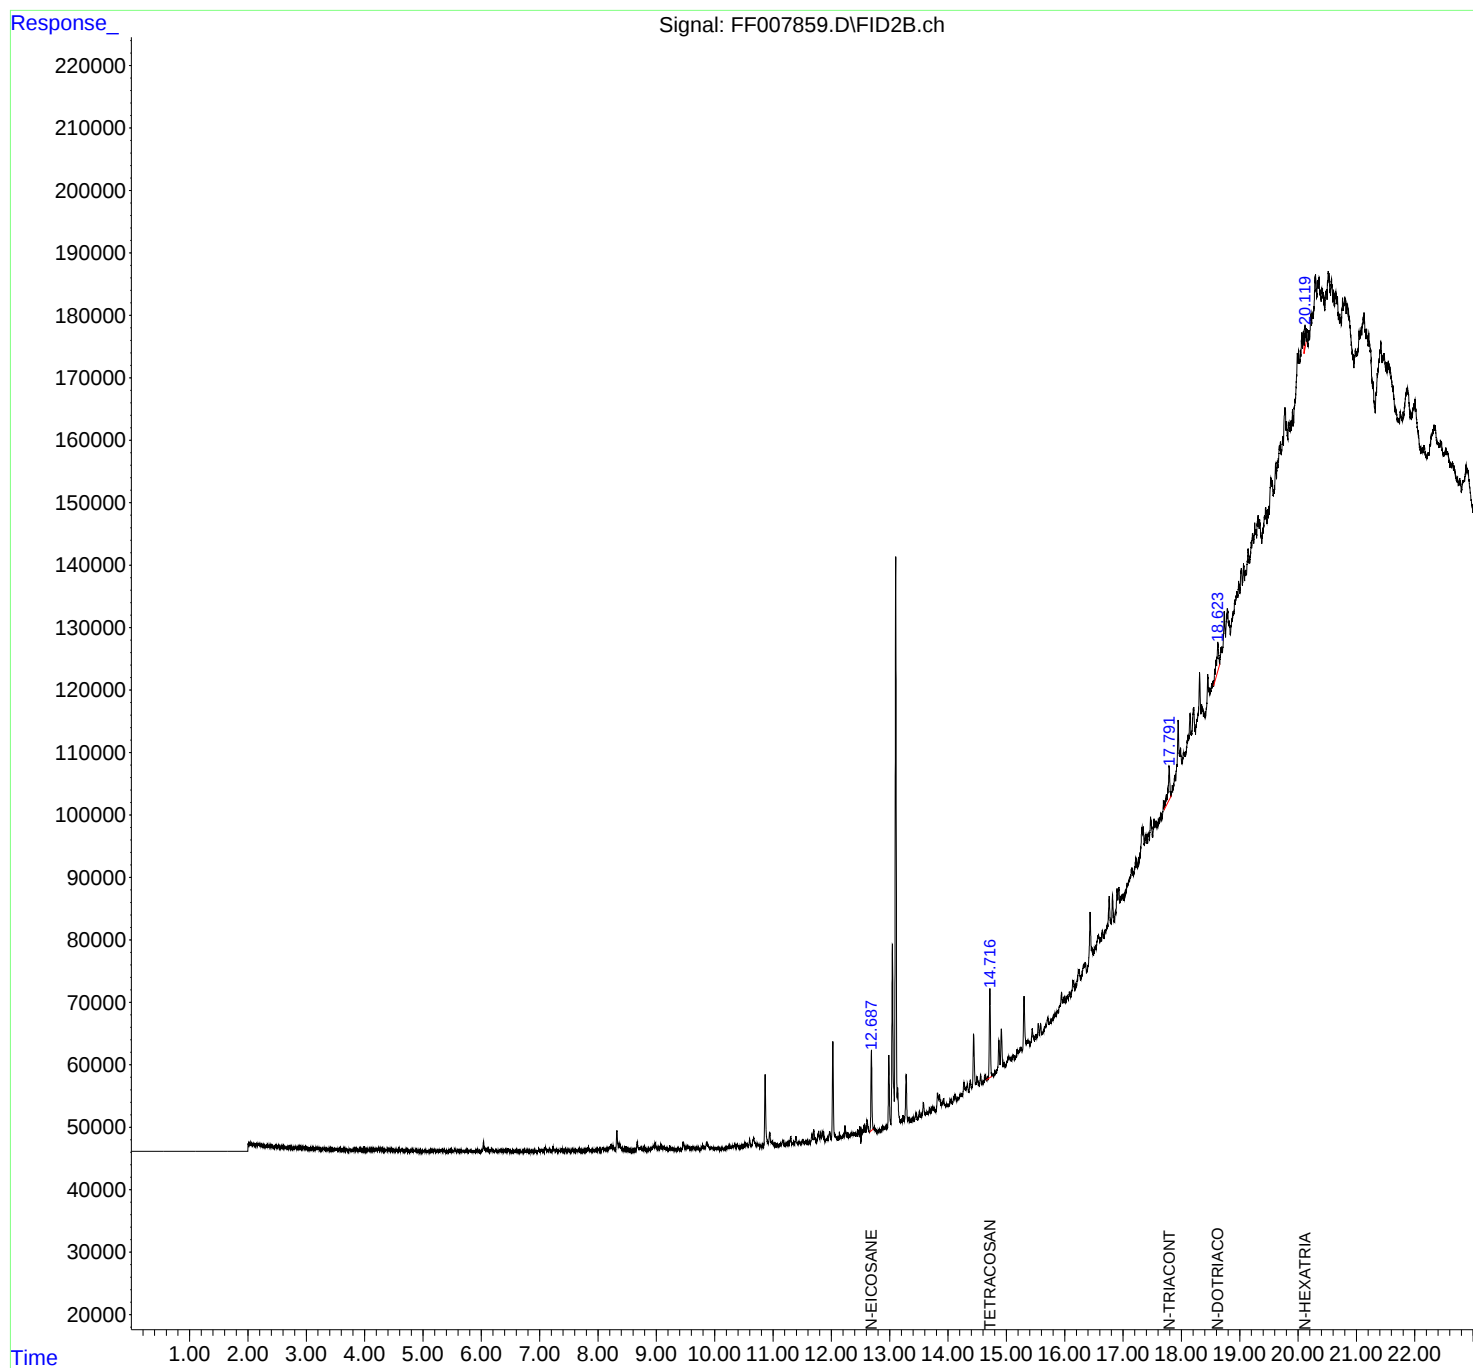


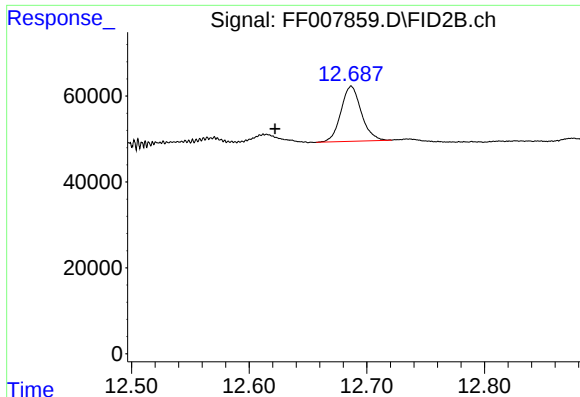

#7 N-EICOSANE


R.T.: 12.687 min
Delta R.T.: 0.065 min
Response: 153570
Conc: 1.04 ug/ml

Instrument :
FID_F
ClientSampleId :

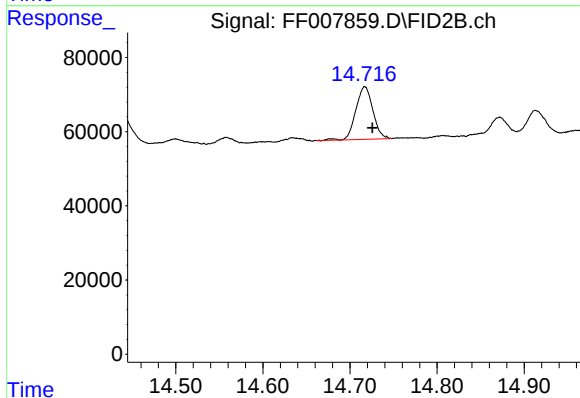


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.717 min
Delta R.T.: -0.009 min
Response: 192553
Conc: 1.51 ug/ml

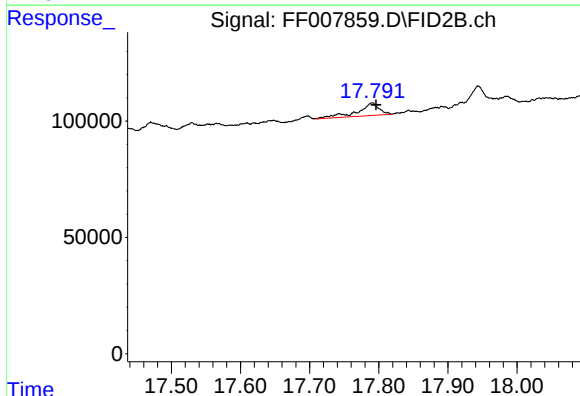


#13 N-TRIACONTANE

R.T.: 17.791 min
Delta R.T.: -0.005 min
Response: 117384
Conc: 0.91 ug/ml

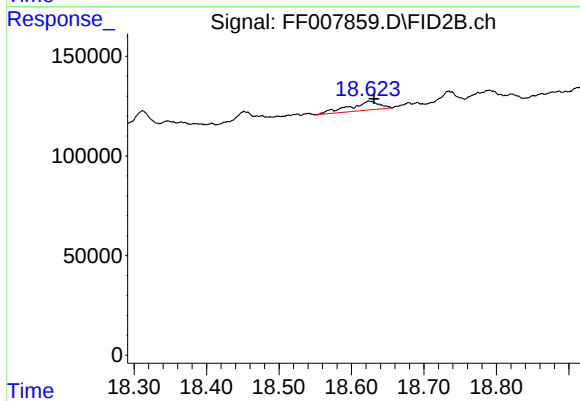

#14 N-DOTRIACONTANE

R.T.: 18.624 min
Delta R.T.: -0.007 min
Response: 129144
Conc: 1.11 ug/ml

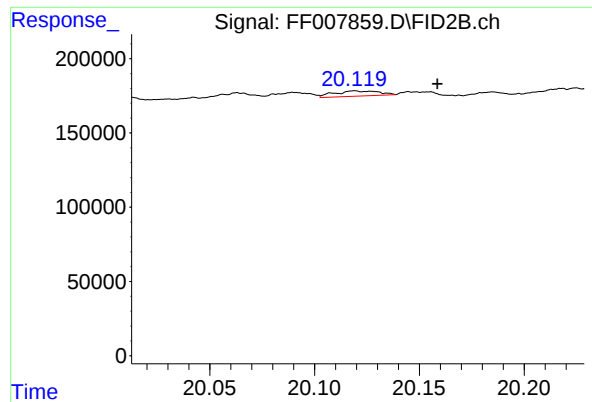

#16 N-HEXATRIACONTANE

R.T.: 20.119 min
Delta R.T.: -0.040 min
Response: 51334
Conc: 0.68 ug/ml

Instrument :
FID_F
ClientSampleId :