

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
 Data File : FF007860.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2020 17:13
 Operator : DD\AJ
 Sample : L4631-05 5X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 12 01:59:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	408702	3.200 ug/ml
Target Compounds			
4) N-TETRADECANE	8.322f	86791	0.615 ug/ml
13) N-TRIACONTANE	17.791	175919	1.360 ug/ml
14) N-DOTRIACONTANE	18.620	139021	1.199 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007860.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 17:13
Operator : DD\AJ
Sample : L4631-05 5X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 01:59:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

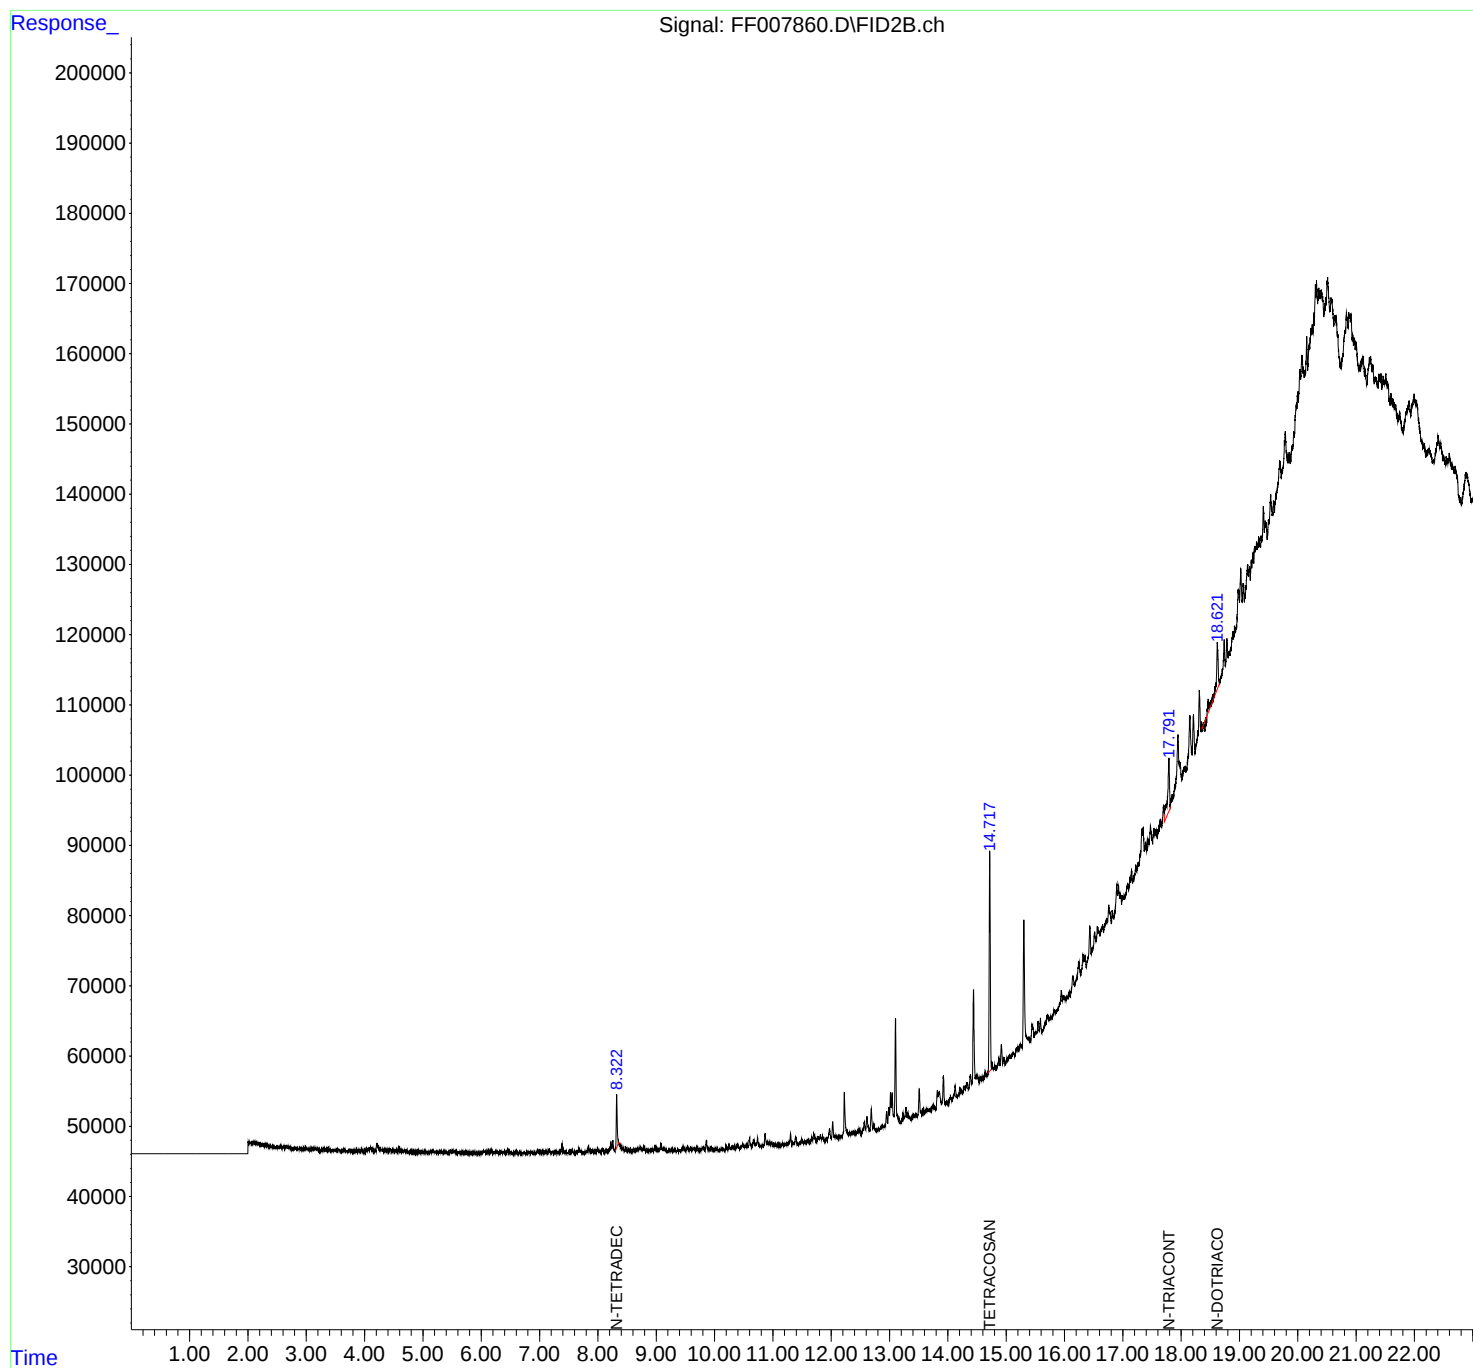


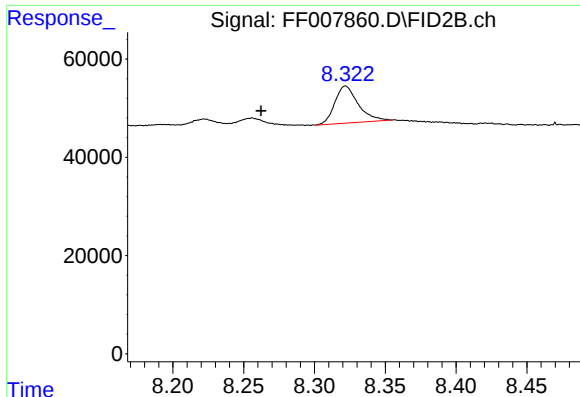

#4 N-TETRADECANE


R.T.: 8.322 min
Delta R.T.: 0.060 min
Response: 86791
Conc: 0.61 ug/ml

Instrument :
FID_F
ClientSampleId :

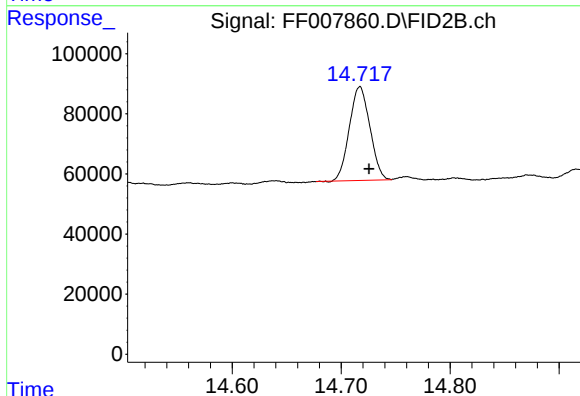


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.717 min
Delta R.T.: -0.008 min
Response: 408702
Conc: 3.20 ug/ml

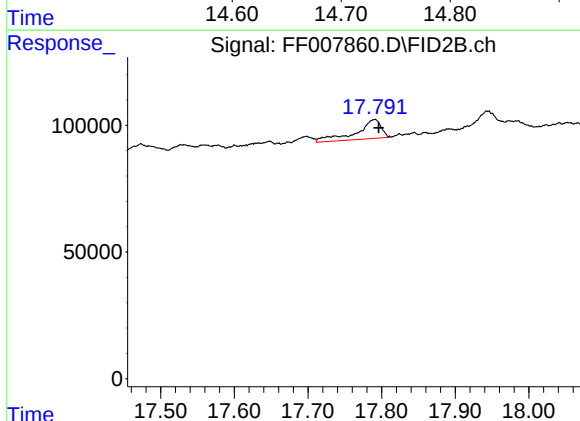

#13 N-TRIACONTANE

R.T.: 17.791 min
Delta R.T.: -0.005 min
Response: 175919
Conc: 1.36 ug/ml

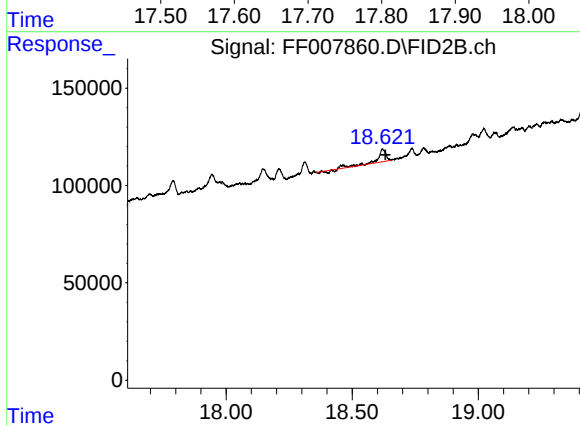

#14 N-DOTRIACONTANE

R.T.: 18.620 min
Delta R.T.: -0.011 min
Response: 139021
Conc: 1.20 ug/ml