

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
 Data File : FF007863.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2020 18:46
 Operator : DD\AJ
 Sample : L4680-01 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 12 01:59:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	312013	2.443 ug/ml
Target Compounds			
4) N-TETRADECANE	8.322f	200858	1.422 ug/ml
7) N-EICOSANE	12.685f	317655	2.143 ug/ml
10) N-TETRACOSANE	14.913	206571	1.428 ug/ml
13) N-TRIACONTANE	17.787	109613	0.847 ug/ml
14) N-DOTRIACONTANE	18.618	131960	1.138 ug/ml
16) N-HEXATRIACONTANE	20.152	64625	0.851 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007863.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 18:46
Operator : DD\AJ
Sample : L4680-01 5X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 01:59:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

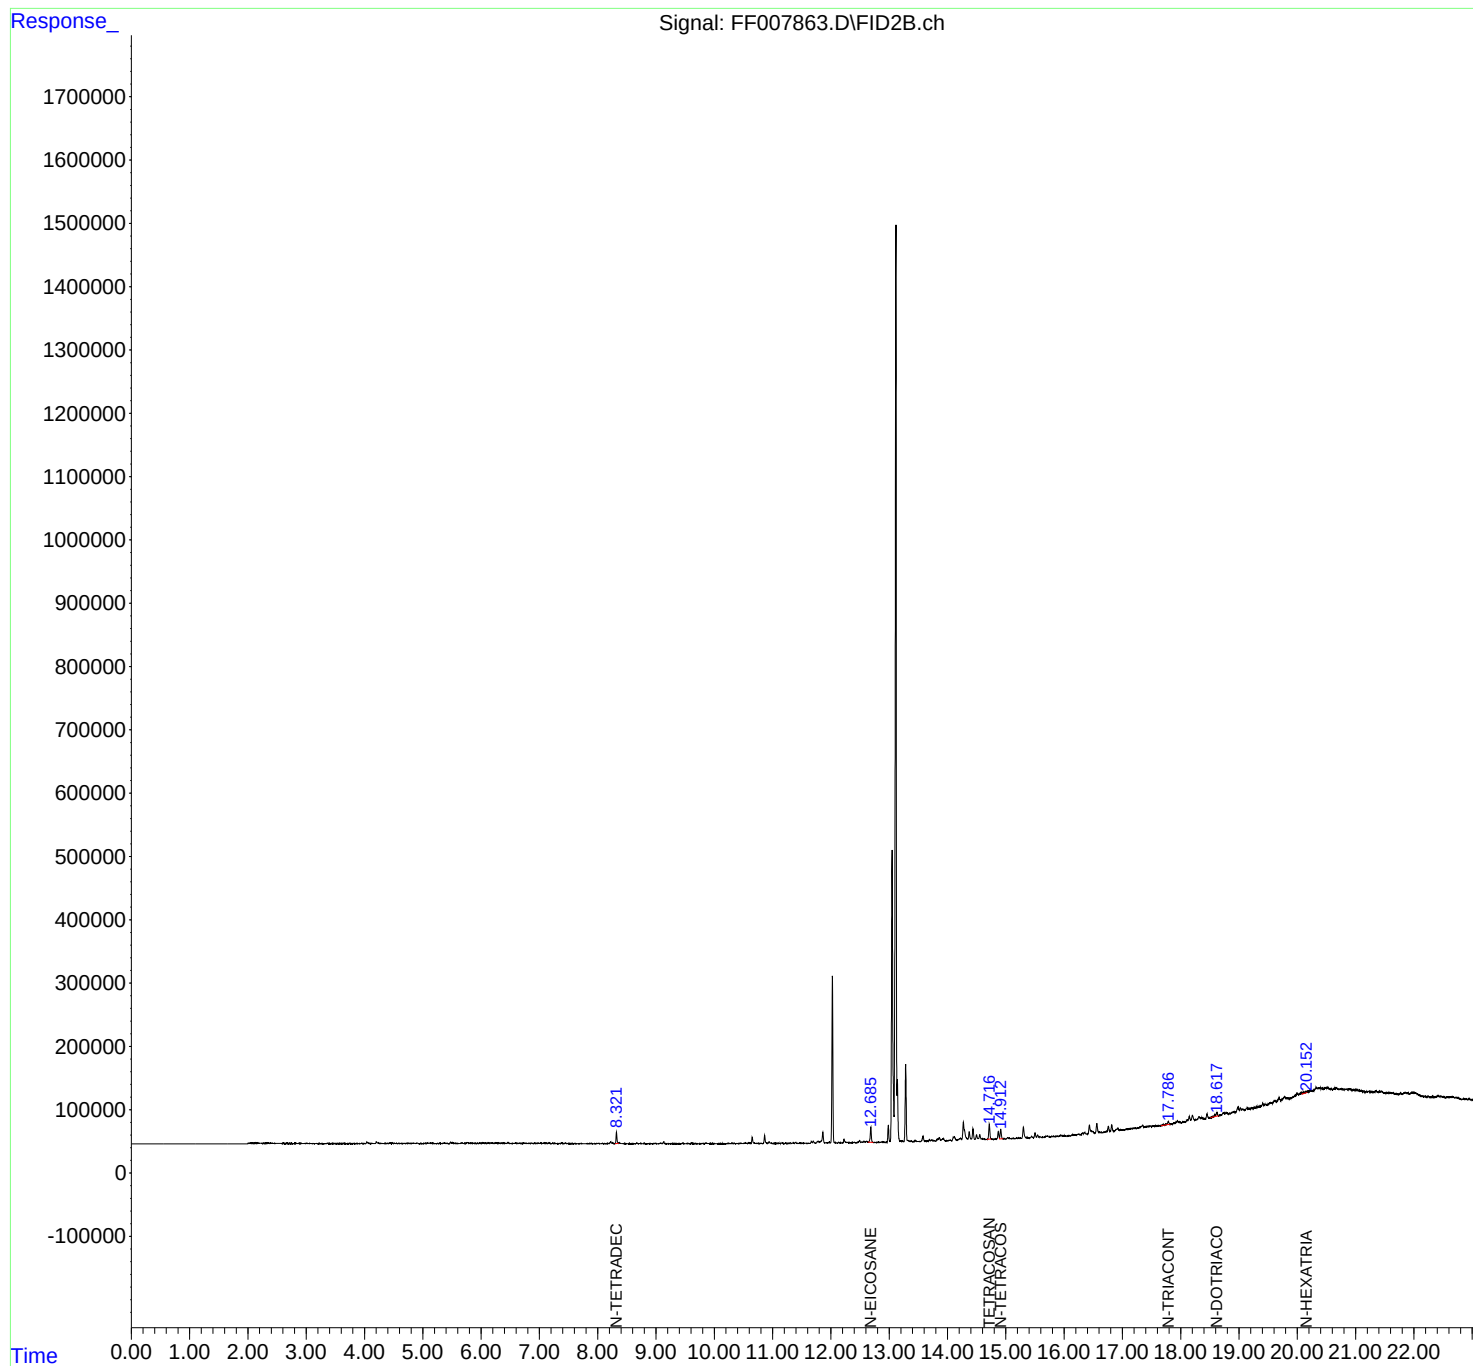


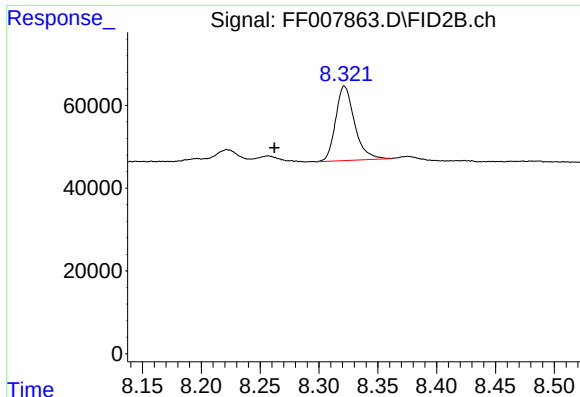

#4 N-TETRADECANE


R.T.: 8.322 min
Delta R.T.: 0.059 min
Response: 200858
Conc: 1.42 ug/ml

Instrument :
FID_F
ClientSampleId :

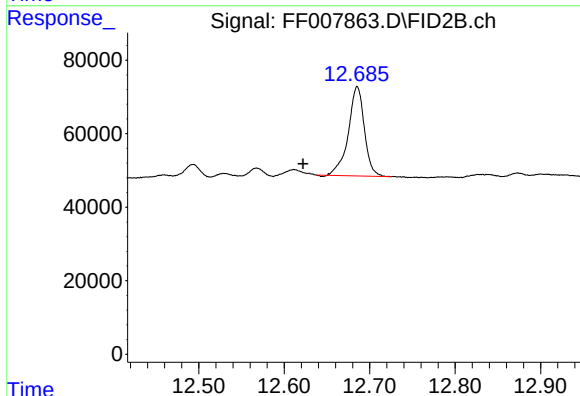


#7 N-EICOSANE

R.T.: 12.685 min
Delta R.T.: 0.063 min
Response: 317655
Conc: 2.14 ug/ml

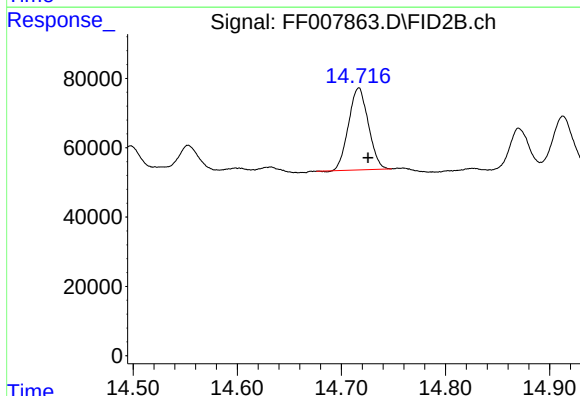


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.717 min
Delta R.T.: -0.009 min
Response: 312013
Conc: 2.44 ug/ml

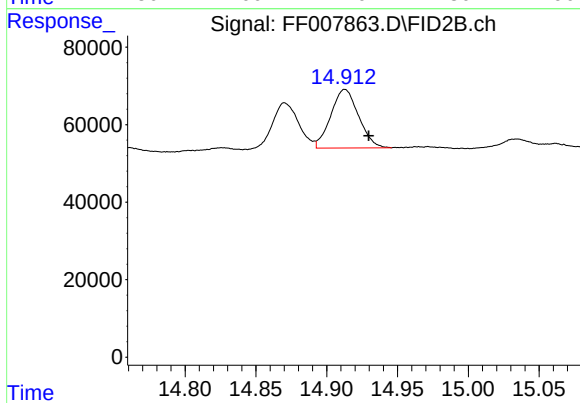

#10 N-TETRACOSANE


R.T.: 14.913 min
Delta R.T.: -0.017 min
Response: 206571
Conc: 1.43 ug/ml

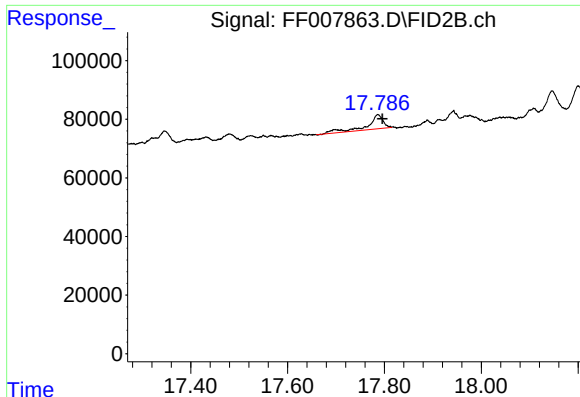

#13 N-TRIACONTANE


R.T.: 17.787 min
Delta R.T.: -0.010 min
Response: 109613
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

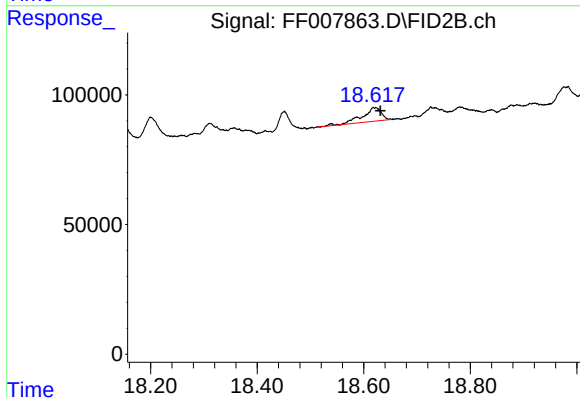

#14 N-DOTRIACONTANE

R.T.: 18.618 min
Delta R.T.: -0.013 min
Response: 131960
Conc: 1.14 ug/ml

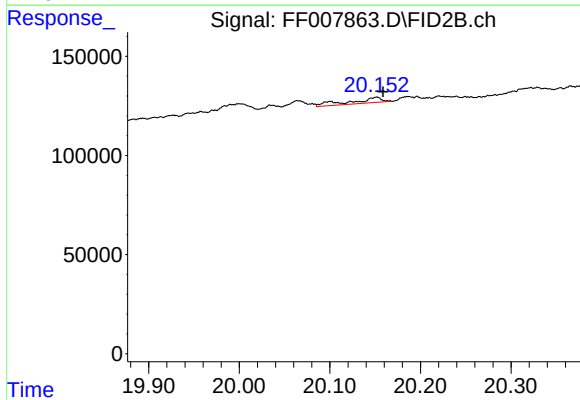

#16 N-HEXATRIACONTANE

R.T.: 20.152 min
Delta R.T.: -0.007 min
Response: 64625
Conc: 0.85 ug/ml