

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF111120\  
 Data File : FF007866.D  
 Signal(s) : FID2B.ch  
 Acq On : 11 Nov 2020 20:20  
 Operator : DD\AJ  
 Sample : L4631-03 5X  
 Misc :  
 ALS Vial : 69 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Nov 12 02:00:32 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF110220.M  
 Quant Title :  
 QLast Update : Tue Nov 03 01:29:25 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units  |
|-------------------------------|---------|----------|-------------|
| -----                         |         |          |             |
| System Monitoring Compounds   |         |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 14.717  | 370285   | 2.899 ug/ml |
| Target Compounds              |         |          |             |
| 7) N-EICOSANE                 | 12.686f | 287054   | 1.937 ug/ml |
| 10) N-TETRACOSANE             | 14.913  | 160067   | 1.107 ug/ml |
| 12) N-OCTACOSANE              | 16.897  | 85183    | 0.628 ug/ml |
| 13) N-TRIACONTANE             | 17.790  | 228412   | 1.765 ug/ml |
| 14) N-DOTRIACONTANE           | 18.621  | 197738   | 1.706 ug/ml |
| 15) N-TETRATRIACONTANE        | 19.402  | 41665    | 0.444 ug/ml |
| -----                         |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF111120\  
Data File : FF007866.D  
Signal(s) : FID2B.ch  
Acq On : 11 Nov 2020 20:20  
Operator : DD\AJ  
Sample : L4631-03 5X  
Misc :  
ALS Vial : 69 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Nov 12 02:00:32 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF110220.M  
Quant Title :  
QLast Update : Tue Nov 03 01:29:25 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

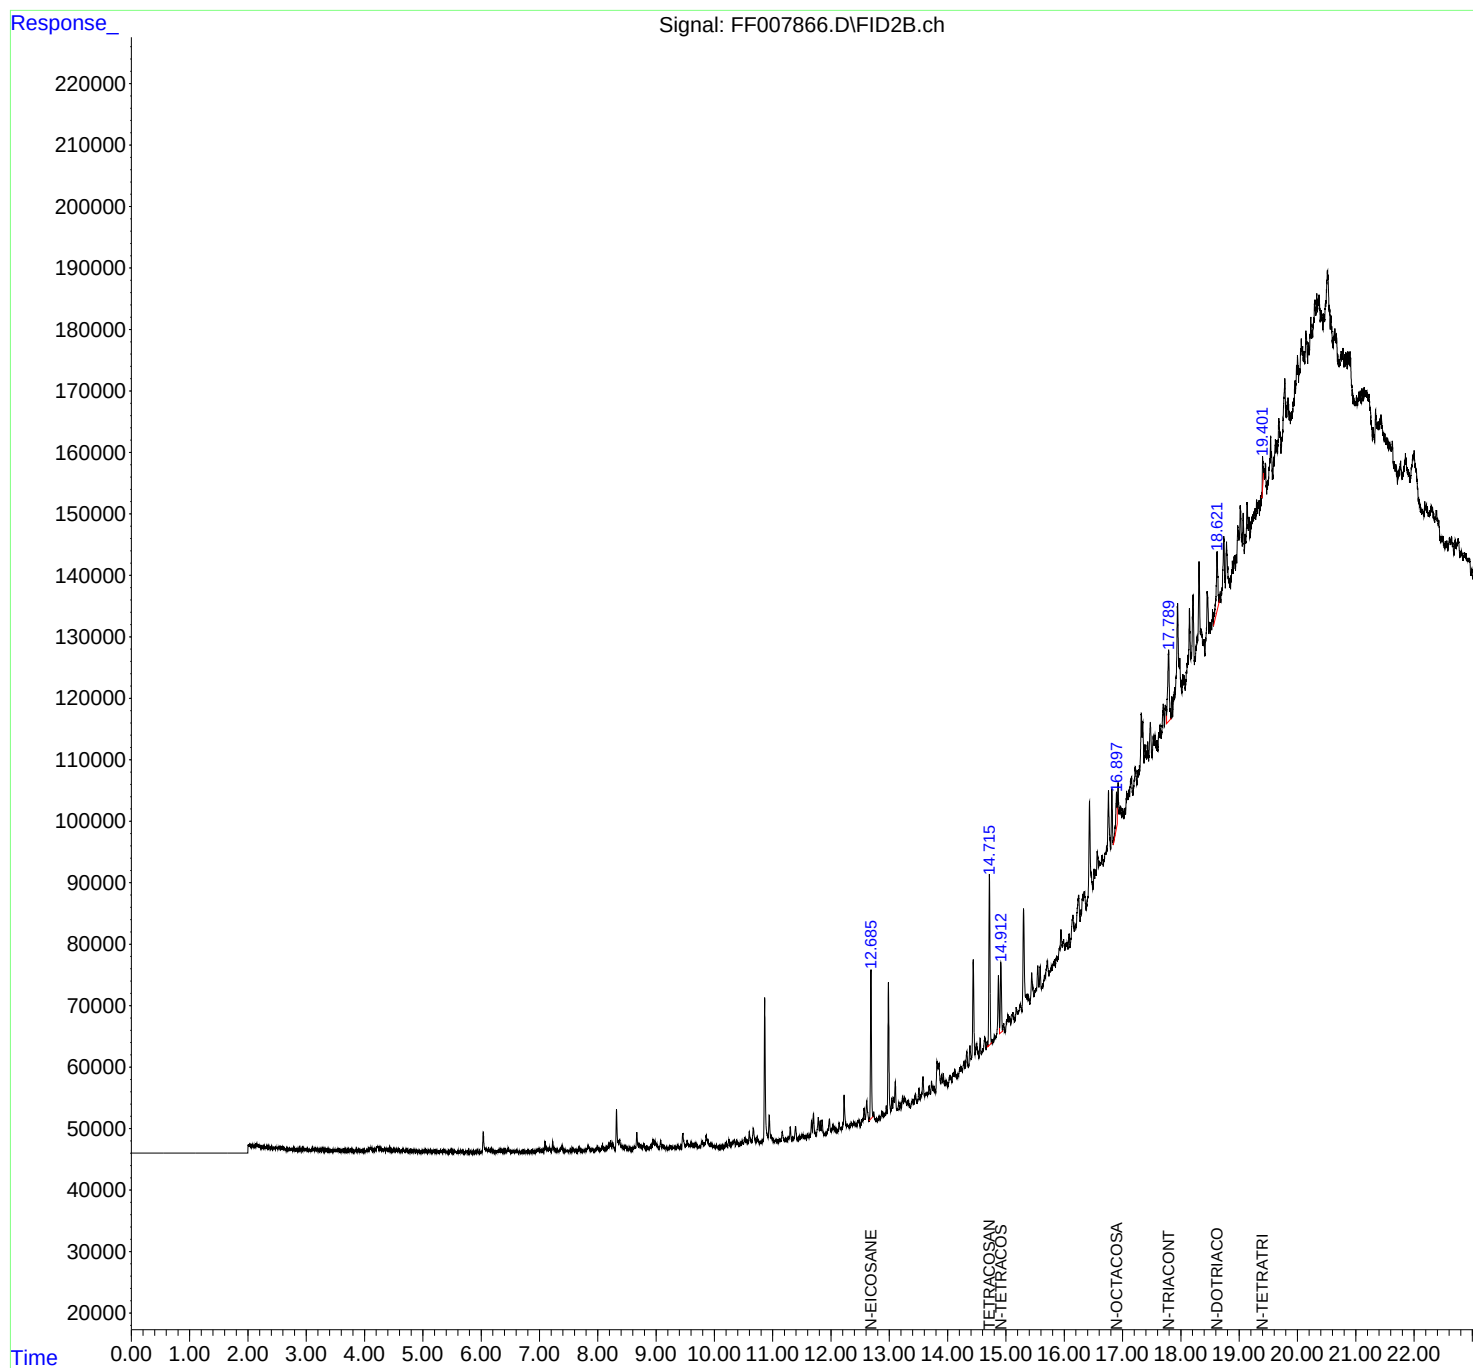


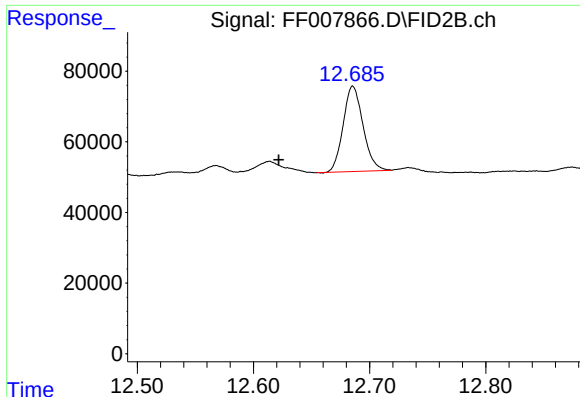

#7 N-EICOSANE


R.T.: 12.686 min  
Delta R.T.: 0.064 min  
Response: 287054  
Conc: 1.94 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

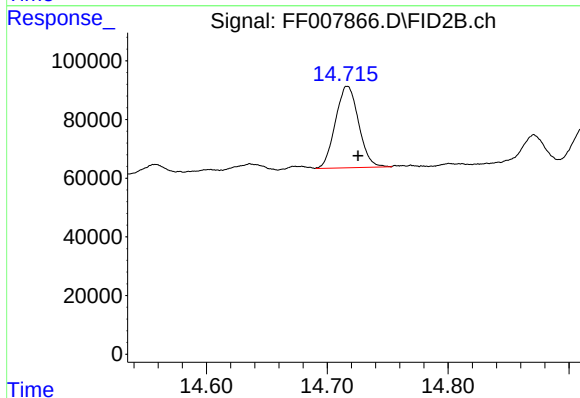


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.717 min  
Delta R.T.: -0.009 min  
Response: 370285  
Conc: 2.90 ug/ml

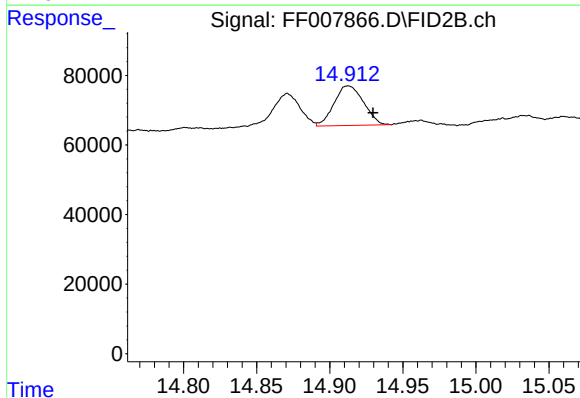


#10 N-TETRACOSANE

R.T.: 14.913 min  
Delta R.T.: -0.017 min  
Response: 160067  
Conc: 1.11 ug/ml

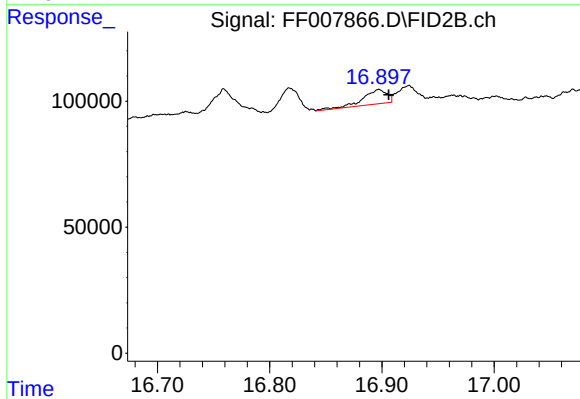

#12 N-OCTACOSANE


R.T.: 16.897 min  
Delta R.T.: -0.009 min  
Response: 85183  
Conc: 0.63 ug/ml

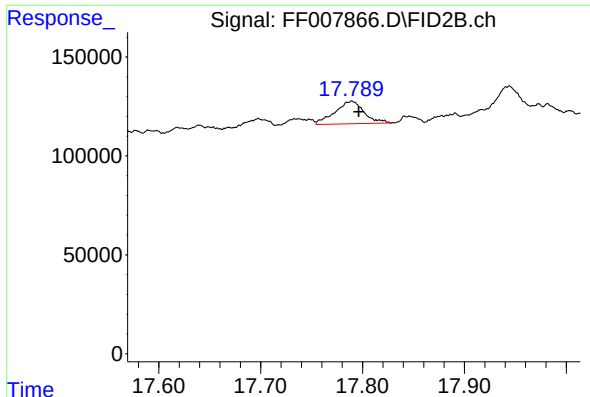

#13 N-TRIACONTANE


R.T.: 17.790 min  
Delta R.T.: -0.007 min  
Response: 228412  
Conc: 1.77 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

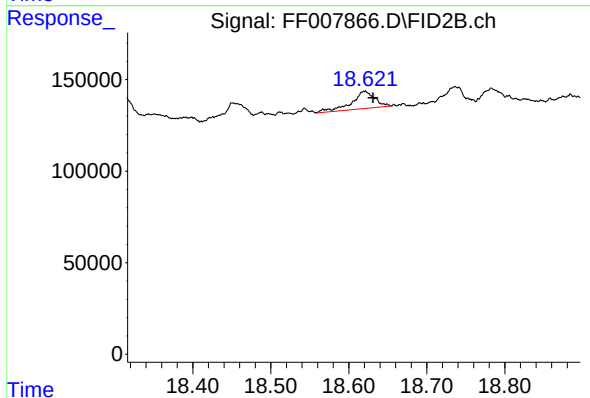

#14 N-DOTRIACONTANE

R.T.: 18.621 min  
Delta R.T.: -0.010 min  
Response: 197738  
Conc: 1.71 ug/ml

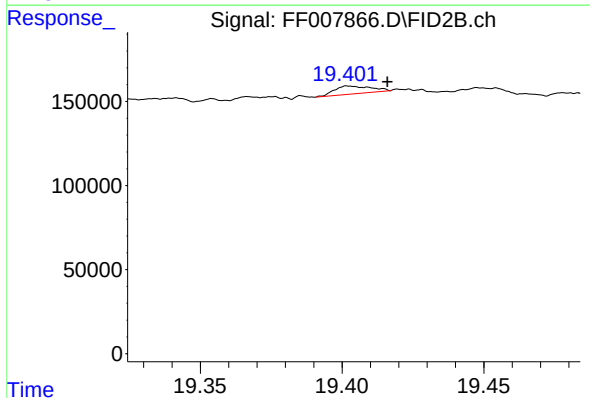

#15 N-TETRATRIACONTANE

R.T.: 19.402 min  
Delta R.T.: -0.014 min  
Response: 41665  
Conc: 0.44 ug/ml