

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007851.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 12:09
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 12 01:57:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.459	10069058	72.744 ug/ml
12) N-OCTACOSANE	16.899	9087824	67.002 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007851.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 12:09
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 12 01:57:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

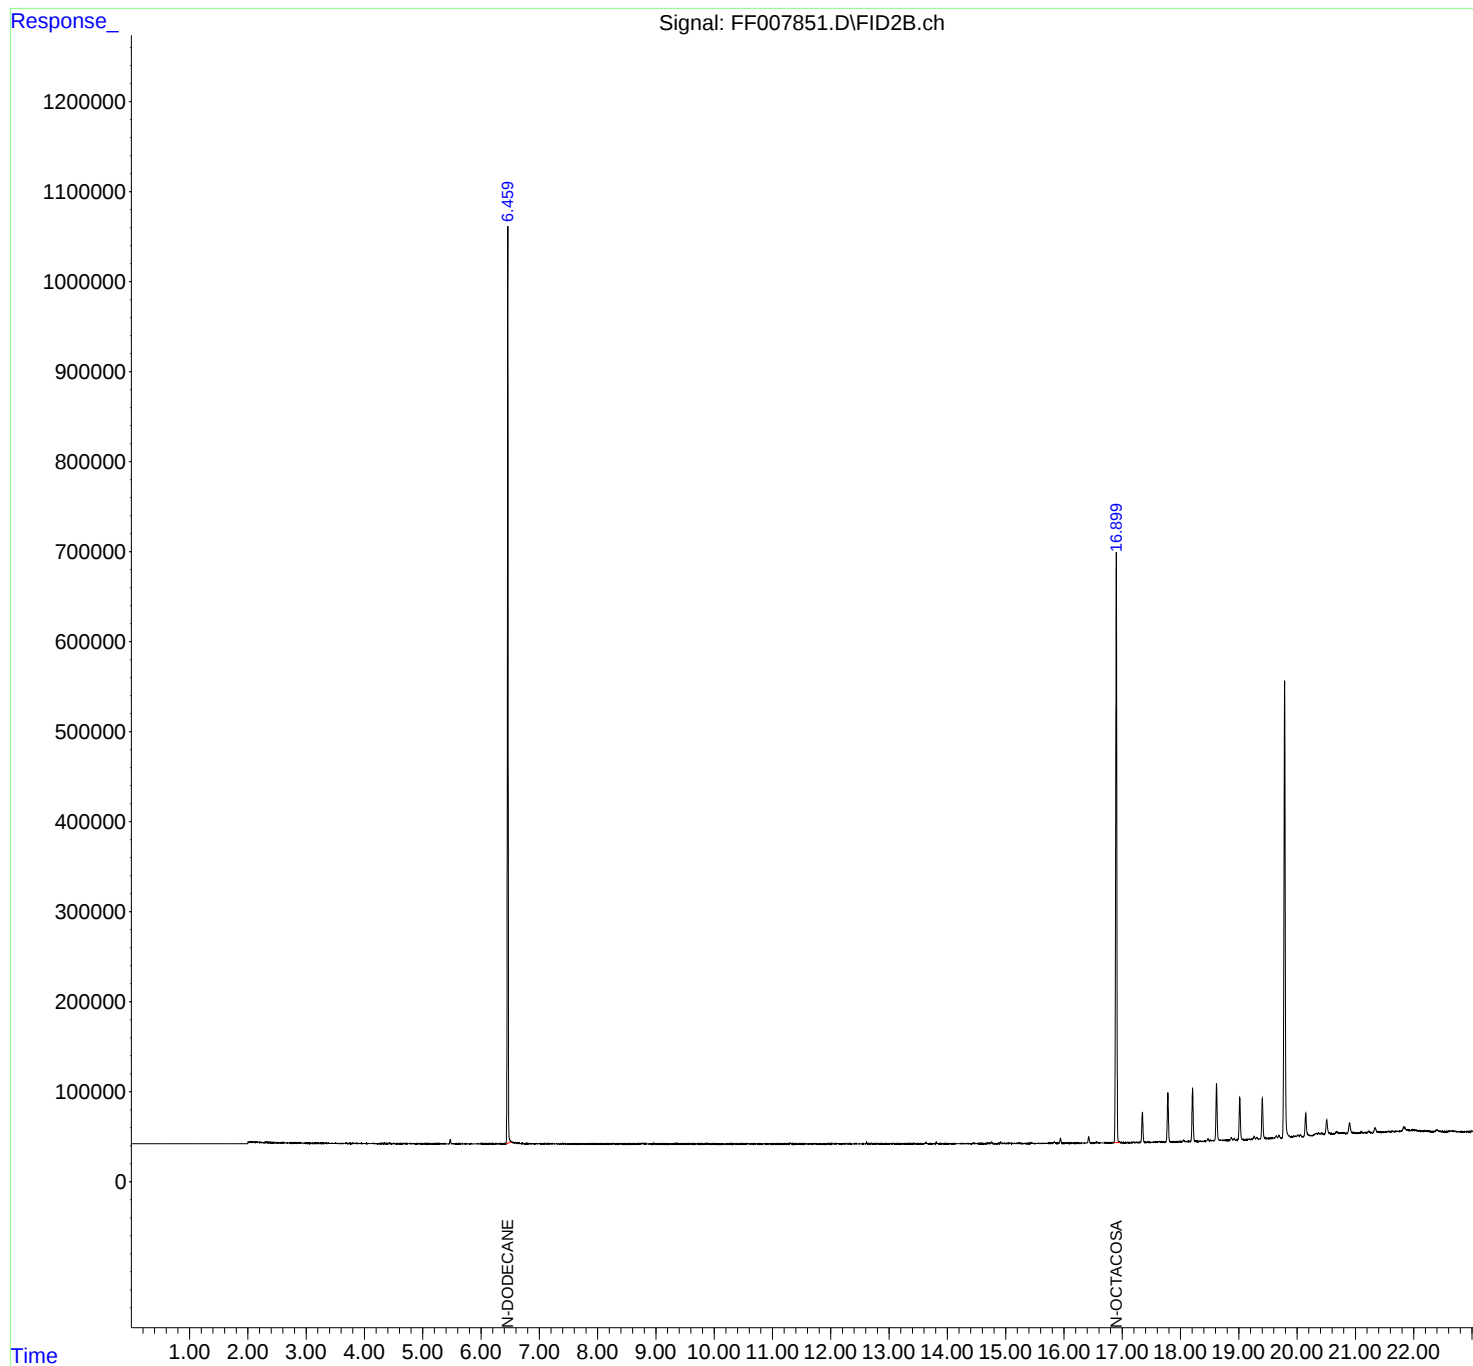


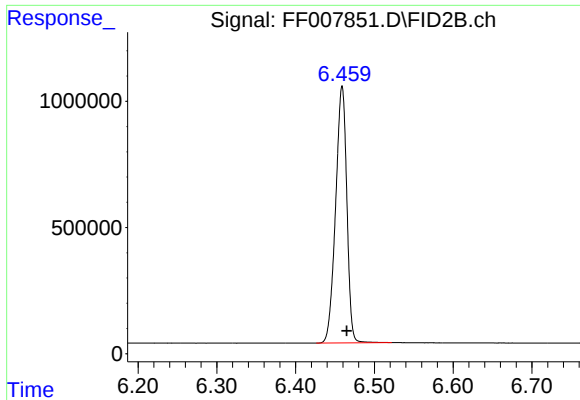

#3 N-DODECANE


R.T.: 6.459 min
Delta R.T.: -0.006 min
Response: 10069058
Conc: 72.74 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

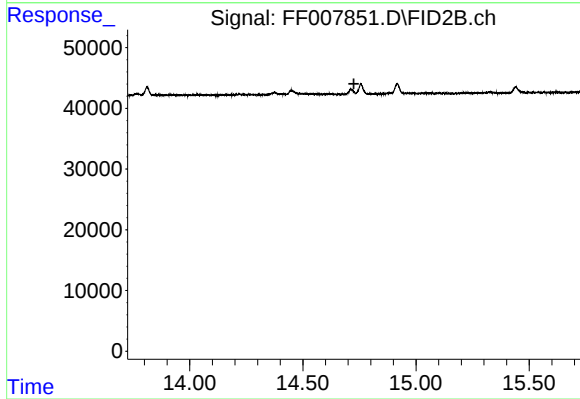

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.726 min
Response: 0
Conc: N.D.

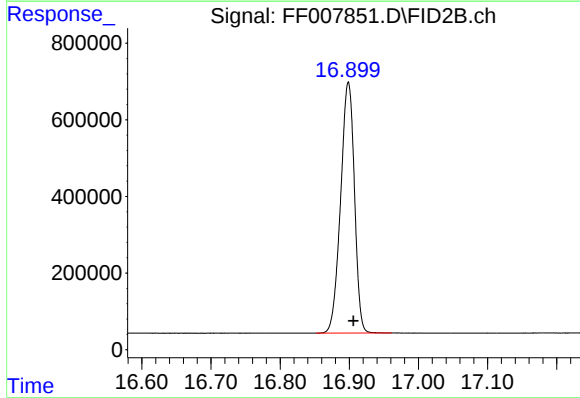

#12 N-OCTACOSANE

R.T.: 16.899 min
Delta R.T.: -0.007 min
Response: 9087824
Conc: 67.00 ug/ml