

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
 Data File : FF007853.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2020 13:34
 Operator : DD\AJ
 Sample : PB132940BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB132940BS

Integration File: autoint1.e
 Quant Time: Nov 12 01:57:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.713	2929953	22.938 ug/ml
Target Compounds			
2) N-DECANE	4.434	3223514	23.693 ug/ml
3) N-DODECANE	6.459	3346419	24.176 ug/ml
4) N-TETRADECANE	8.254	3426056	24.261 ug/ml
5) N-HEXADECANE	9.856	3437827	23.654 ug/ml
6) N-OCTADECANE	11.300	3451303	23.256 ug/ml
7) N-EICOSANE	12.613	3452747	23.294 ug/ml
8) N-DOCOSANE	13.813	3365425	23.100 ug/ml
10) N-TETRACOSANE	14.918	3224611	22.298 ug/ml
11) N-HEXACOSANE	15.942	3074952	21.909 ug/ml
12) N-OCTACOSANE	16.893	2936976	21.654 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007853.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 13:34
Operator : DD\AJ
Sample : PB132940BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
PB132940BS

Integration File: autoint1.e
Quant Time: Nov 12 01:57:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

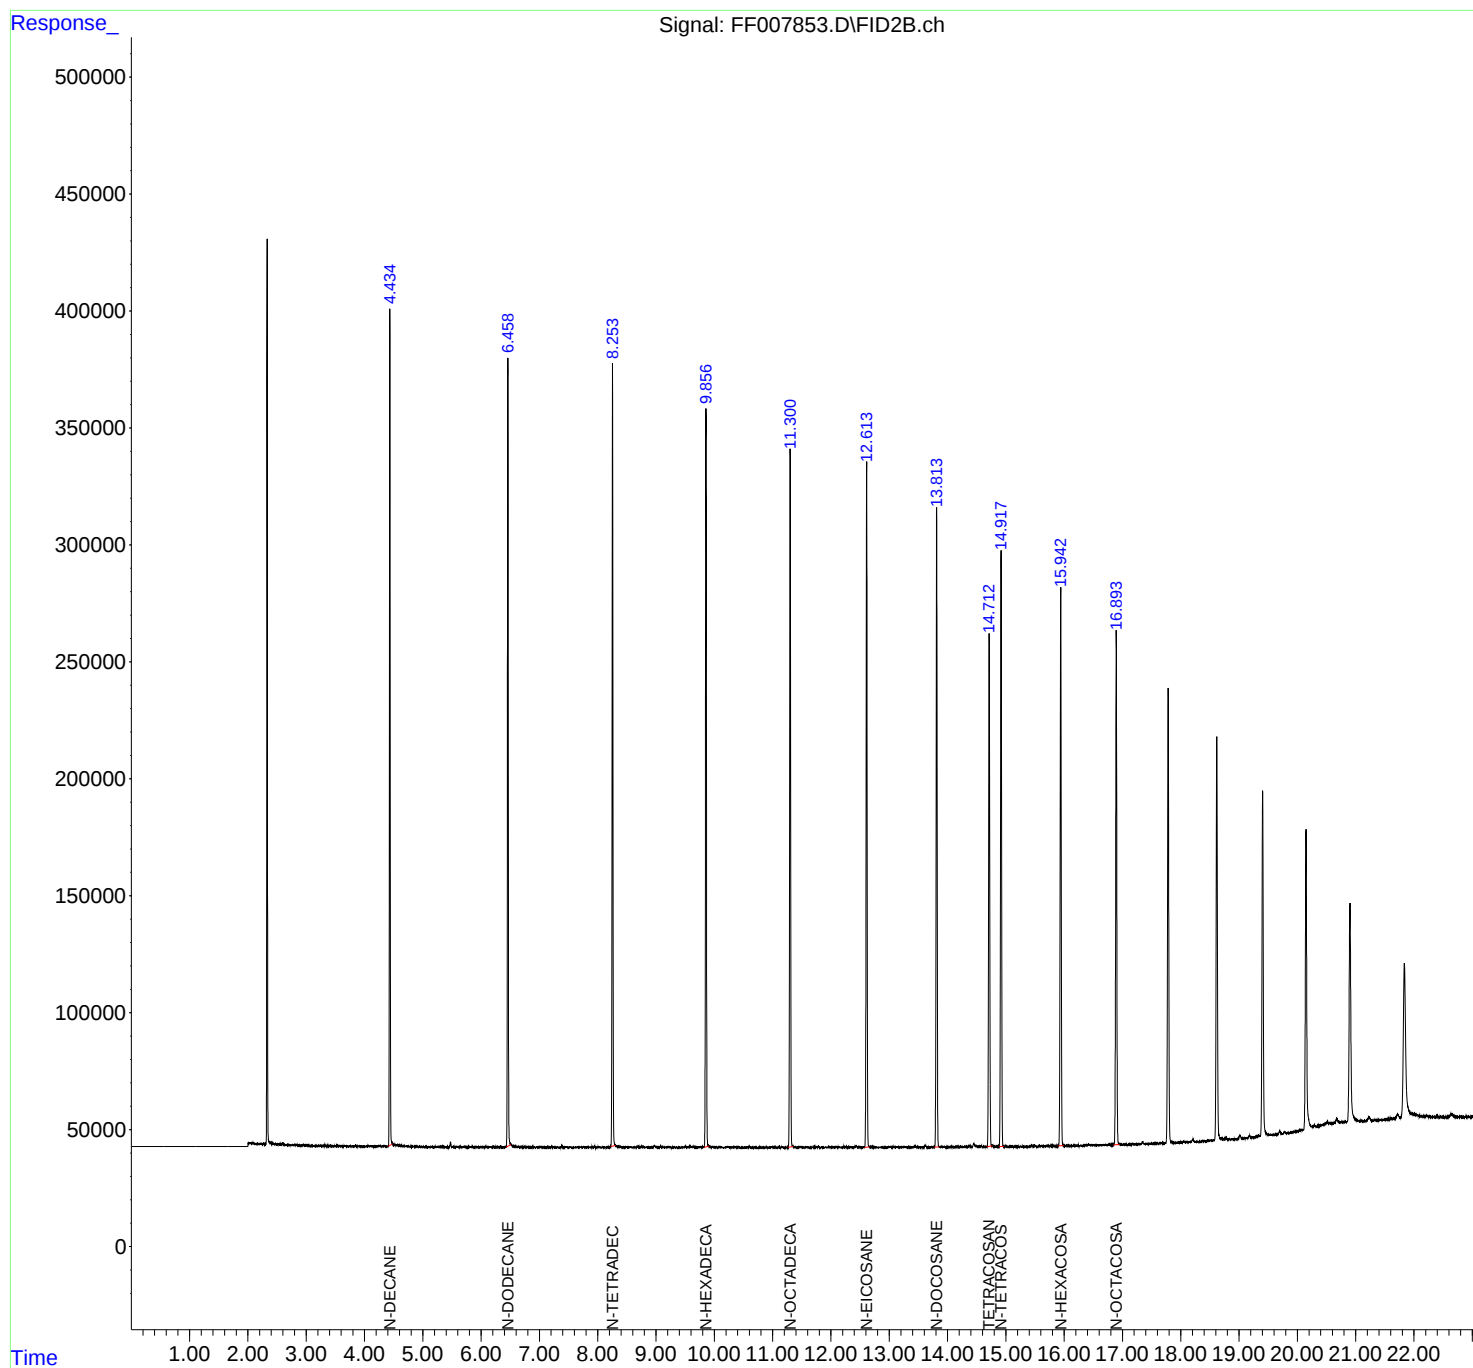


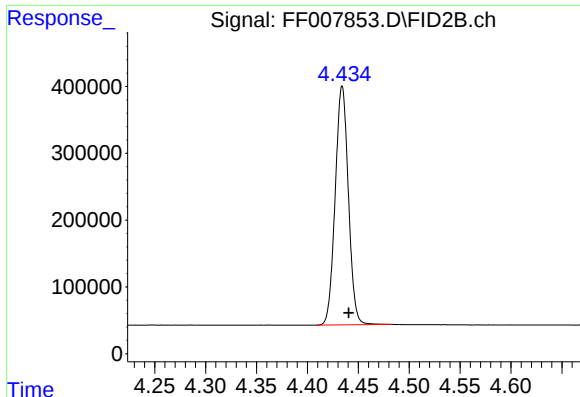

#2 N-DECANE


R.T.: 4.434 min
Delta R.T.: -0.006 min
Response: 3223514
Conc: 23.69 ug/ml

Instrument :
FID_F
ClientSampleId :
PB132940BS

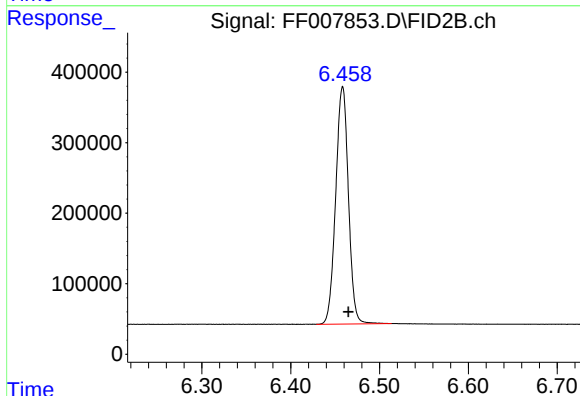


#3 N-DODECANE

R.T.: 6.459 min
Delta R.T.: -0.006 min
Response: 3346419
Conc: 24.18 ug/ml

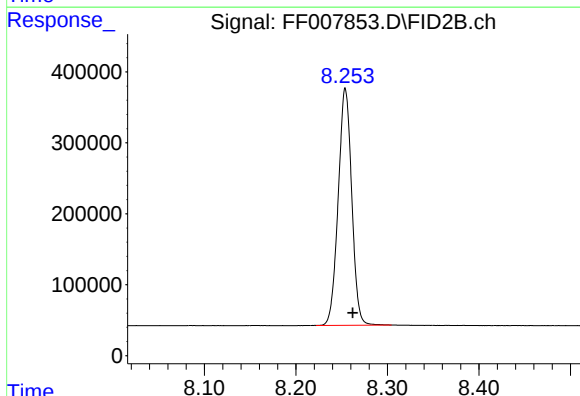


#4 N-TETRADECANE

R.T.: 8.254 min
Delta R.T.: -0.008 min
Response: 3426056
Conc: 24.26 ug/ml

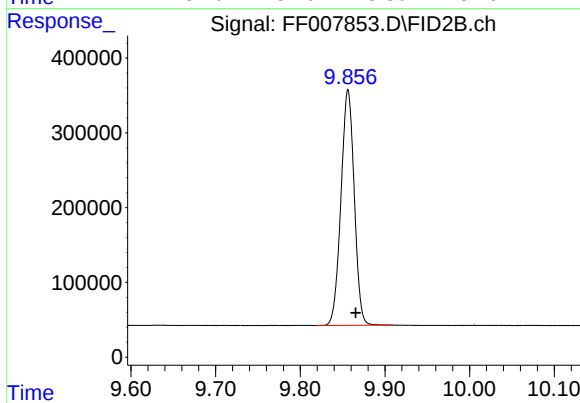

#5 N-HEXADECANE


R.T.: 9.856 min
Delta R.T.: -0.009 min
Response: 3437827
Conc: 23.65 ug/ml

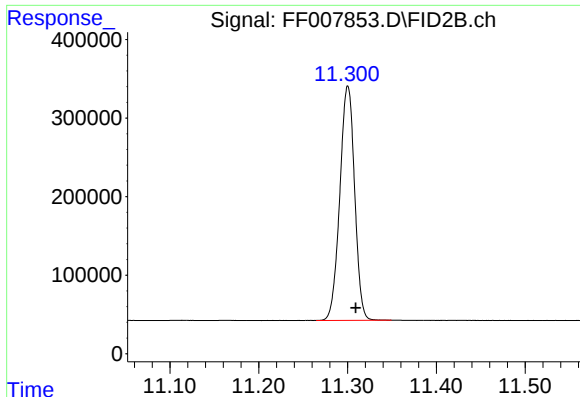

#6 N-OCTADECANE


R.T.: 11.300 min
Delta R.T.: -0.009 min
Response: 3451303
Conc: 23.26 ug/ml

Instrument :
FID_F
ClientSampleId :
PB132940BS

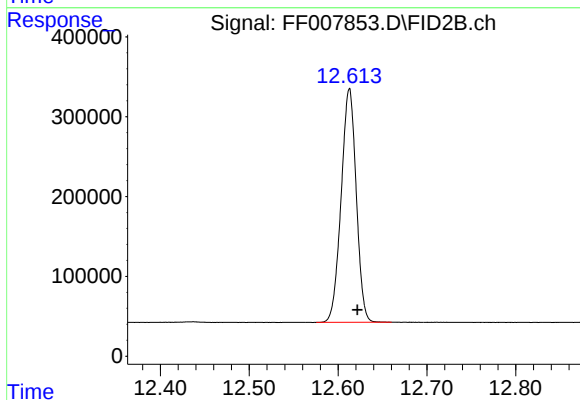


#7 N-EICOSANE

R.T.: 12.613 min
Delta R.T.: -0.009 min
Response: 3452747
Conc: 23.29 ug/ml

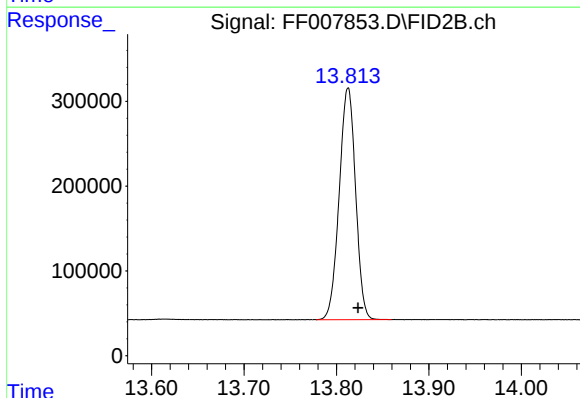


#8 N-DOCOSANE

R.T.: 13.813 min
Delta R.T.: -0.011 min
Response: 3365425
Conc: 23.10 ug/ml

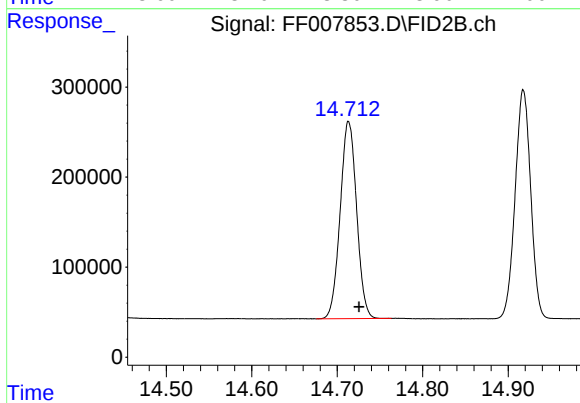

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.713 min
Delta R.T.: -0.012 min
Response: 2929953
Conc: 22.94 ug/ml

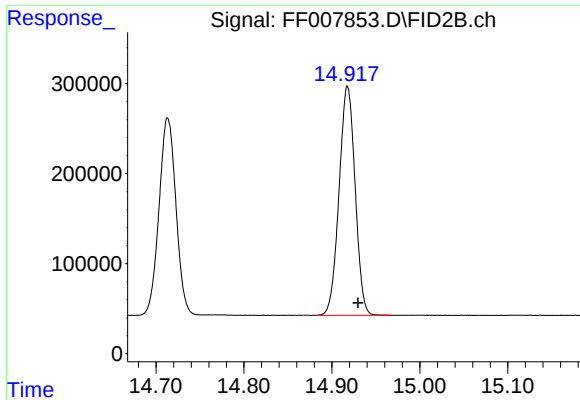

#10 N-TETRACOSANE


R.T.: 14.918 min
Delta R.T.: -0.012 min
Response: 3224611
Conc: 22.30 ug/ml

Instrument :
FID_F
ClientSampleId :
PB132940BS

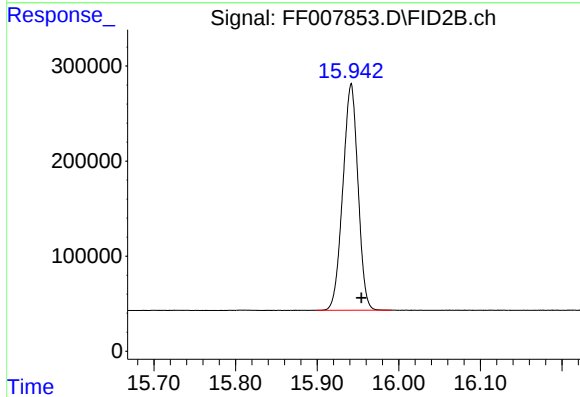

#11 N-HEXACOSANE

R.T.: 15.942 min
Delta R.T.: -0.013 min
Response: 3074952
Conc: 21.91 ug/ml

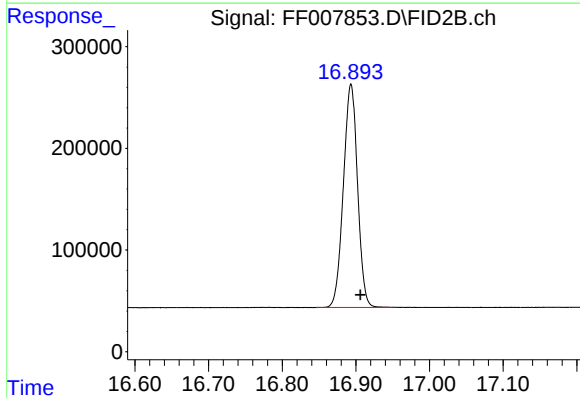

#12 N-OCTACOSANE

R.T.: 16.893 min
Delta R.T.: -0.013 min
Response: 2936976
Conc: 21.65 ug/ml