

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
 Data File : FF007861.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2020 17:44
 Operator : DD\AJ
 Sample : L4680-05MS
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PAV-B7-110920-10-20MS

Integration File: autoint1.e
 Quant Time: Nov 12 01:59:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.718	2556211	20.012 ug/ml
Target Compounds			
2) N-DECANE	4.436	3195028	23.483 ug/ml
3) N-DODECANE	6.461	3325361	24.024 ug/ml
4) N-TETRADECANE	8.258	3398062	24.063 ug/ml
5) N-HEXADECANE	9.860	3395963	23.366 ug/ml
6) N-OCTADECANE	11.304	3345657	22.544 ug/ml
7) N-EICOSANE	12.616	3405541	22.975 ug/ml
8) N-DOCOSANE	13.817	3141652	21.564 ug/ml
10) N-TETRACOSANE	14.921	3617276	25.014 ug/ml
11) N-HEXACOSANE	15.946	2969919	21.161 ug/ml
12) N-OCTACOSANE	16.898	2905329	21.420 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111120\
Data File : FF007861.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2020 17:44
Operator : DD\AJ
Sample : L4680-05MS
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PAV-B7-110920-10-20MS

Integration File: autoint1.e
Quant Time: Nov 12 01:59:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

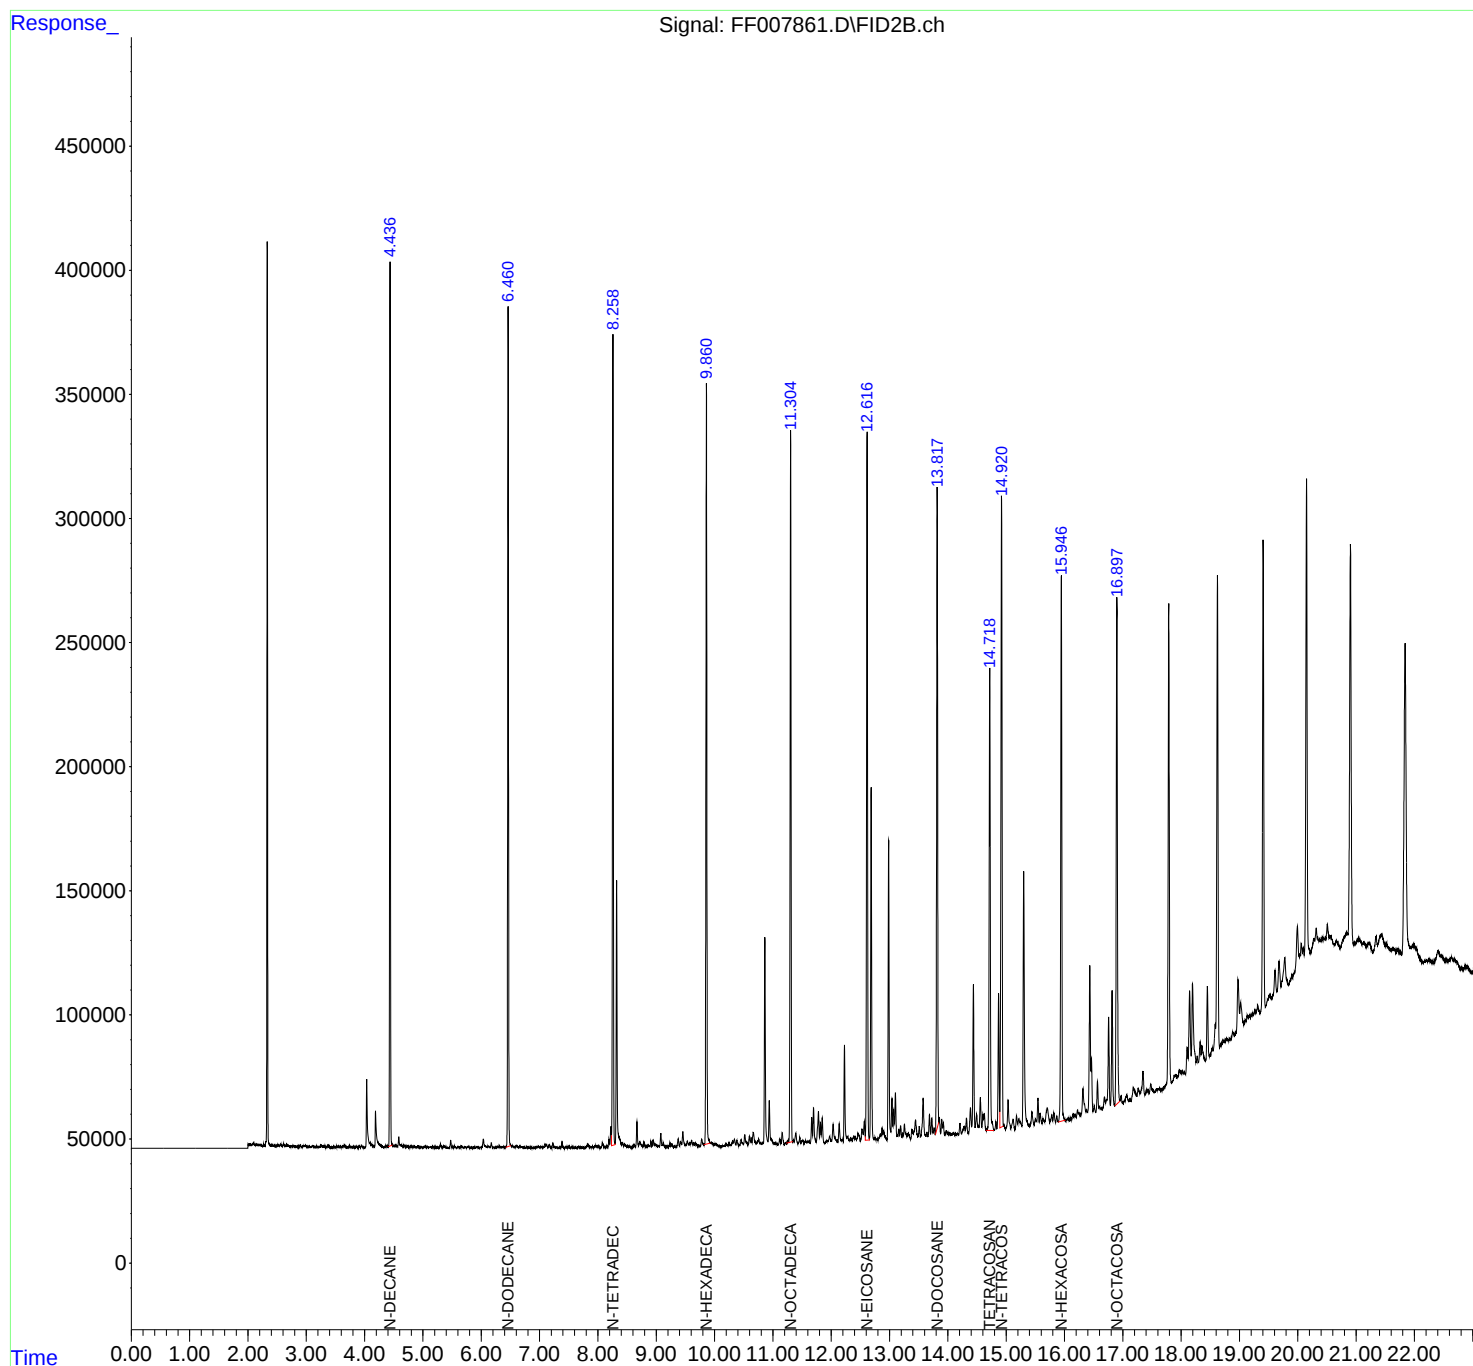


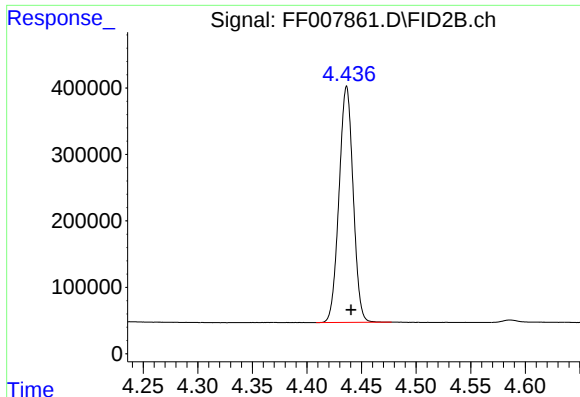

#2 N-DECANE


R.T.: 4.436 min
Delta R.T.: -0.004 min
Response: 3195028
Conc: 23.48 ug/ml

Instrument :
FID_F
ClientSampleId :
PAV-B7-110920-10-20MS

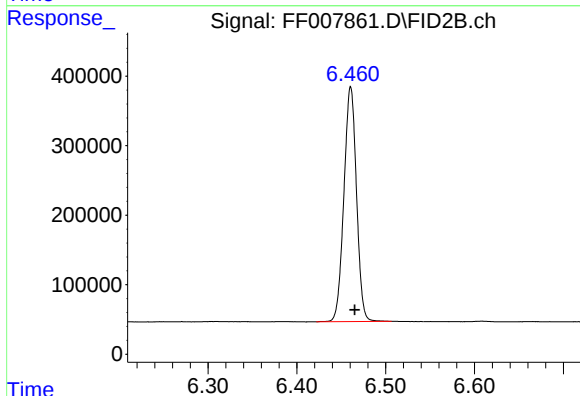


#3 N-DODECANE

R.T.: 6.461 min
Delta R.T.: -0.004 min
Response: 3325361
Conc: 24.02 ug/ml

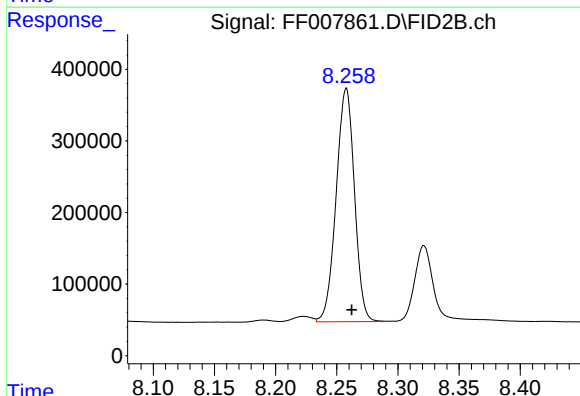


#4 N-TETRADECANE

R.T.: 8.258 min
Delta R.T.: -0.004 min
Response: 3398062
Conc: 24.06 ug/ml

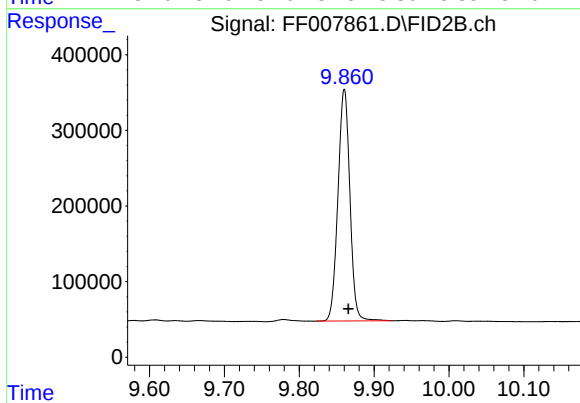

#5 N-HEXADECANE


R.T.: 9.860 min
Delta R.T.: -0.005 min
Response: 3395963
Conc: 23.37 ug/ml

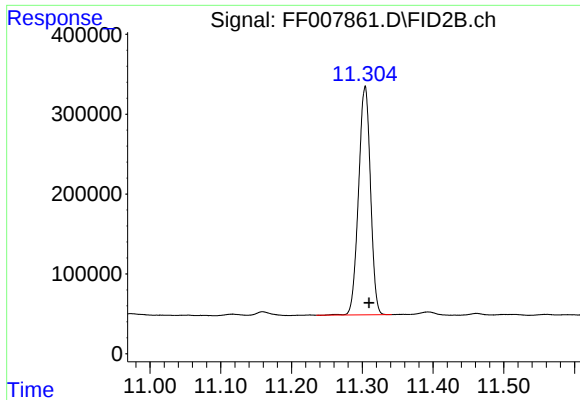

#6 N-OCTADECANE


R.T.: 11.304 min
Delta R.T.: -0.005 min
Response: 3345657
Conc: 22.54 ug/ml

Instrument :
FID_F
ClientSampleId :
PAV-B7-110920-10-20MS

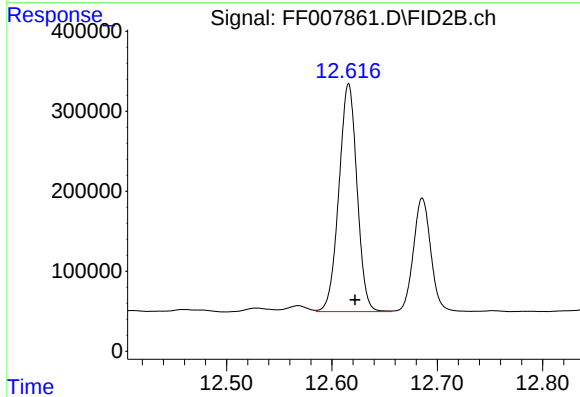


#7 N-EICOSANE

R.T.: 12.616 min
Delta R.T.: -0.006 min
Response: 3405541
Conc: 22.98 ug/ml

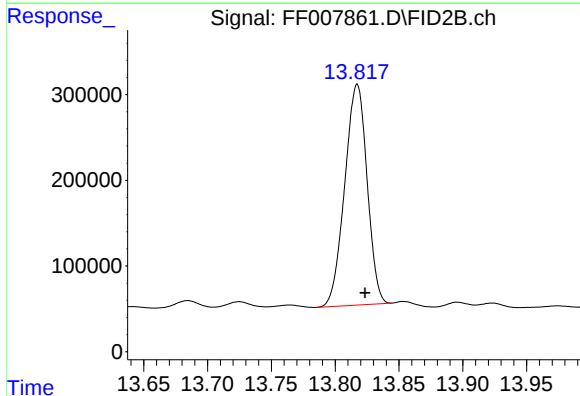


#8 N-DOCOSANE

R.T.: 13.817 min
Delta R.T.: -0.006 min
Response: 3141652
Conc: 21.56 ug/ml

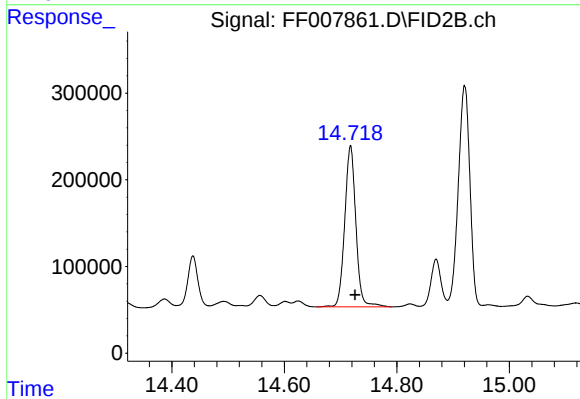

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.718 min
Delta R.T.: -0.008 min
Response: 2556211
Conc: 20.01 ug/ml

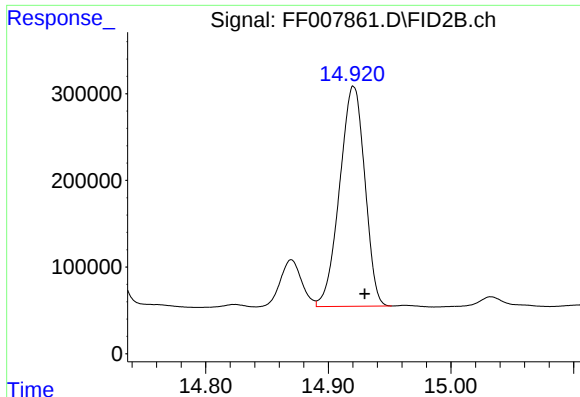

#10 N-TETRACOSANE


R.T.: 14.921 min
Delta R.T.: -0.009 min
Response: 3617276
Conc: 25.01 ug/ml

Instrument :
FID_F
ClientSampleId :
PAV-B7-110920-10-20MS

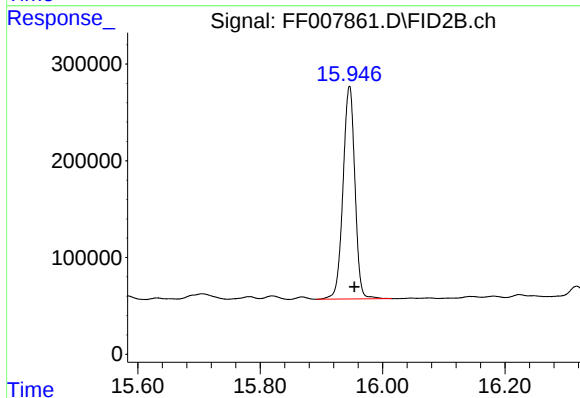

#11 N-HEXACOSANE

R.T.: 15.946 min
Delta R.T.: -0.008 min
Response: 2969919
Conc: 21.16 ug/ml

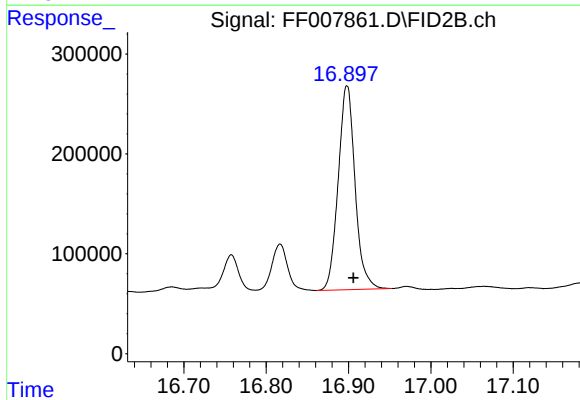

#12 N-OCTACOSANE

R.T.: 16.898 min
Delta R.T.: -0.008 min
Response: 2905329
Conc: 21.42 ug/ml