

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011649.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2022 18:12
Operator : YP\AJ
Sample : N5578-02
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FFF-PMW-02D

Integration File: autoint1.e
Quant Time: Nov 14 02:24:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.056	2051889	17.294 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.476	26886	0.218 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011649.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2022 18:12
Operator : YP\AJ
Sample : N5578-02
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FFF-PMW-02D

Integration File: autoint1.e
Quant Time: Nov 14 02:24:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

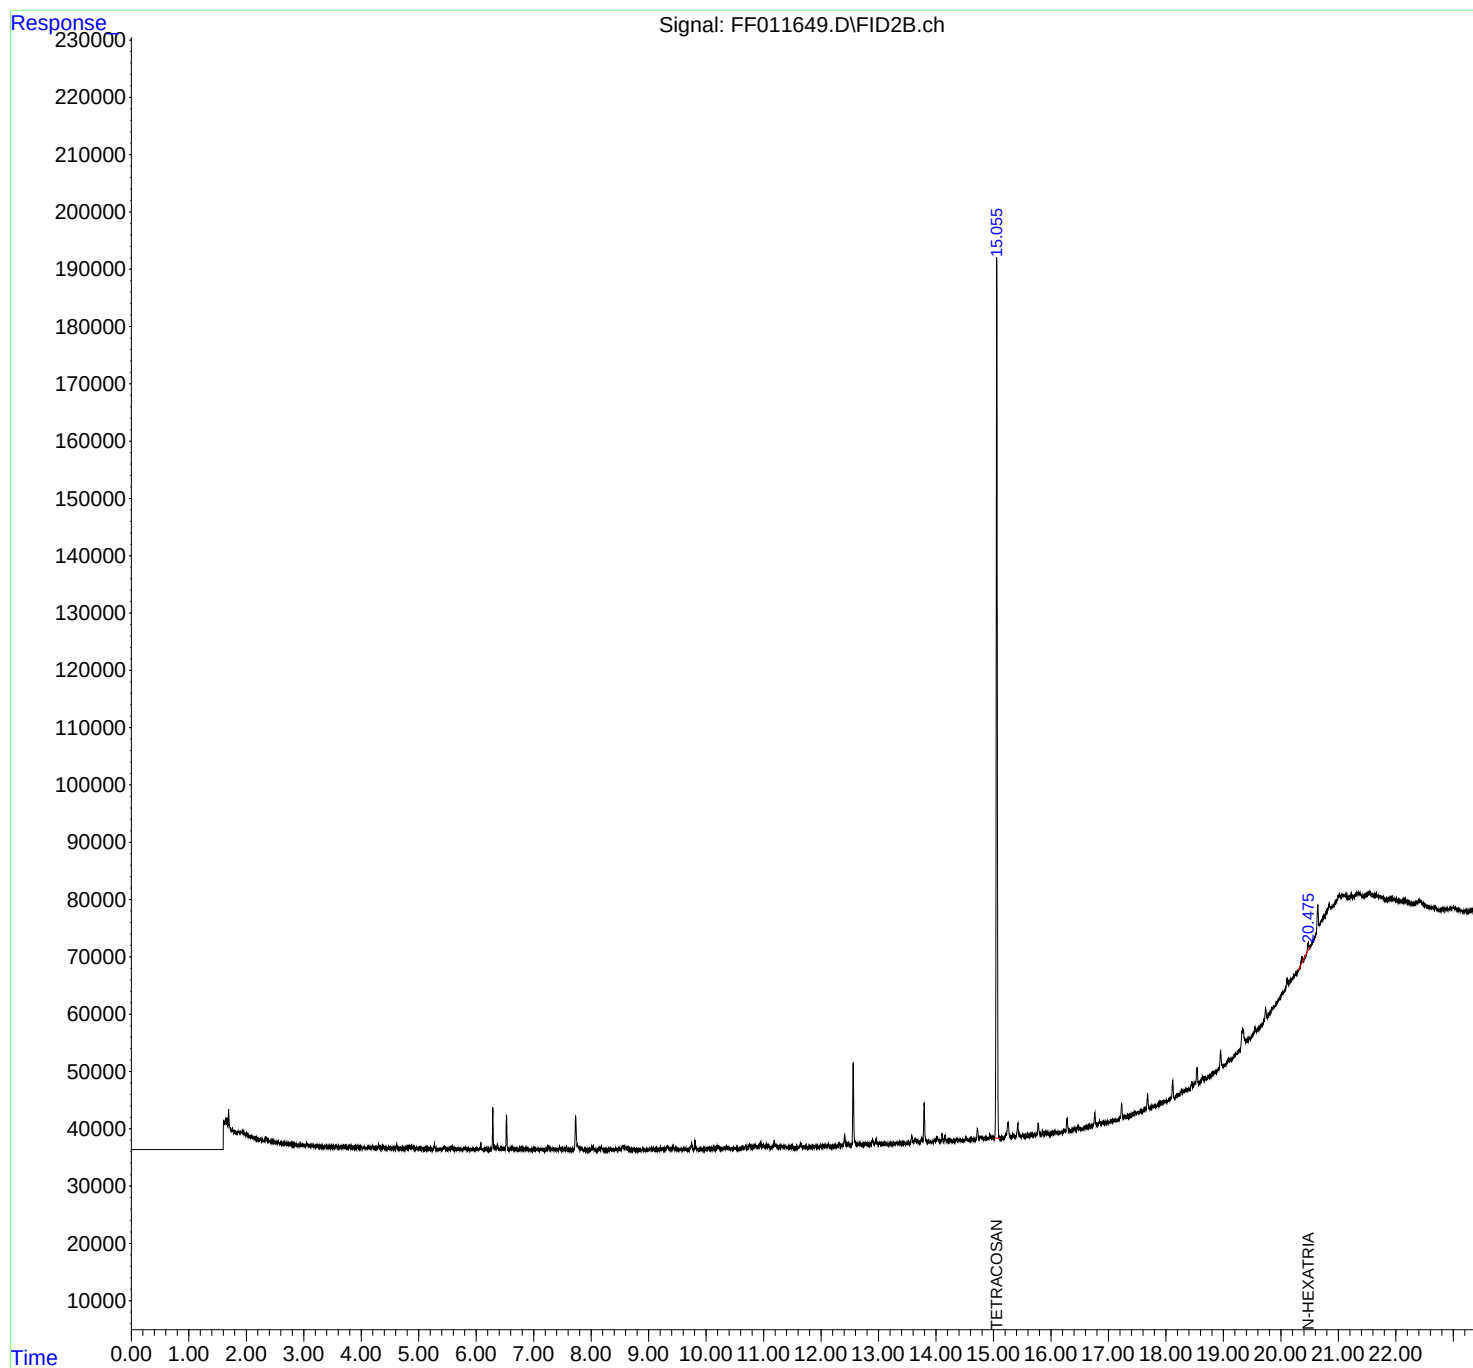


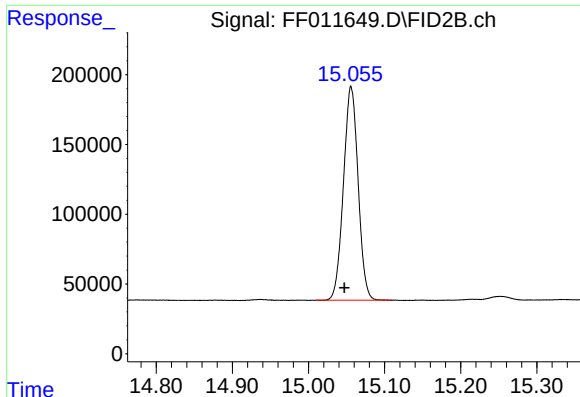

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.056 min
Delta R.T.: 0.009 min
Response: 2051889
Conc: 17.29 ug/ml

Instrument :
FID_F
ClientSampleId :
FFF-PMW-02D

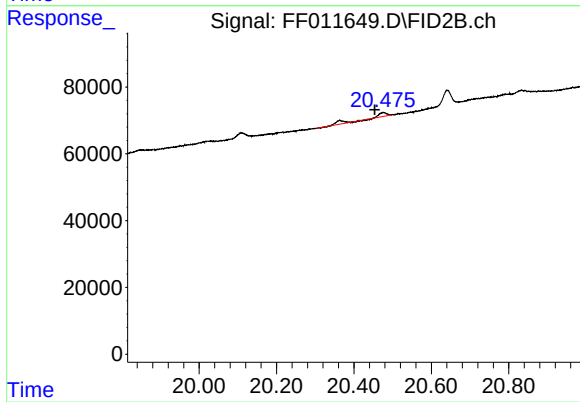

#16 N-HEXATRIACONTANE

R.T.: 20.476 min
Delta R.T.: 0.022 min
Response: 26886
Conc: 0.22 ug/ml