

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
 Data File : FF011653.D
 Signal(s) : FID2B.ch
 Acq On : 11 Nov 2022 20:12
 Operator : YP\AJ
 Sample : N5578-06
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 LOC-25-10

Integration File: autoint1.e
 Quant Time: Nov 14 02:25:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.056	2202654	18.565 ug/ml
Target Compounds			
15) N-TETRATRIACONTANE	19.735	31445	0.239 ug/ml
16) N-HEXATRIACONTANE	20.475	213872	1.736 ug/ml
17) N-OCTATRIACONTANE	21.216	824263	7.079 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011653.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2022 20:12
Operator : YP\AJ
Sample : N5578-06
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
LOC-25-10

Integration File: autoint1.e
Quant Time: Nov 14 02:25:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

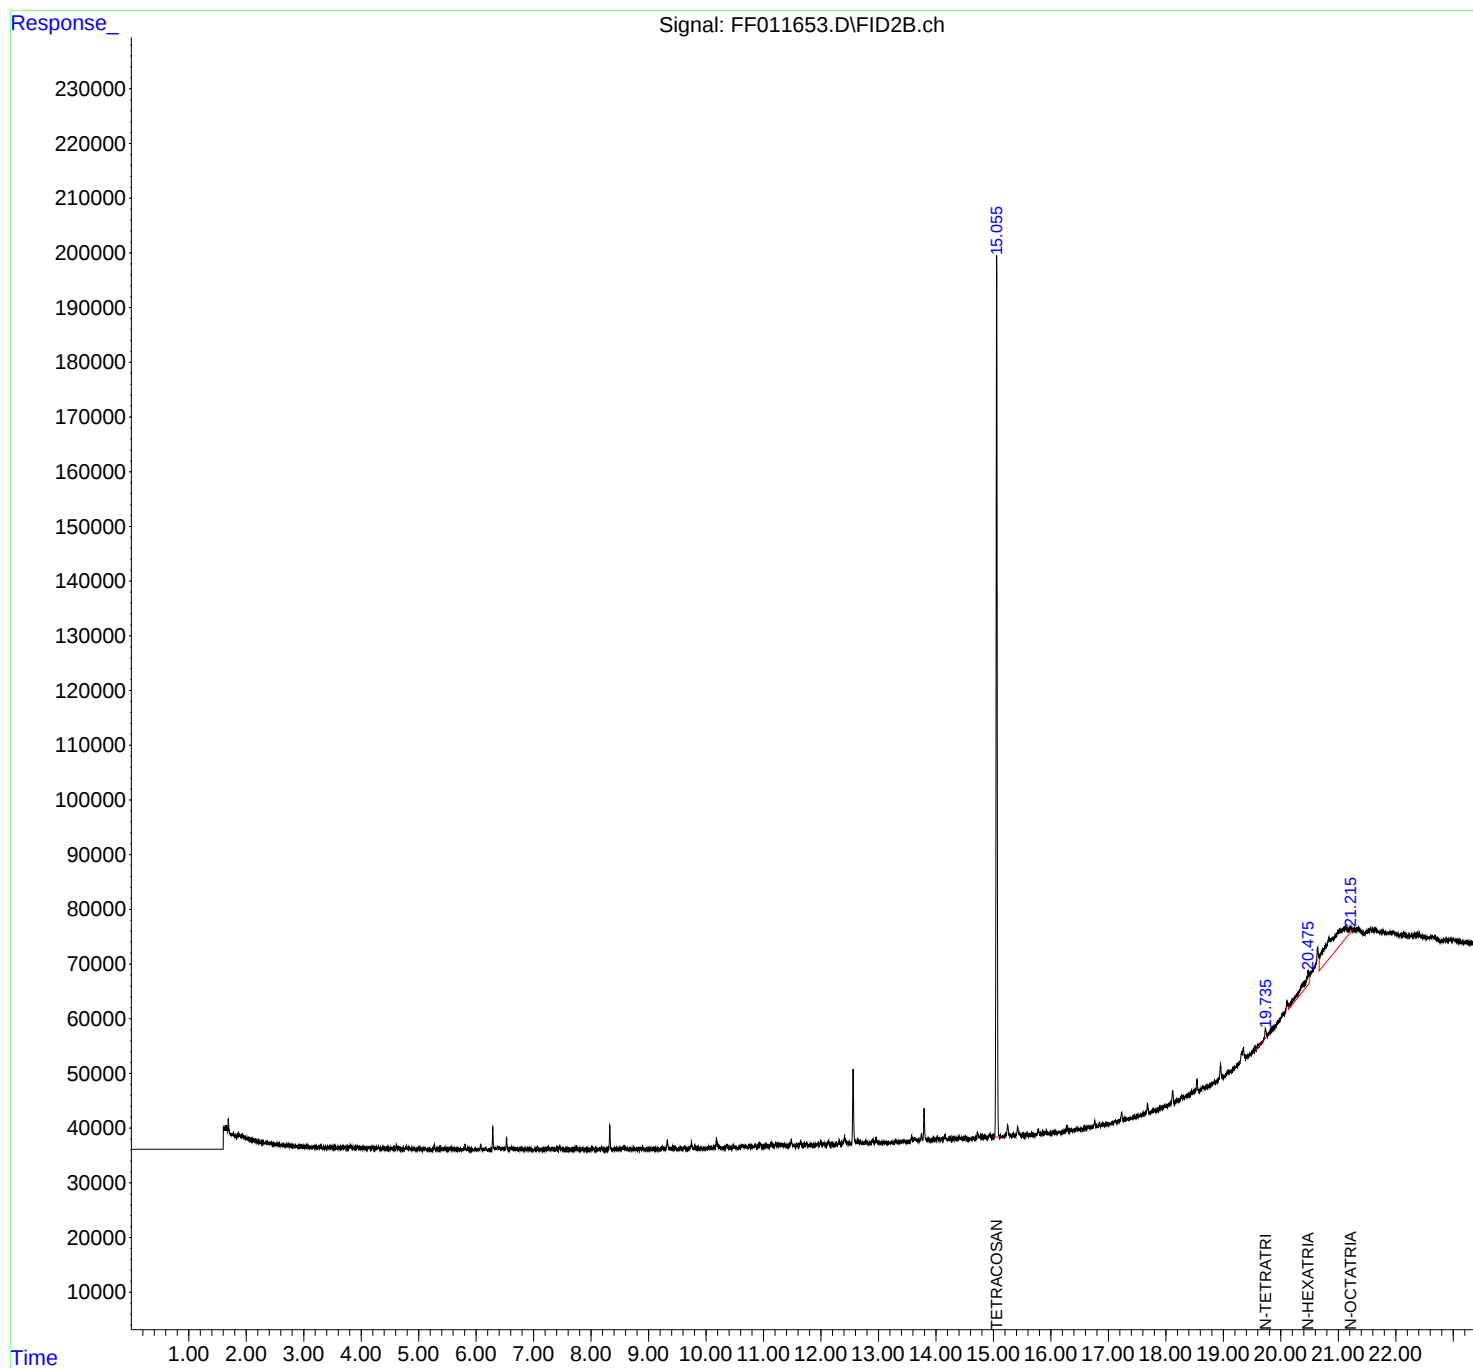


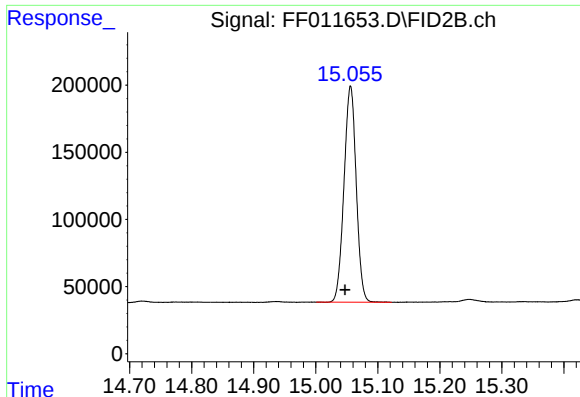

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.056 min
Delta R.T.: 0.009 min
Response: 2202654
Conc: 18.57 ug/ml

Instrument :
FID_F
ClientSampleId :
LOC-25-10

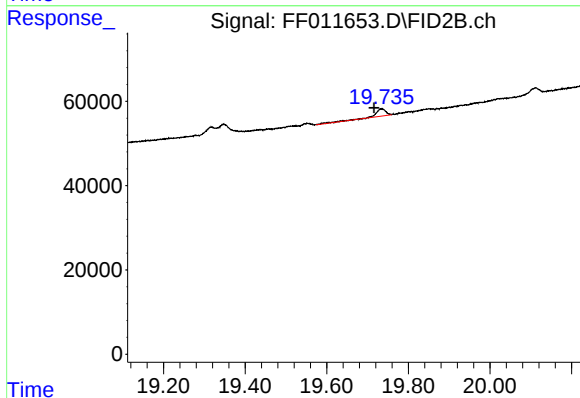


#15 N-TETRATRIACONTANE

R.T.: 19.735 min
Delta R.T.: 0.019 min
Response: 31445
Conc: 0.24 ug/ml

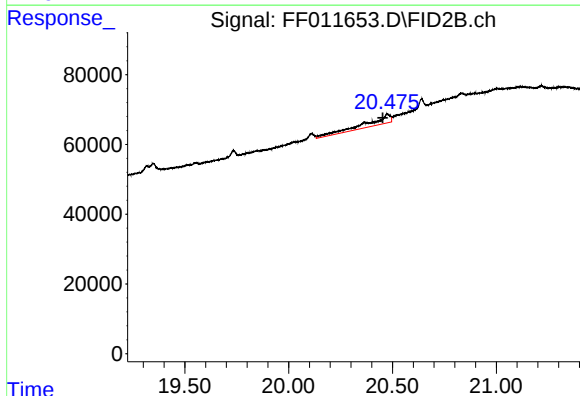

#16 N-HEXATRIACONTANE

R.T.: 20.475 min
Delta R.T.: 0.021 min
Response: 213872
Conc: 1.74 ug/ml

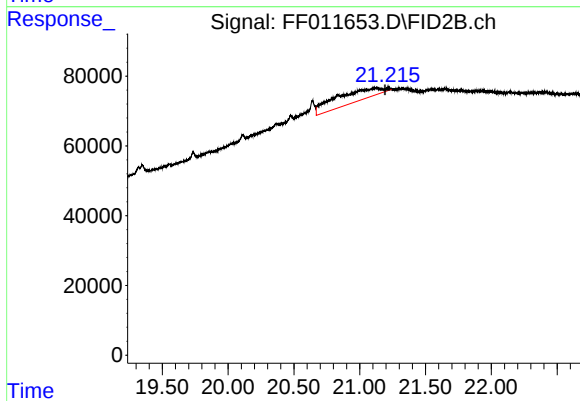

#17 N-OCTATRIACONTANE

R.T.: 21.216 min
Delta R.T.: 0.021 min
Response: 824263
Conc: 7.08 ug/ml