

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
 Data File : FF011661.D
 Signal(s) : FID2B.ch
 Acq On : 12 Nov 2022 01:11
 Operator : YP\AJ
 Sample : N5578-12
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CAC-HPT-2-GW-(27-30)

Integration File: autoint1.e
 Quant Time: Nov 14 02:27:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.055	1283800	10.821 ug/ml
Target Compounds			
3) N-DODECANE	6.774	47986	0.357 ug/ml
4) N-TETRADECANE	8.598	181099	1.338 ug/ml
5) N-HEXADECANE	10.204	352601	2.565 ug/ml
6) N-OCTADECANE	11.646	305481	2.208 ug/ml
7) N-EICOSANE	12.955	229370	1.659 ug/ml
8) N-DOCOSANE	14.154	115953	0.859 ug/ml
10) N-TETRACOSANE	15.256	77724	0.573 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011661.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 01:11
Operator : YP\AJ
Sample : N5578-12
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAC-HPT-2-GW-(27-30)

Integration File: autoint1.e
Quant Time: Nov 14 02:27:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

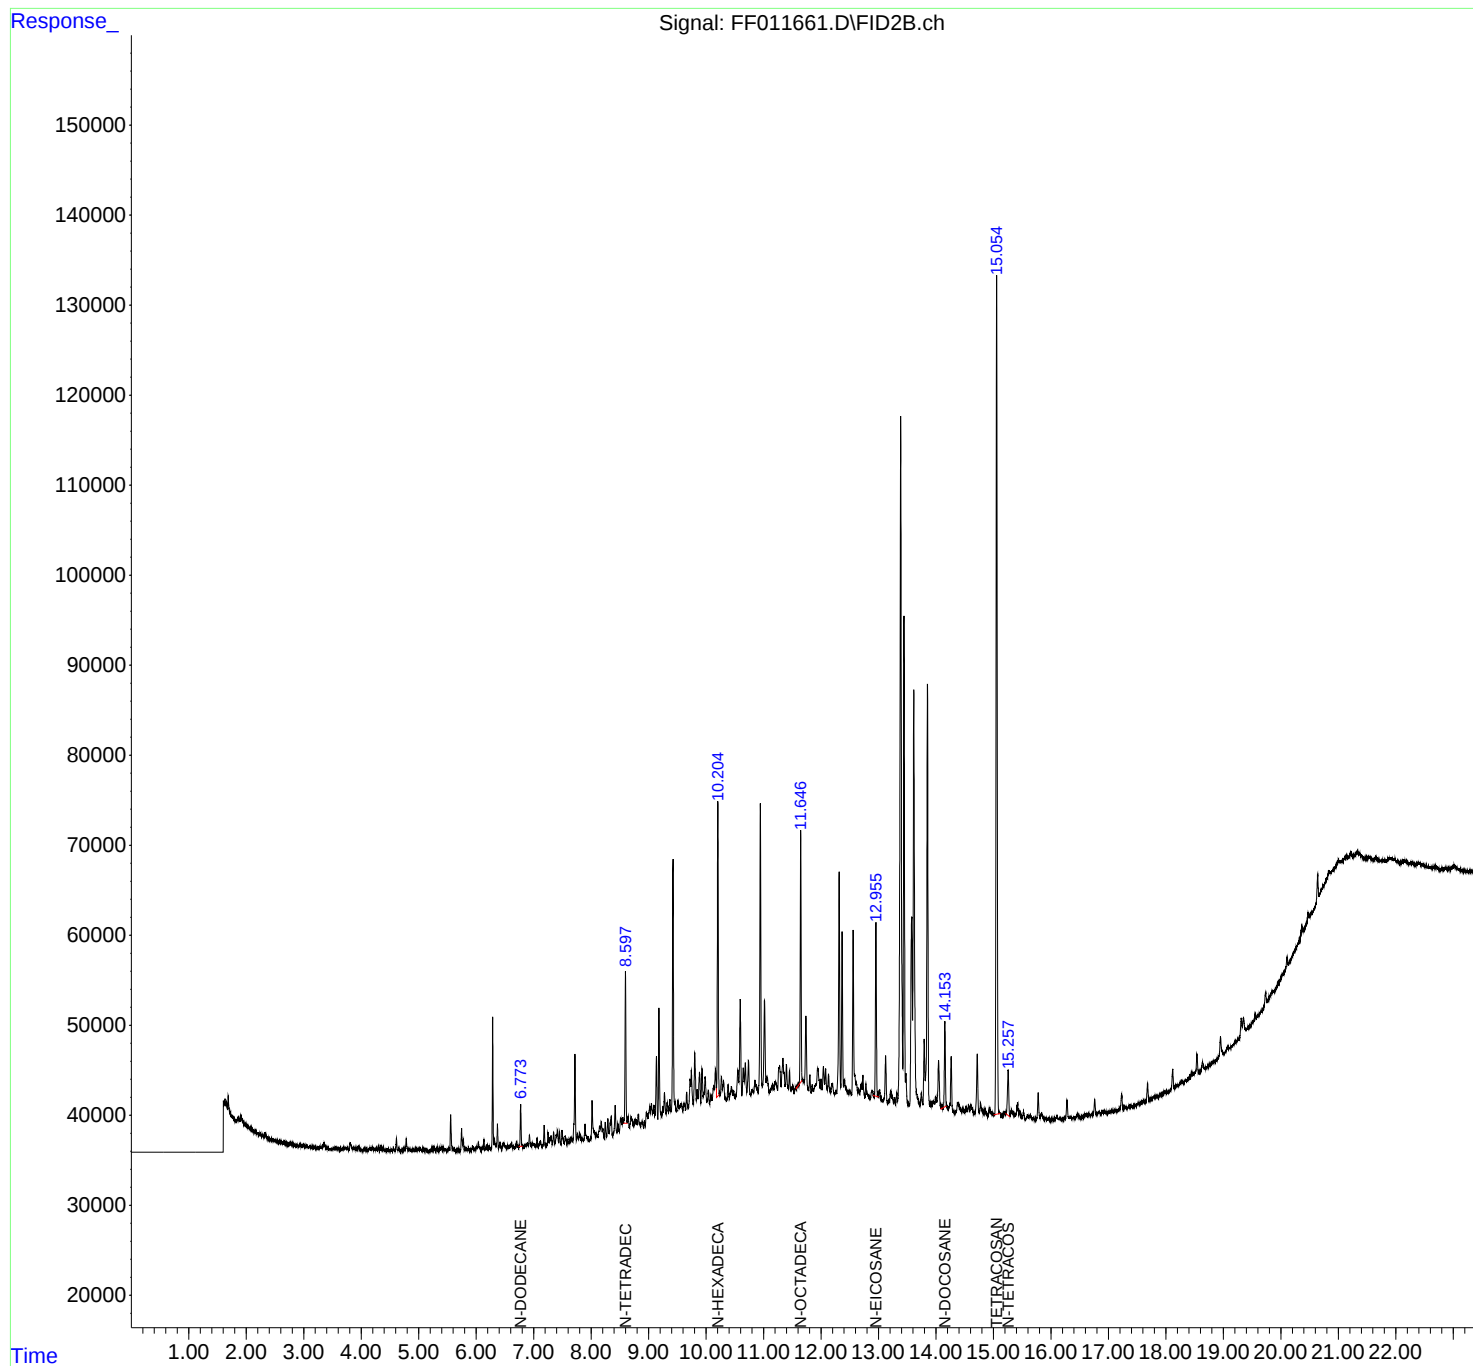


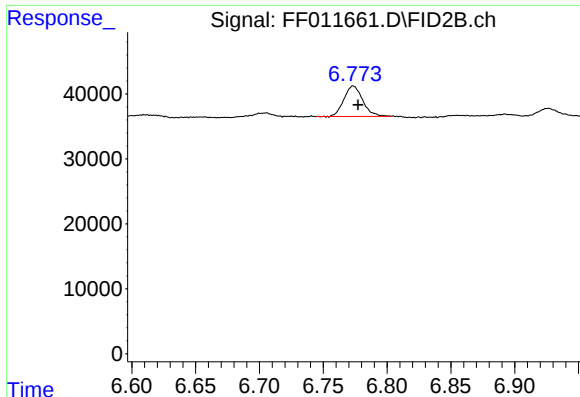

#3 N-DODECANE


R.T.: 6.774 min
Delta R.T.: -0.004 min
Response: 47986
Conc: 0.36 ug/ml

Instrument :
FID_F
ClientSampleId :
CAC-HPT-2-GW-(27-30)

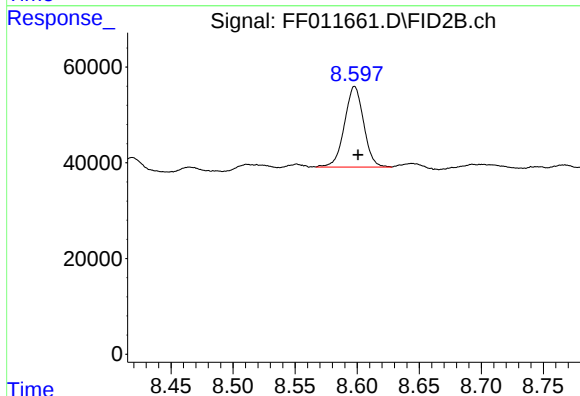


#4 N-TETRADECANE

R.T.: 8.598 min
Delta R.T.: -0.003 min
Response: 181099
Conc: 1.34 ug/ml

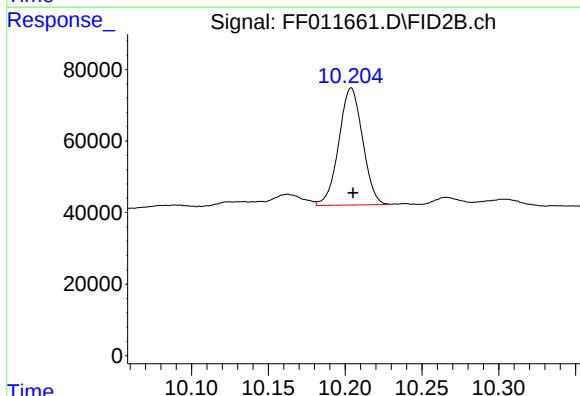


#5 N-HEXADECANE

R.T.: 10.204 min
Delta R.T.: -0.001 min
Response: 352601
Conc: 2.56 ug/ml

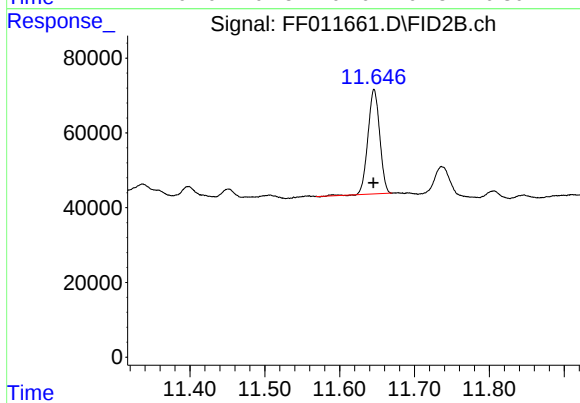

#6 N-OCTADECANE


R.T.: 11.646 min
Delta R.T.: 0.000 min
Response: 305481
Conc: 2.21 ug/ml

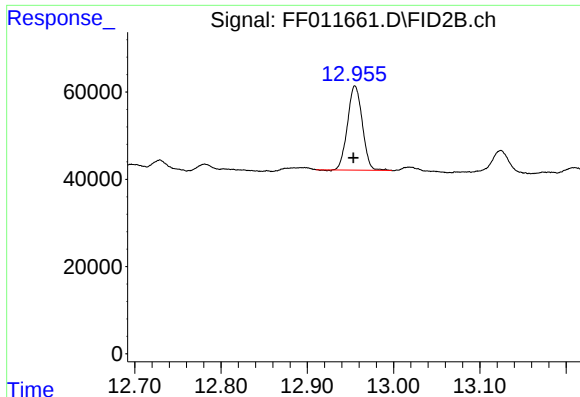

#7 N-EICOSANE


R.T.: 12.955 min
Delta R.T.: 0.002 min
Response: 229370
Conc: 1.66 ug/ml

Instrument :
FID_F
ClientSampleId :
CAC-HPT-2-GW-(27-30)

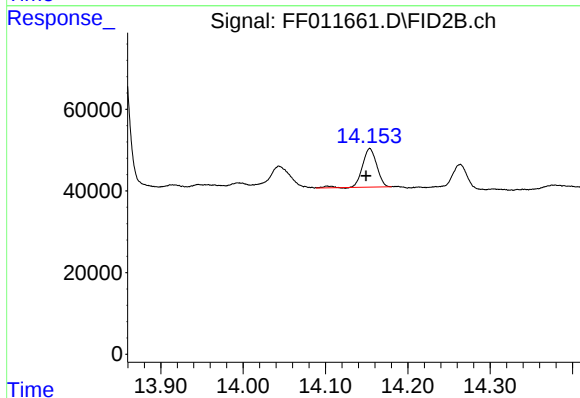


#8 N-DOCOSANE

R.T.: 14.154 min
Delta R.T.: 0.005 min
Response: 115953
Conc: 0.86 ug/ml

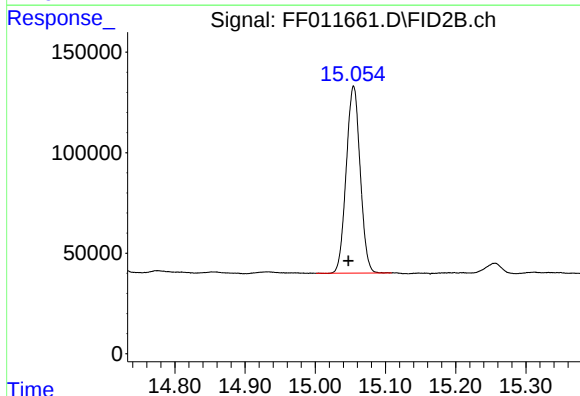

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.055 min
Delta R.T.: 0.008 min
Response: 1283800
Conc: 10.82 ug/ml

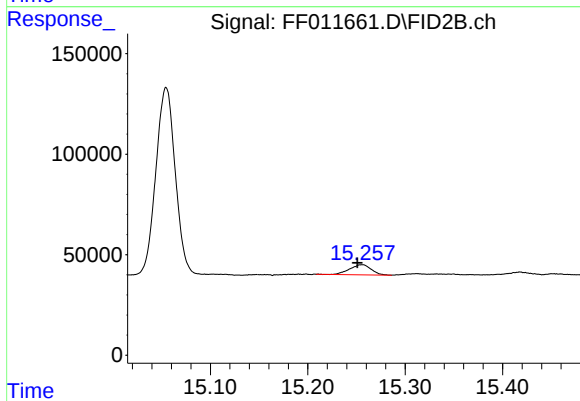

#10 N-TETRACOSANE

R.T.: 15.256 min
Delta R.T.: 0.005 min
Response: 77724
Conc: 0.57 ug/ml