

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
 Data File : FF011662.D
 Signal(s) : FID2B.ch
 Acq On : 12 Nov 2022 01:41
 Operator : YP\AJ
 Sample : N5578-13
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CAC-HPT-2-GW-(35-38)

Integration File: autoint1.e
 Quant Time: Nov 14 02:27:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.053	1425234	12.013 ug/ml
Target Compounds			
4) N-TETRADECANE	8.567	370918	2.741 ug/ml
5) N-HEXADECANE	10.263f	205008	1.491 ug/ml
12) N-OCTACOSANE	17.279f	220071	1.661 ug/ml
13) N-TRIACONTANE	18.117	51197	0.388 ug/ml
14) N-DOTRIACONTANE	18.948	81304	0.604 ug/ml
15) N-TETRATRIACONTANE	19.734	47146	0.358 ug/ml
16) N-HEXATRIACONTANE	20.476	68704	0.558 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011662.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 01:41
Operator : YP\AJ
Sample : N5578-13
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAC-HPT-2-GW-(35-38)

Integration File: autoint1.e
Quant Time: Nov 14 02:27:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

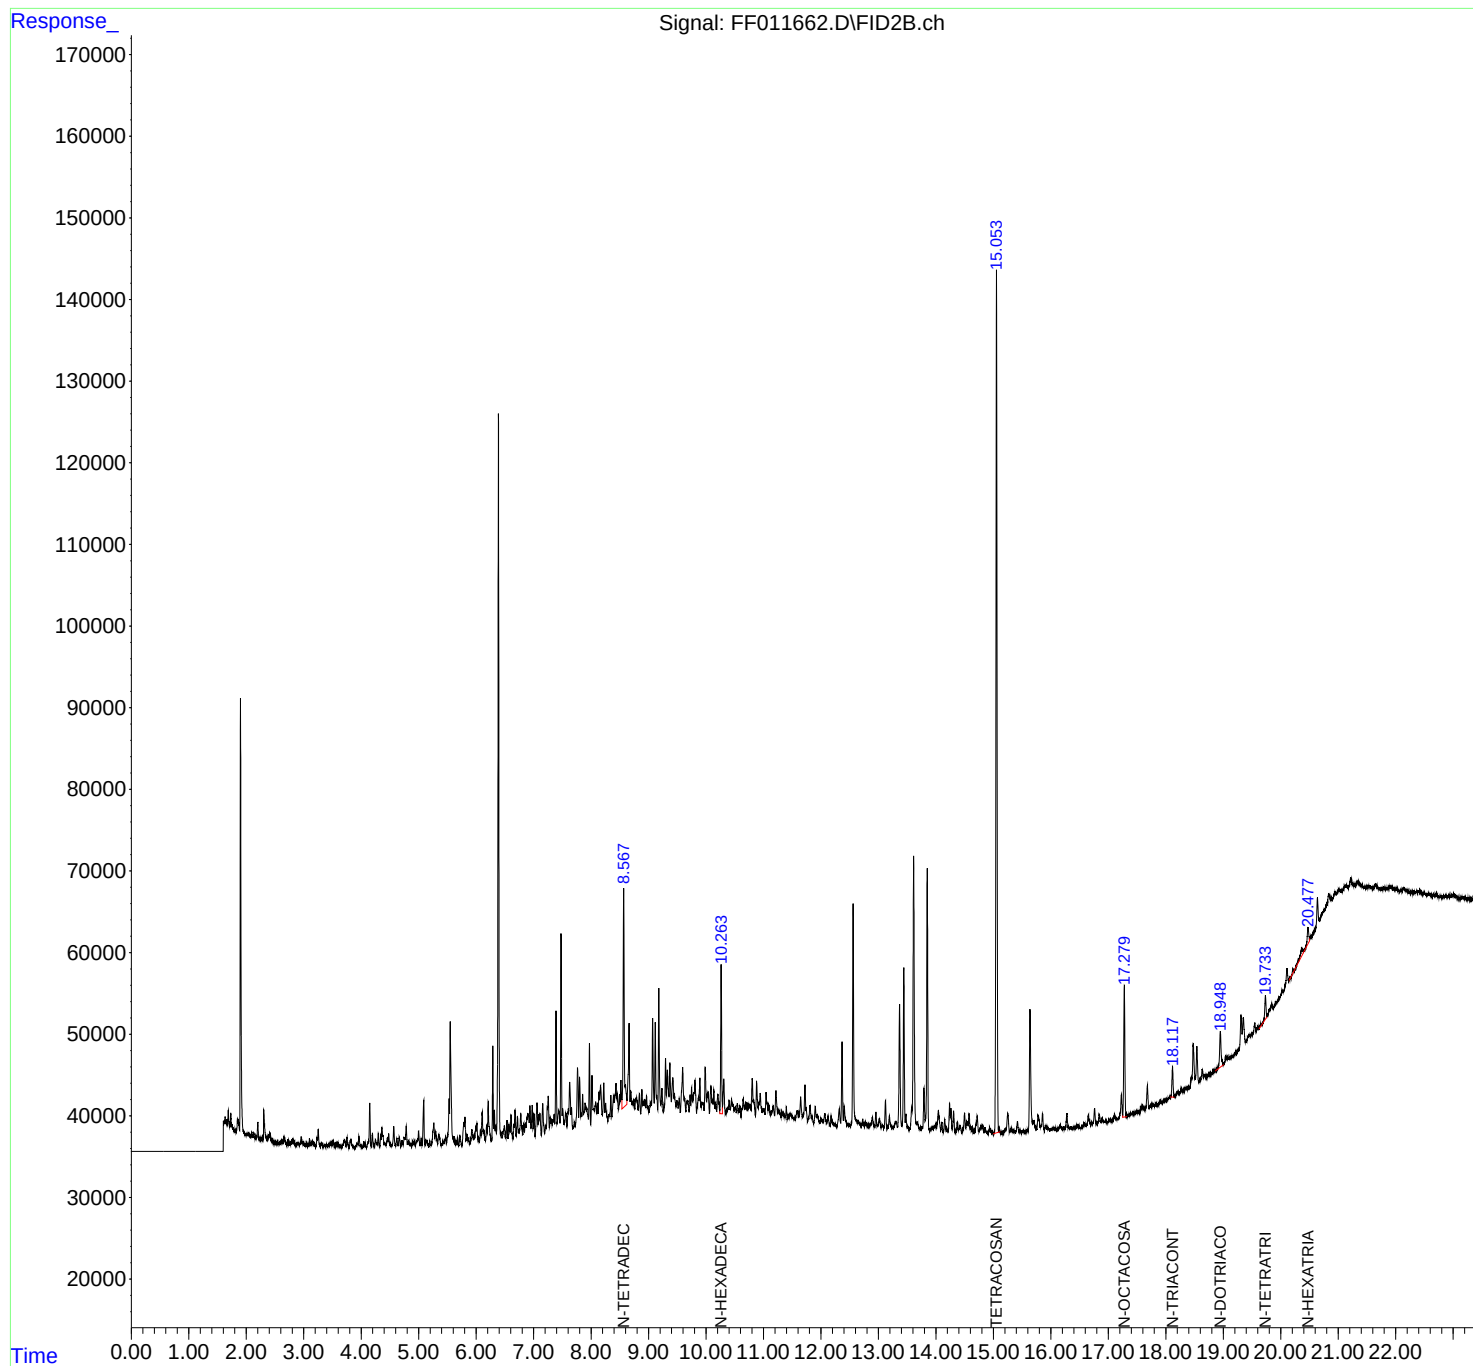


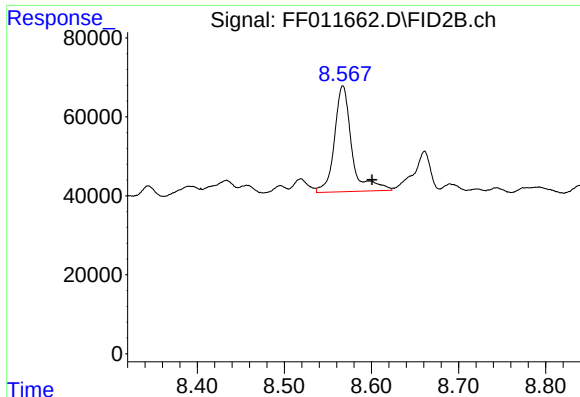

#4 N-TETRADECANE


R.T.: 8.567 min
Delta R.T.: -0.034 min
Response: 370918
Conc: 2.74 ug/ml

Instrument :
FID_F
ClientSampleId :
CAC-HPT-2-GW-(35-38)

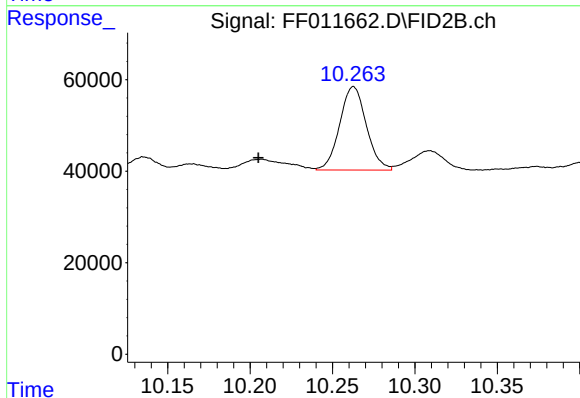


#5 N-HEXADECANE

R.T.: 10.263 min
Delta R.T.: 0.058 min
Response: 205008
Conc: 1.49 ug/ml

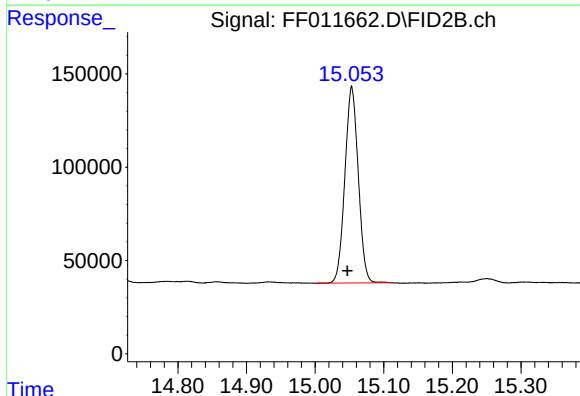


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.053 min
Delta R.T.: 0.006 min
Response: 1425234
Conc: 12.01 ug/ml

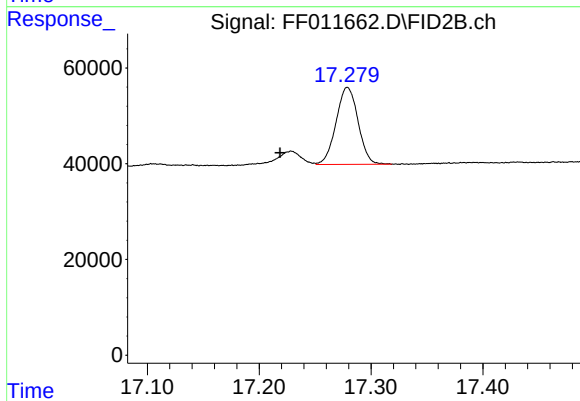

#12 N-OCTACOSANE


R.T.: 17.279 min
Delta R.T.: 0.060 min
Response: 220071
Conc: 1.66 ug/ml

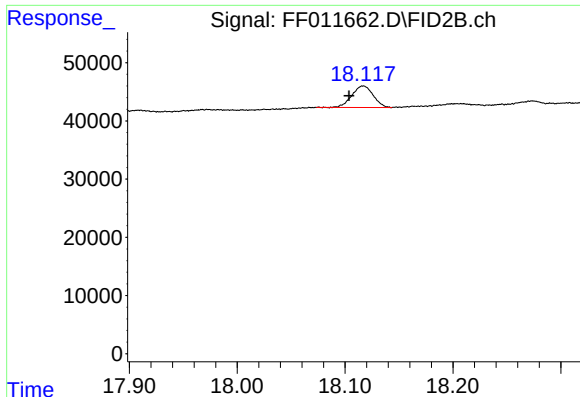

#13 N-TRIACONTANE


R.T.: 18.117 min
Delta R.T.: 0.013 min
Response: 51197
Conc: 0.39 ug/ml

Instrument :
FID_F
ClientSampleId :
CAC-HPT-2-GW-(35-38)

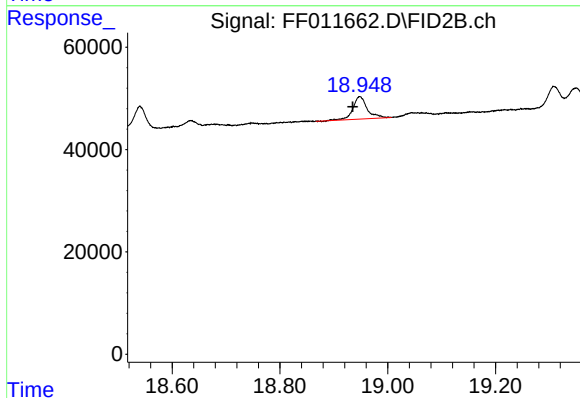


#14 N-DOTRIACONTANE

R.T.: 18.948 min
Delta R.T.: 0.013 min
Response: 81304
Conc: 0.60 ug/ml

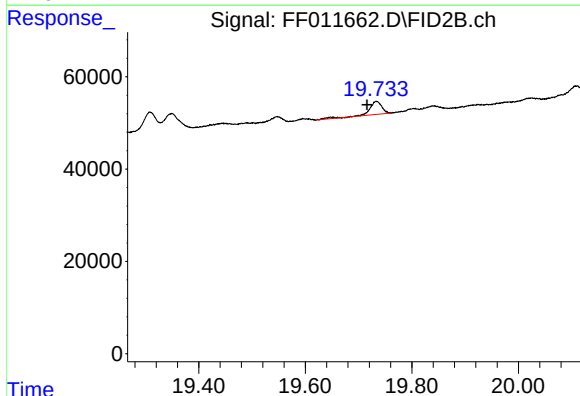

#15 N-TETRATRIACONTANE

R.T.: 19.734 min
Delta R.T.: 0.017 min
Response: 47146
Conc: 0.36 ug/ml

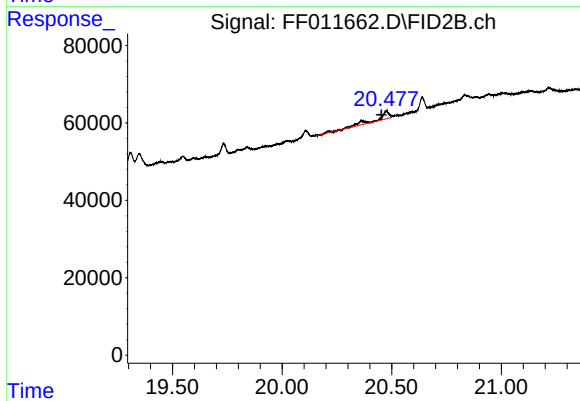

#16 N-HEXATRIACONTANE

R.T.: 20.476 min
Delta R.T.: 0.022 min
Response: 68704
Conc: 0.56 ug/ml