

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
 Data File : FF011664.D
 Signal(s) : FID2B.ch
 Acq On : 12 Nov 2022 02:41
 Operator : YP\AJ
 Sample : N5578-15
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CAC-HPT-3-GW-(14-17)

Integration File: autoint1.e
 Quant Time: Nov 14 02:27:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.055	1483893	12.507 ug/ml
Target Compounds			
3) N-DODECANE	6.785	102674	0.764 ug/ml
4) N-TETRADECANE	8.552	47101	0.348 ug/ml
5) N-HEXADECANE	10.181	64220	0.467 ug/ml
14) N-DOTRIACONTANE	18.949	48638	0.361 ug/ml
15) N-TETRATRIACONTANE	19.733	22913	0.174 ug/ml
16) N-HEXATRIACONTANE	20.474	69143	0.561 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011664.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 02:41
Operator : YP\AJ
Sample : N5578-15
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAC-HPT-3-GW-(14-17)

Integration File: autoint1.e
Quant Time: Nov 14 02:27:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

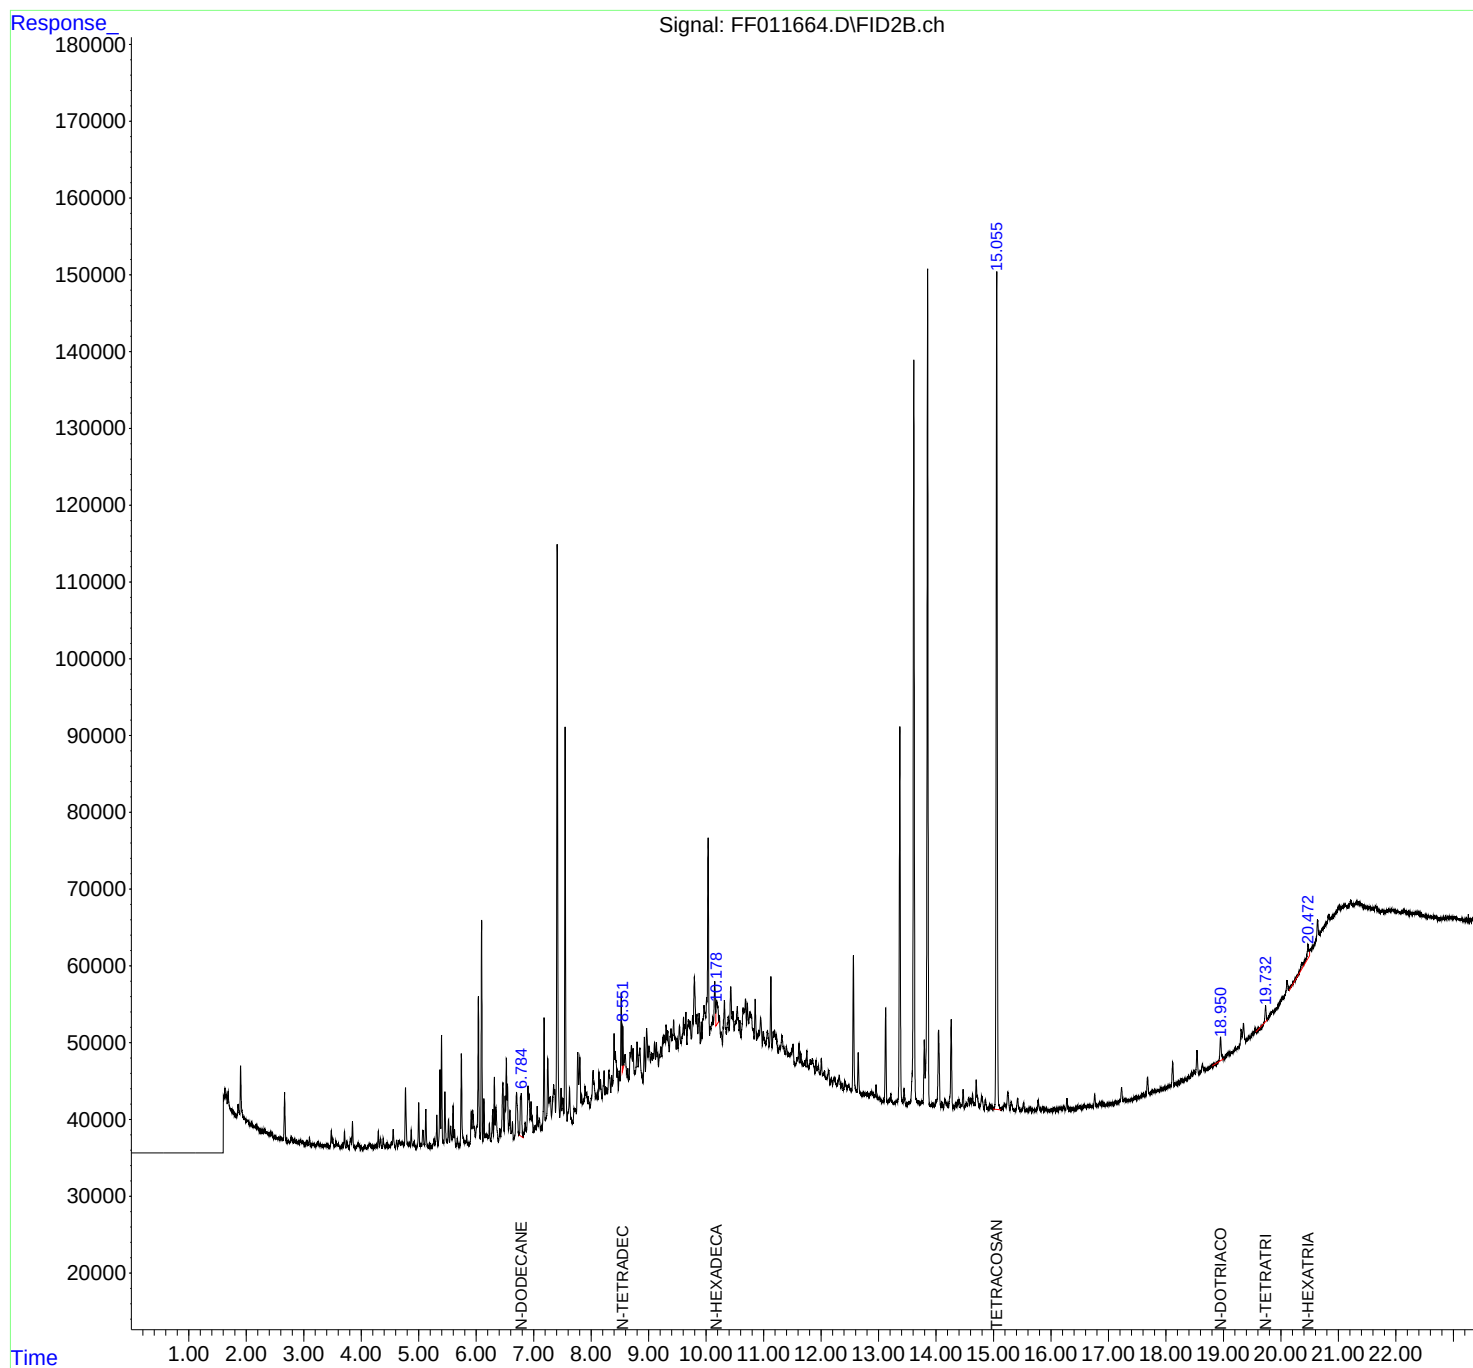


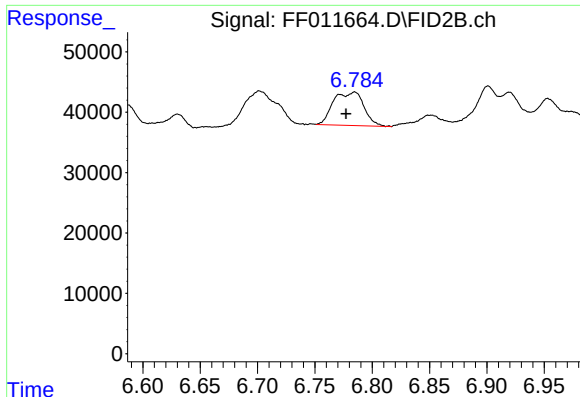

#3 N-DODECANE


R.T.: 6.785 min
Delta R.T.: 0.008 min
Response: 102674
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :
CAC-HPT-3-GW-(14-17)

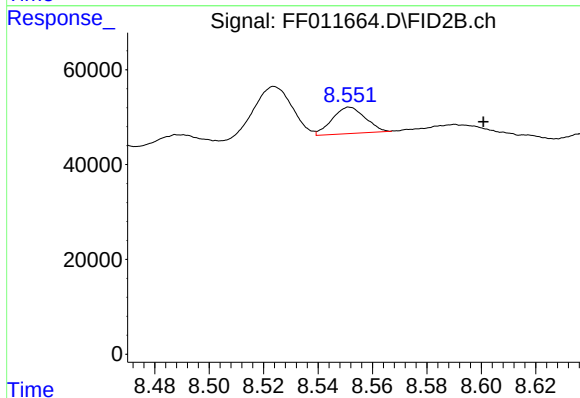


#4 N-TETRADECANE

R.T.: 8.552 min
Delta R.T.: -0.049 min
Response: 47101
Conc: 0.35 ug/ml

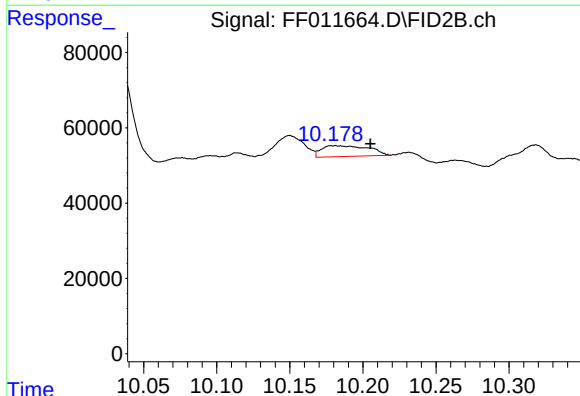


#5 N-HEXADECANE

R.T.: 10.181 min
Delta R.T.: -0.025 min
Response: 64220
Conc: 0.47 ug/ml

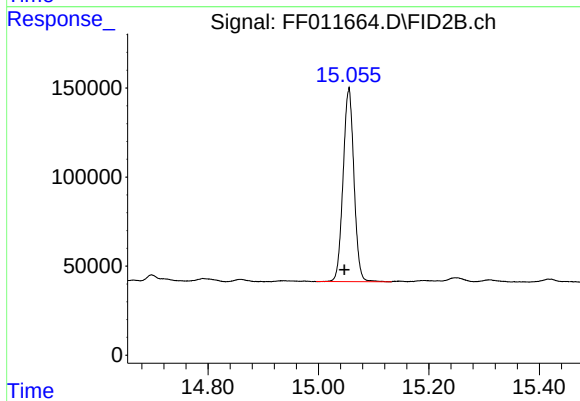

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.055 min
Delta R.T.: 0.008 min
Response: 1483893
Conc: 12.51 ug/ml

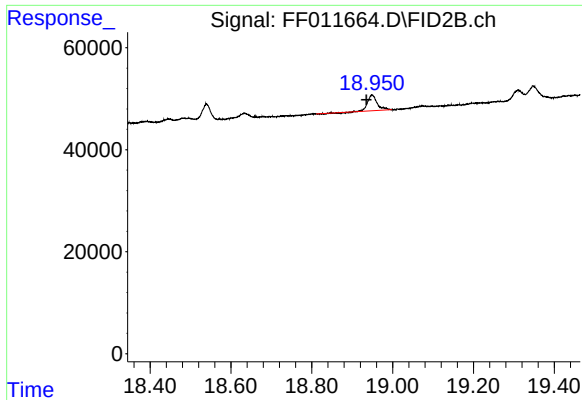

#14 N-DOTRIACONTANE


R.T.: 18.949 min
Delta R.T.: 0.014 min
Response: 48638
Conc: 0.36 ug/ml

Instrument :
FID_F
ClientSampleId :
CAC-HPT-3-GW-(14-17)

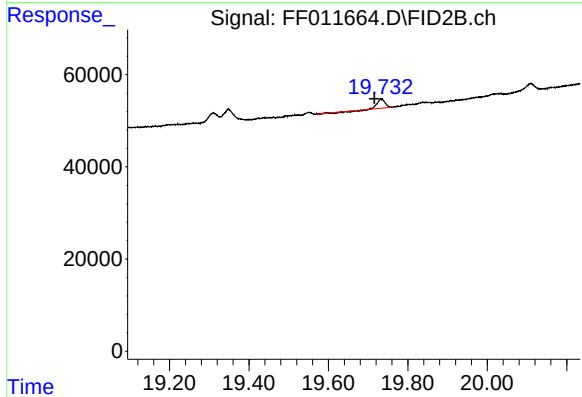

#15 N-TETRATRIACONTANE

R.T.: 19.733 min
Delta R.T.: 0.017 min
Response: 22913
Conc: 0.17 ug/ml

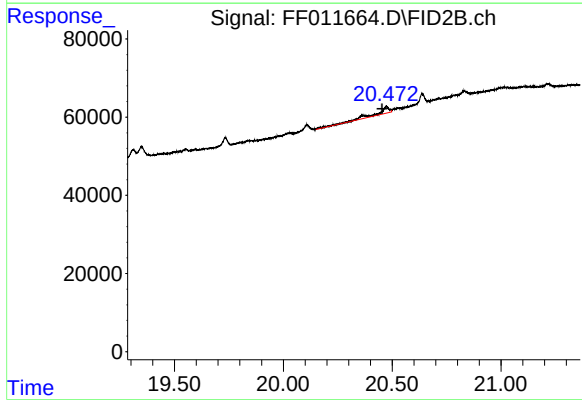

#16 N-HEXATRIACONTANE

R.T.: 20.474 min
Delta R.T.: 0.020 min
Response: 69143
Conc: 0.56 ug/ml