

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011672.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 08:10
Operator : YP\AJ
Sample : N5578-21
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAC-HPT-5-GW-(21-24)

Integration File: autoint1.e
Quant Time: Nov 14 02:28:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	1610000	13.570 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011672.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 08:10
Operator : YP\AJ
Sample : N5578-21
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAC-HPT-5-GW-(21-24)

Integration File: autoint1.e
Quant Time: Nov 14 02:28:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

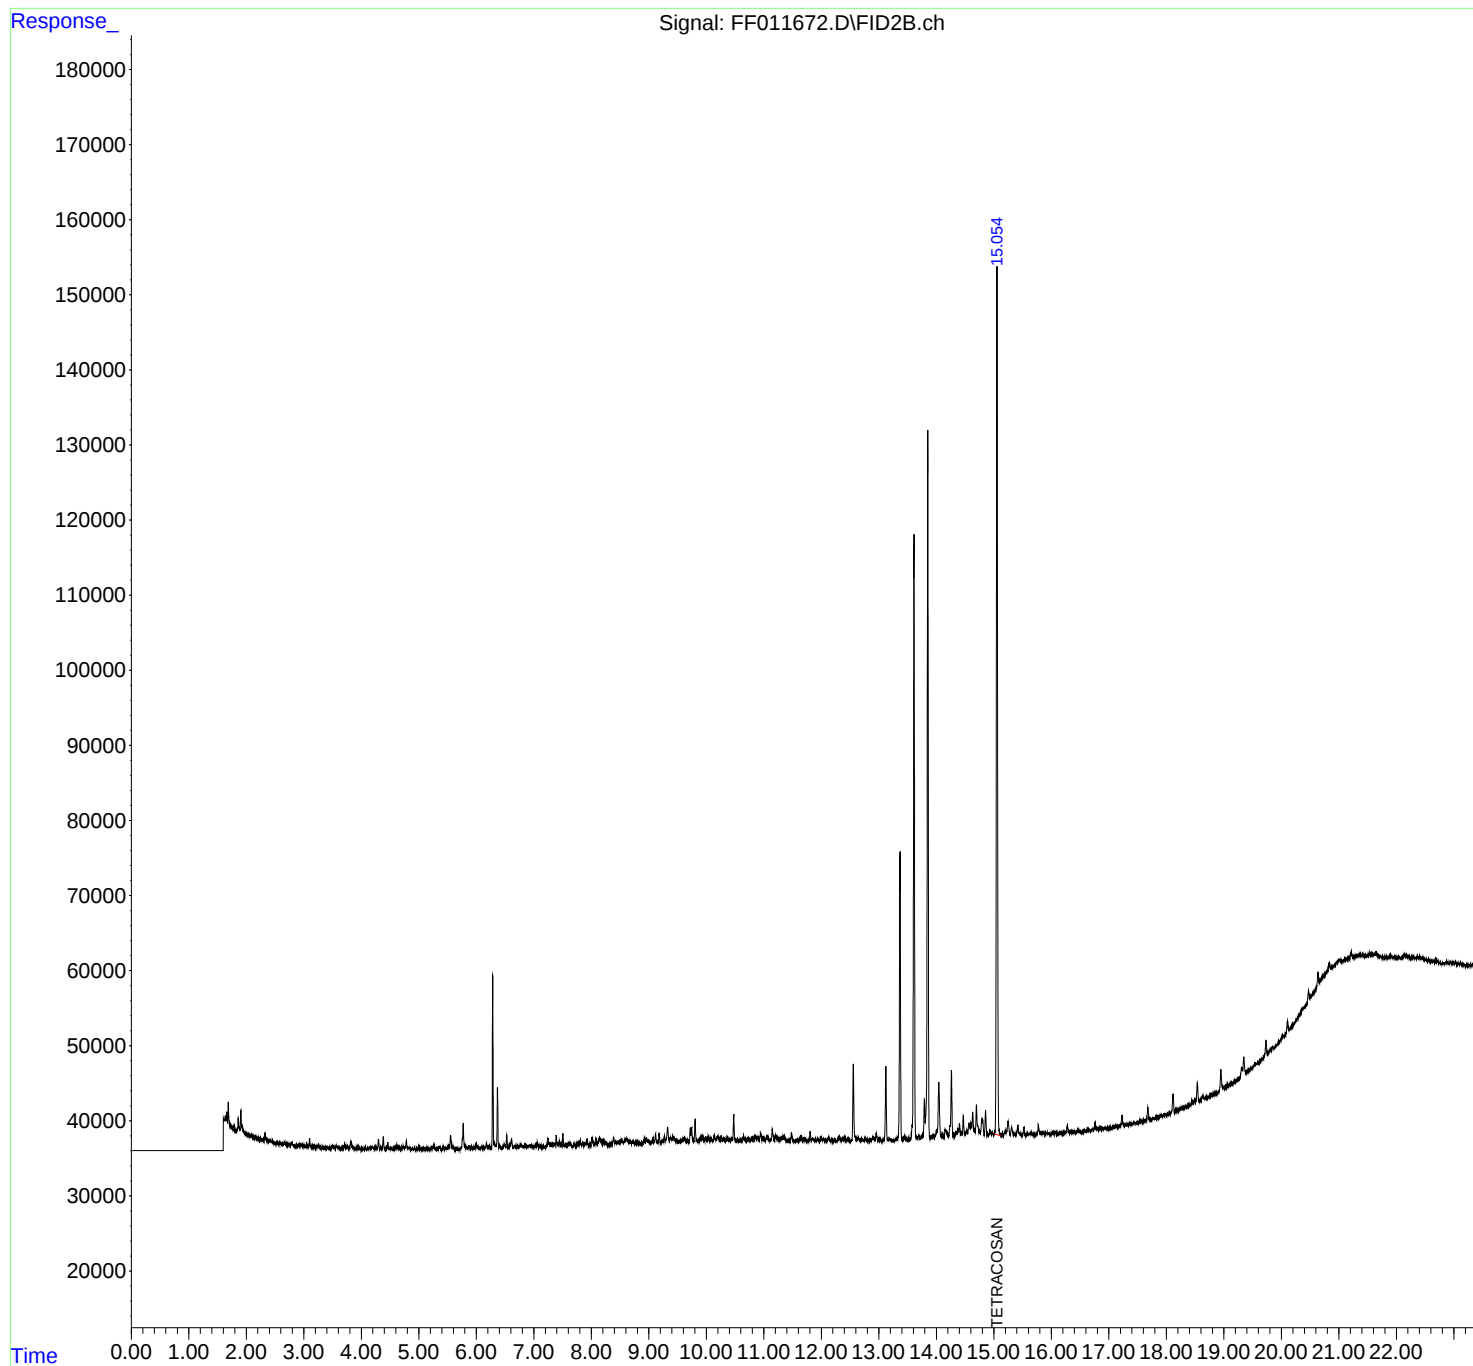

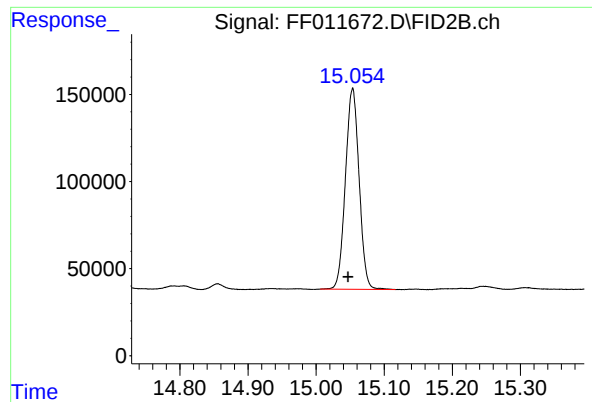

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.054 min
Delta R.T.: 0.007 min
Response: 1610000
Conc: 13.57 ug/ml

Instrument :

FID_F

ClientSampleId :

CAC-HPT-5-GW-(21-24)