

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011679.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 14:38
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 02:30:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.773	3092716	23.011 ug/ml
12) N-OCTACOSANE	17.229	2771699	20.922 ug/ml
14) N-DOTRIACONTANE	18.949	47536	0.353 ug/ml
15) N-TETRATRIACONTANE	19.732	45896	0.348 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011679.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 14:38
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 02:30:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

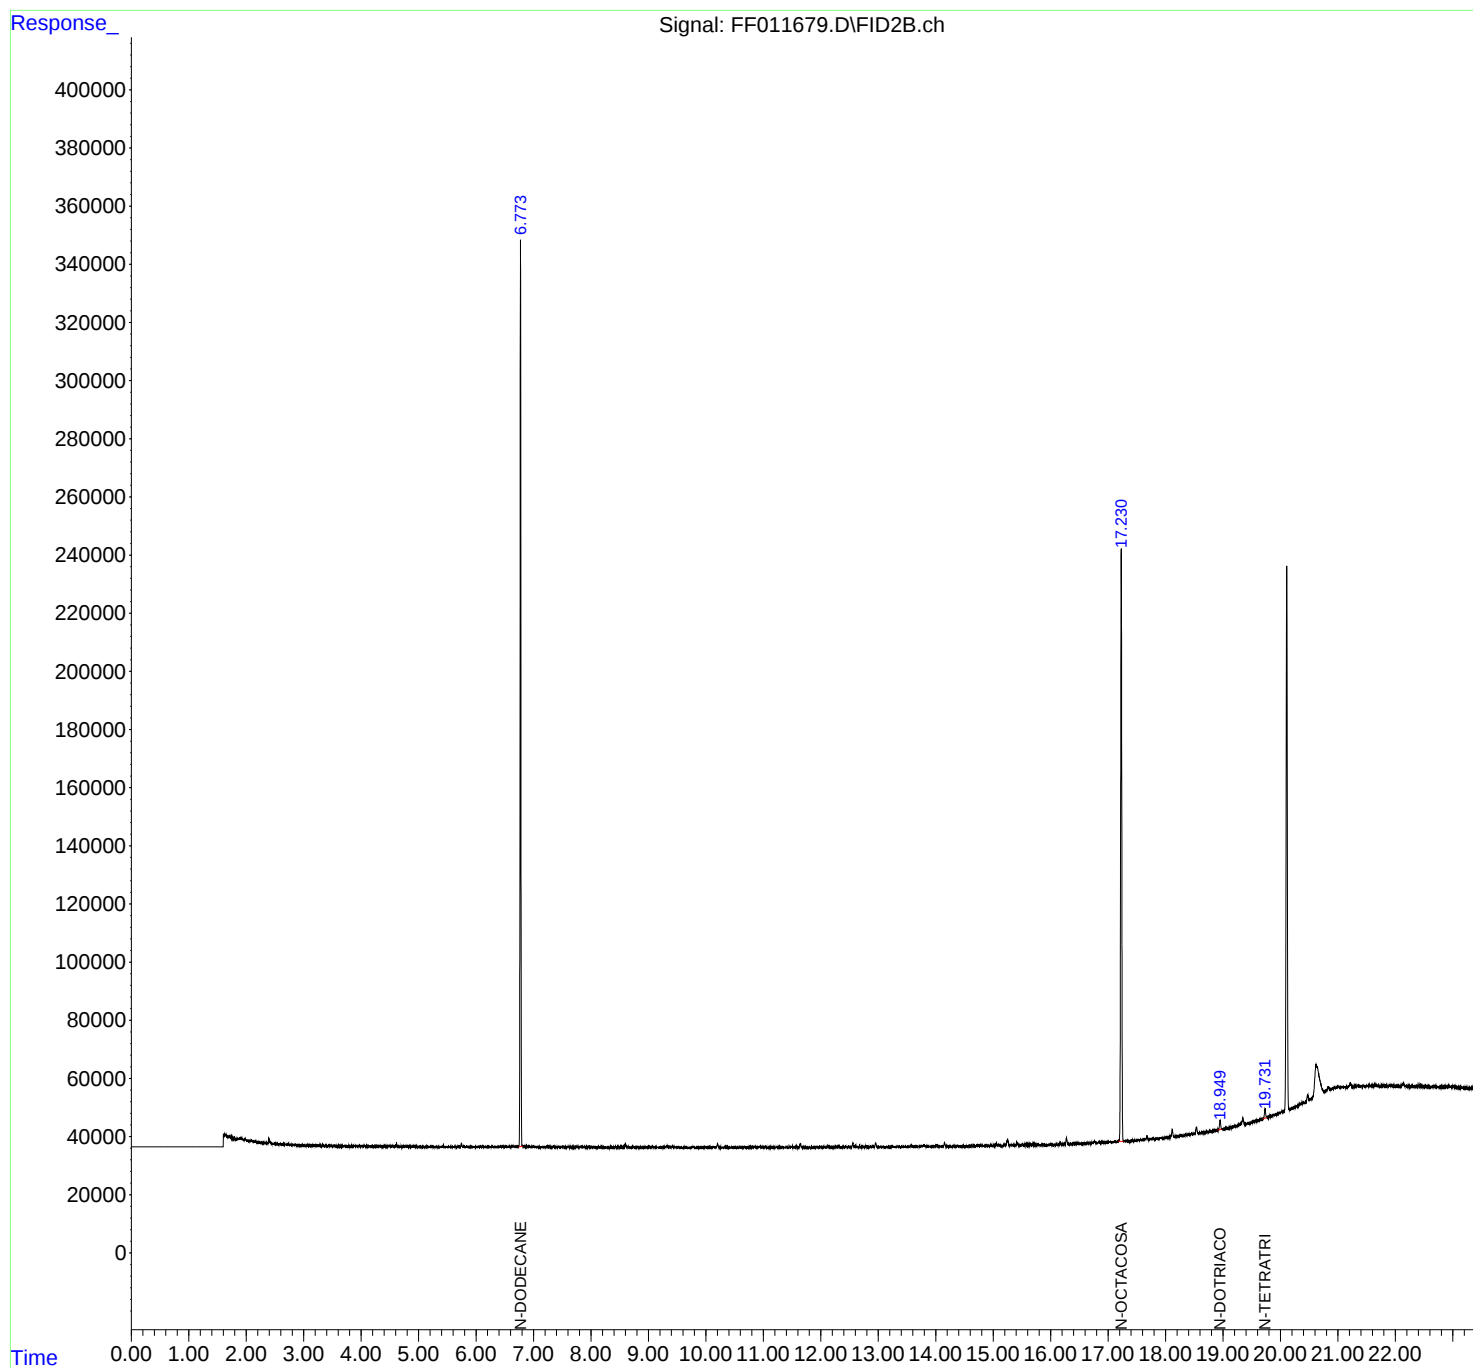


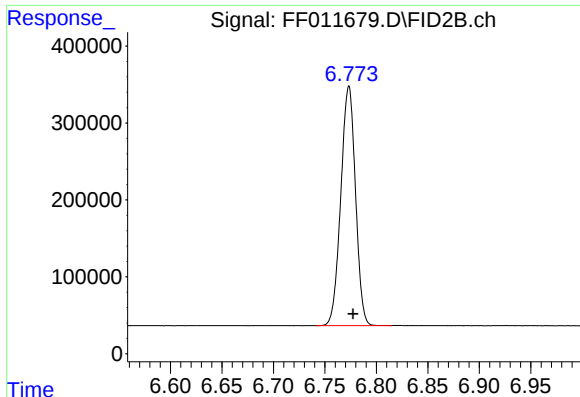

#3 N-DODECANE


R.T.: 6.773 min
Delta R.T.: -0.004 min
Response: 3092716
Conc: 23.01 ug/ml

Instrument :
FID_F
ClientSampleId :

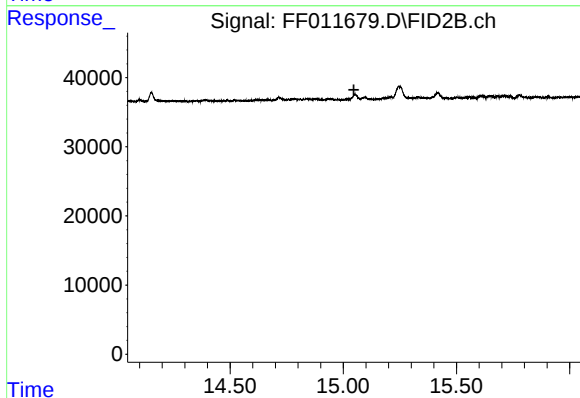


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.047 min
Response: 0
Conc: N.D.

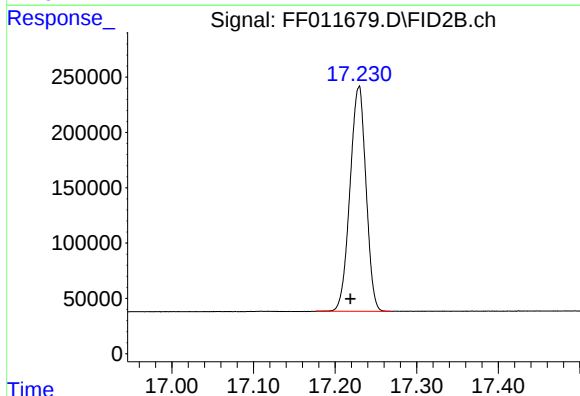


#12 N-OCTACOSANE

R.T.: 17.229 min
Delta R.T.: 0.011 min
Response: 2771699
Conc: 20.92 ug/ml

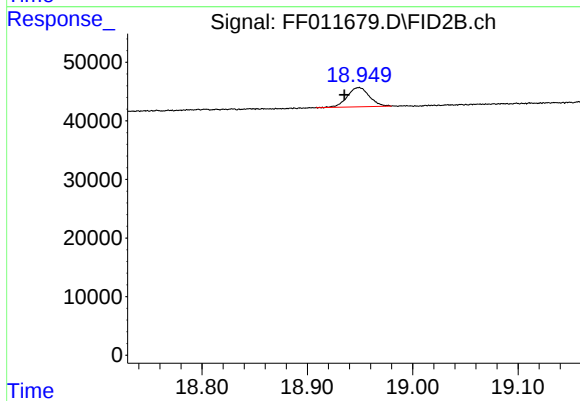

#14 N-DOTRIACONTANE

R.T.: 18.949 min
Delta R.T.: 0.014 min
Response: 47536
Conc: 0.35 ug/ml

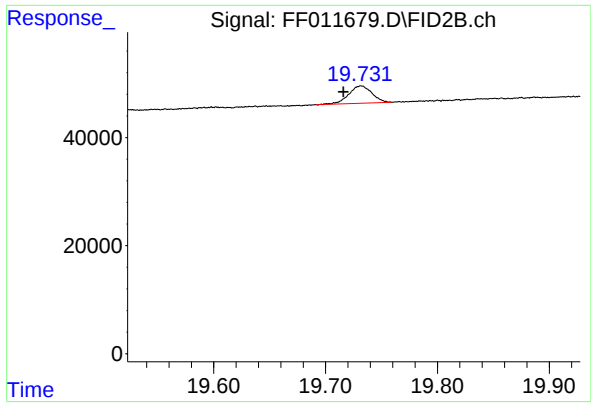

#15 N-TETRATRIACONTANE

R.T.: 19.732 min

Delta R.T.: 0.016 min

Response: 45896

Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :