

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011642.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2022 12:45
Operator : YP\AJ
Sample : N5317-15 20X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PT-DIES-SOIL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2022
Supervised By :Ankita Jodhani 11/14/2022

Integration File: Sample.e
Quant Time: Nov 14 02:23:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.056	97764	0.824 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011642.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2022 12:45
Operator : YP\AJ
Sample : N5317-15 20X
Misc :
ALS Vial : 58 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
PT-DIES-SOIL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2022
Supervised By :Ankita Jodhani 11/14/2022

Integration File: Sample.e
Quant Time: Nov 14 02:23:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

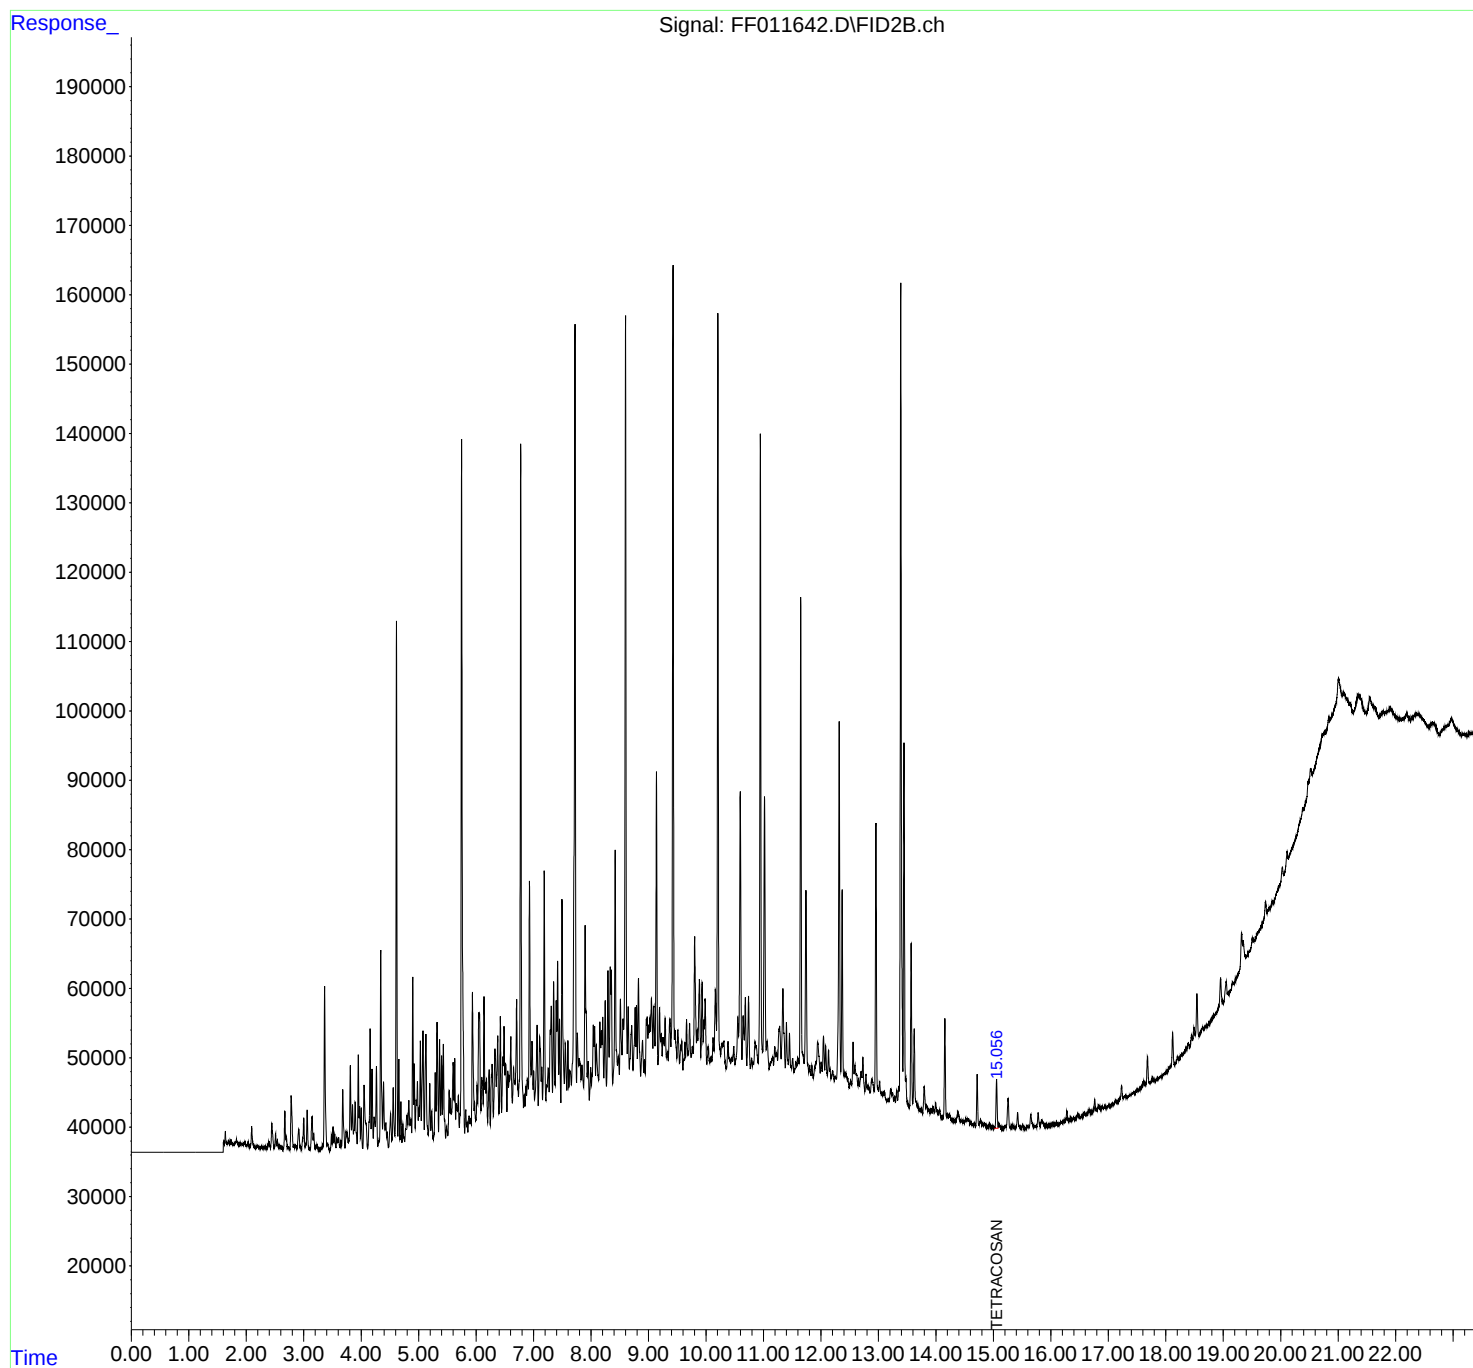

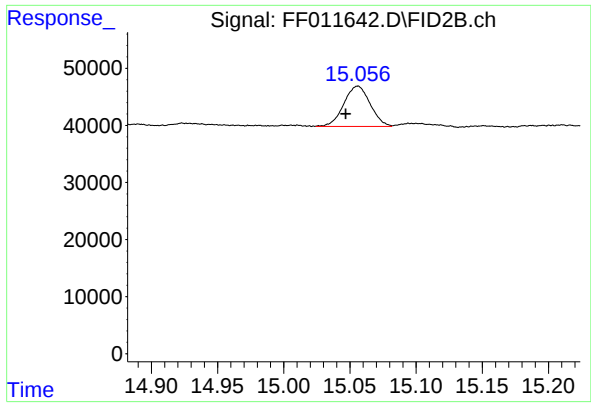

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.056 min
Delta R.T.: 0.009 min
Response: 97764
Conc: 0.82 ug/ml

Instrument :

FID_F

ClientSampleId :

PT-DIES-SOIL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/14/2022

Supervised By :Ankita Jodhani 11/14/2022