

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011665.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 03:11
Operator : YP\AJ
Sample : N5578-16
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAC-HPT-3-GW-(20-23)

Integration File: Sample.e
Quant Time: Nov 14 02:27:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.055	1916894	16.157 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011665.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 03:11
Operator : YP\AJ
Sample : N5578-16
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAC-HPT-3-GW-(20-23)

Integration File: Sample.e
Quant Time: Nov 14 02:27:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

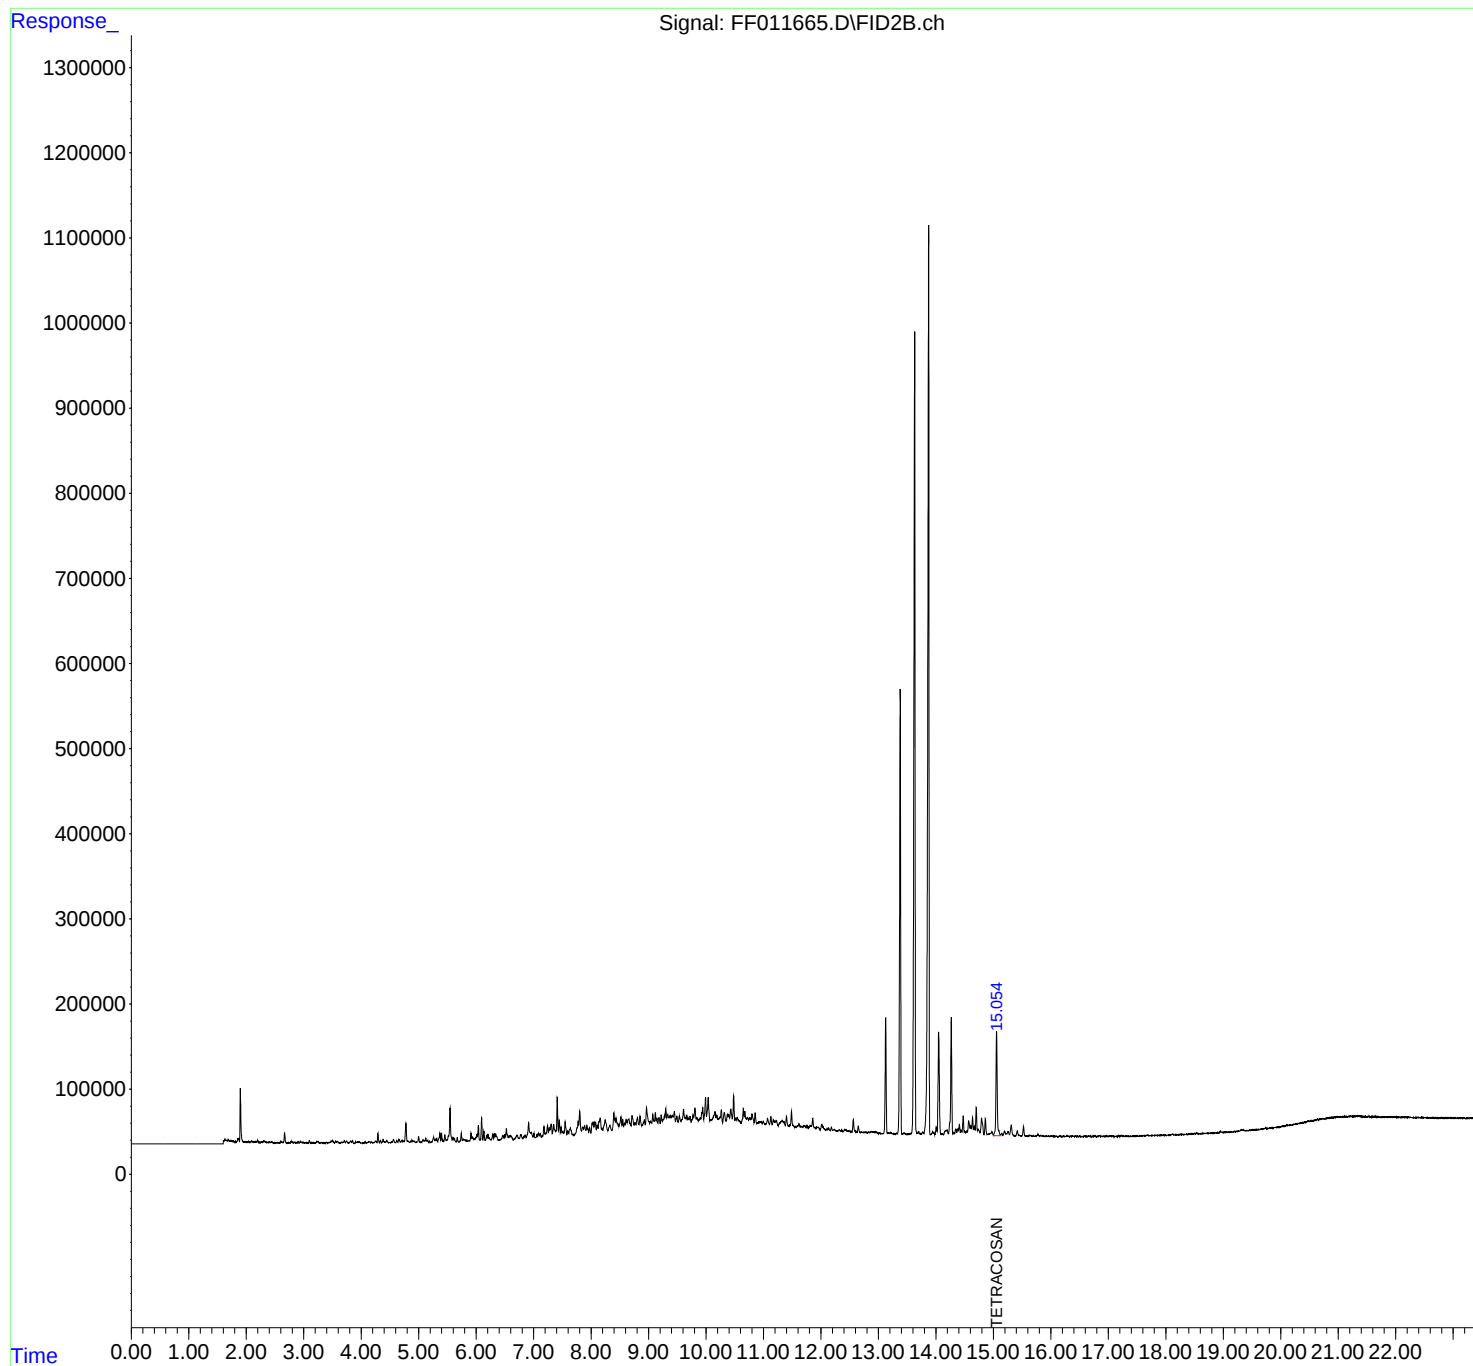

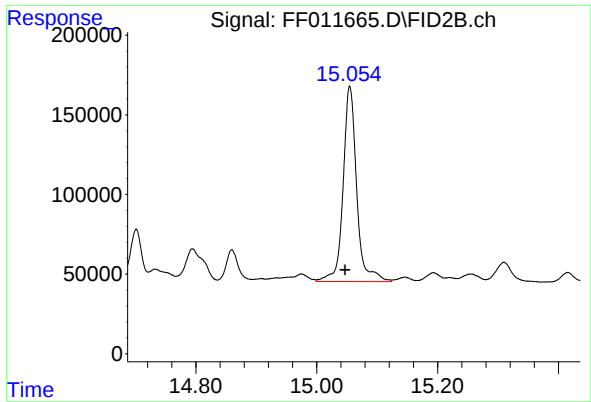

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.055 min
Delta R.T.: 0.008 min
Response: 1916894
Conc: 16.16 ug/ml

Instrument :
FID_F
ClientSampleId :
CAC-HPT-3-GW-(20-23)