

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011666.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 03:41
Operator : YP\AJ
Sample : N5578-17
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAC-HPT-3-GW-(26-29)

Integration File: Sample.e
Quant Time: Nov 14 02:27:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	1429932	12.052 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111122\
Data File : FF011666.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2022 03:41
Operator : YP\AJ
Sample : N5578-17
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CAC-HPT-3-GW-(26-29)

Integration File: Sample.e
Quant Time: Nov 14 02:27:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

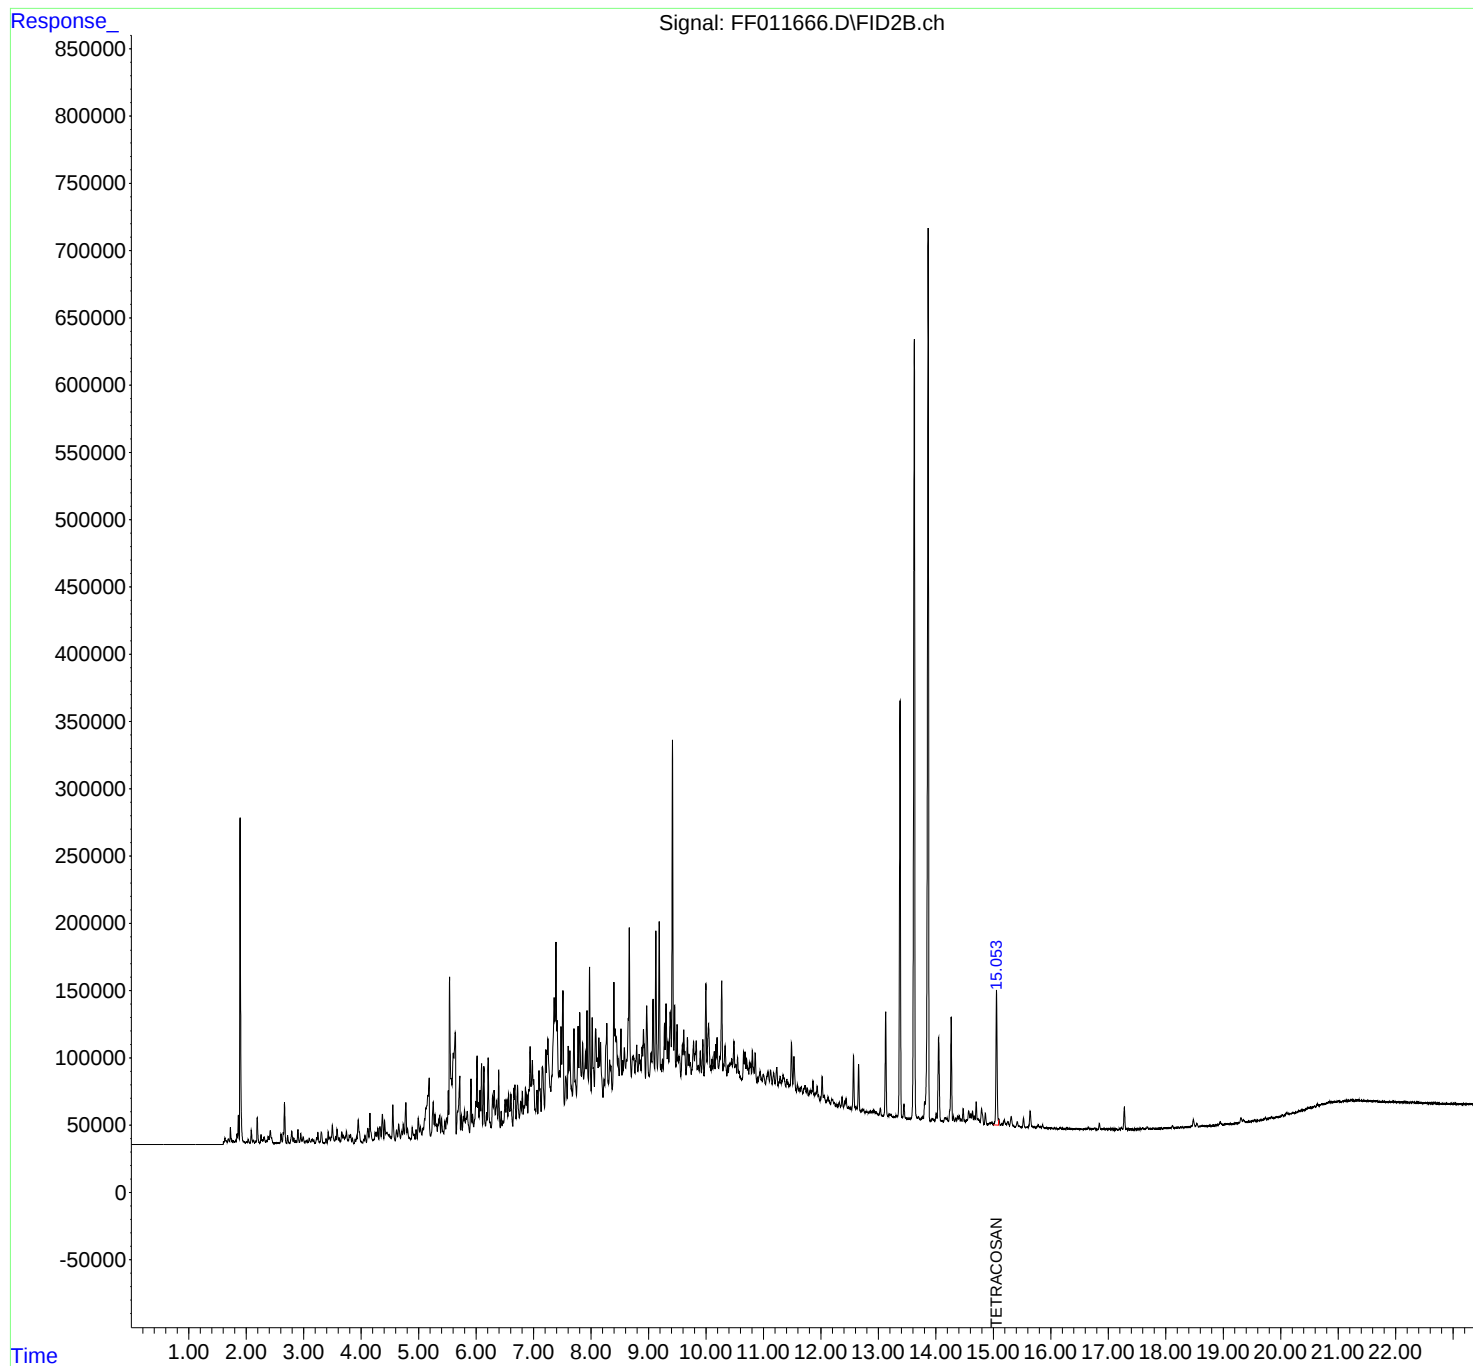

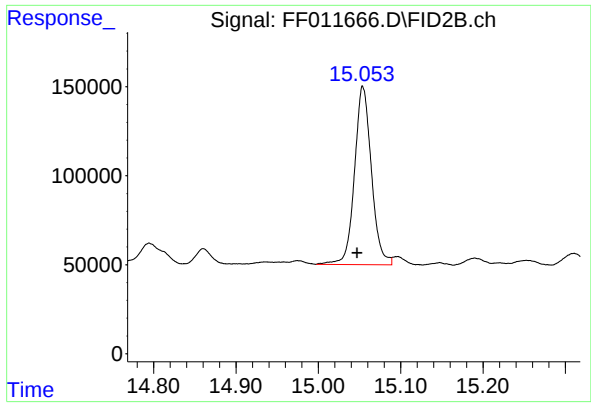

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.054 min
Delta R.T.: 0.007 min
Response: 1429932
Conc: 12.05 ug/ml

Instrument :
FID_F
ClientSampleId :
CAC-HPT-3-GW-(26-29)