

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111125\
Data File : FF016646.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2025 11:31
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 00:16:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.751	3071170	27.647 ug/ml
12)	N-OCTACOSANE	17.245	2941399	25.812 ug/ml
14)	N-DOTRIACONTANE	18.970	47302	0.441 ug/ml
15)	N-TETRATRIACONTANE	19.759	47859	0.487 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111125\
Data File : FF016646.D
Signal(s) : FID2B.ch
Acq On : 11 Nov 2025 11:31
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 00:16:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

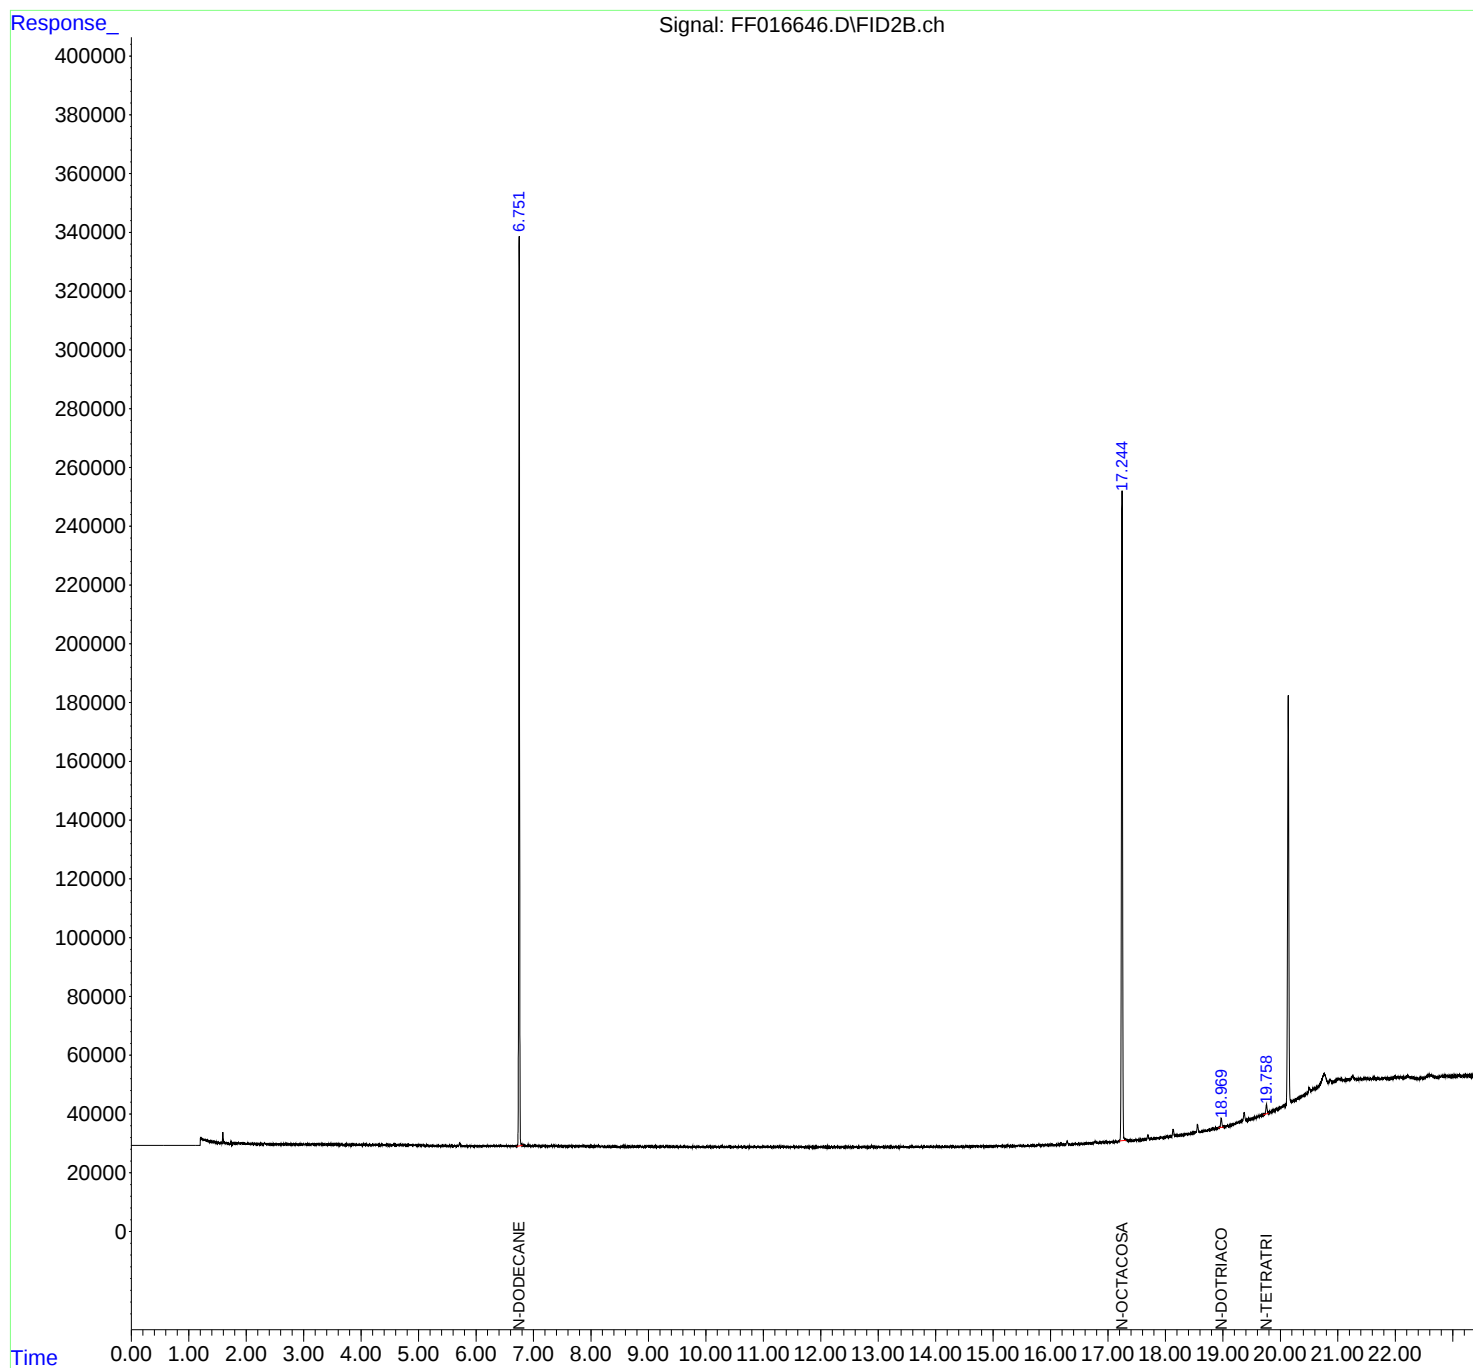


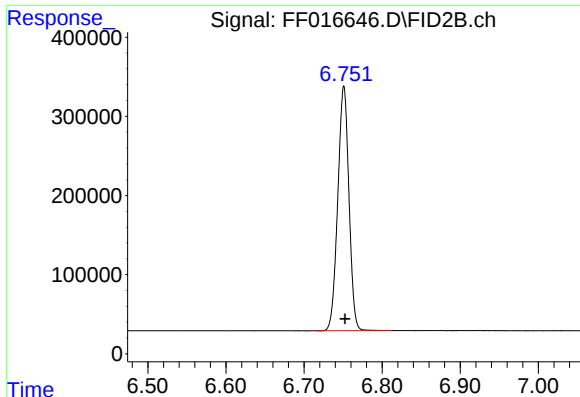

#3 N-DODECANE


R.T.: 6.751 min
Delta R.T.: -0.001 min
Response: 3071170
Conc: 27.65 ug/ml

Instrument :
FID_F
ClientSampleId :

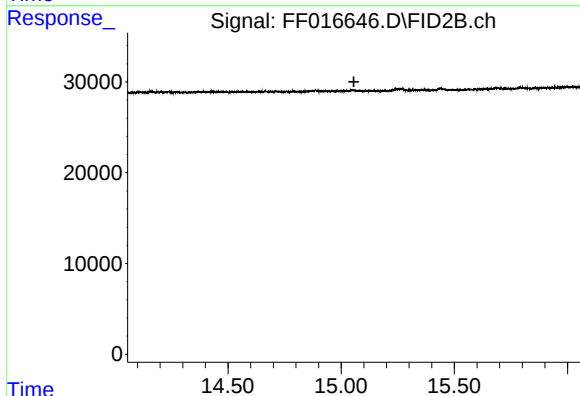


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.056 min
Response: 0
Conc: N.D.

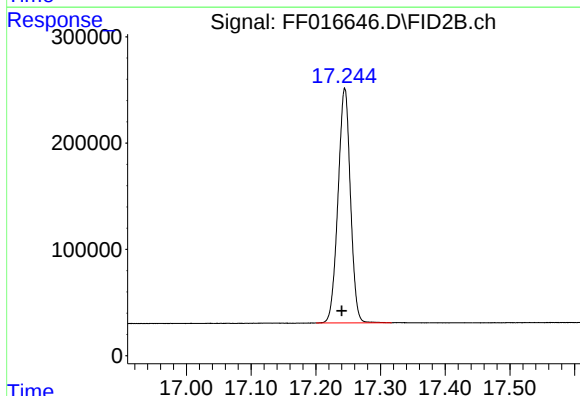


#12 N-OCTACOSANE

R.T.: 17.245 min
Delta R.T.: 0.005 min
Response: 2941399
Conc: 25.81 ug/ml

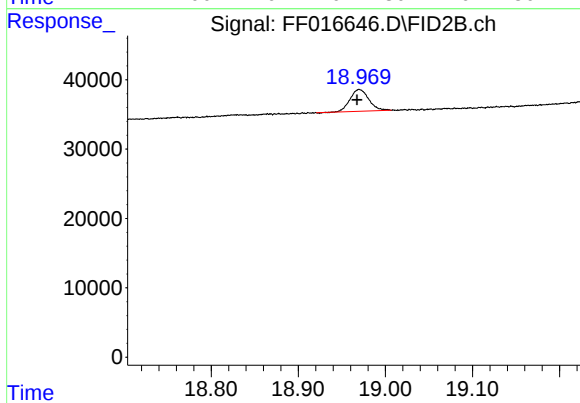

#14 N-DOTRIACONTANE

R.T.: 18.970 min
Delta R.T.: 0.003 min
Response: 47302
Conc: 0.44 ug/ml

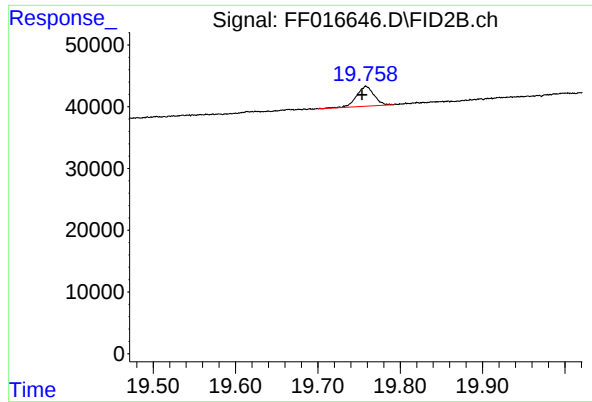

#15 N-TETRATRIACONTANE

R.T.: 19.759 min
Delta R.T.: 0.005 min
Response: 47859
Conc: 0.49 ug/ml

Instrument :

FID_F

ClientSampleId :