

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
 Data File : FF007873.D
 Signal(s) : FID2B.ch
 Acq On : 12 Nov 2020 11:34
 Operator : DD\AJ
 Sample : L4631-03 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 13 00:48:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.716	951489	7.449 ug/ml
Target Compounds			
4) N-TETRADECANE	8.318 ^f	211080	1.495 ug/ml
7) N-EICOSANE	12.612	137699	0.929 ug/ml
8) N-DOCOSANE	13.818	177881	1.221 ug/ml
10) N-TETRACOSANE	14.911	421234	2.913 ug/ml
11) N-HEXACOSANE	15.946	164091	1.169 ug/ml
12) N-OCTACOSANE	16.897	306651	2.261 ug/ml
13) N-TRIACONTANE	17.795	706533	5.460 ug/ml
14) N-DOTRIACONTANE	18.621	565703	4.880 ug/ml
15) N-TETRATRIACONTANE	19.411	364194	3.877 ug/ml
16) N-HEXATRIACONTANE	20.158	624123	8.217 ug/ml
17) N-OCTATRIACONTANE	20.908	209514	3.372 ug/ml
18) N-TETRACONTANE	21.851	60576	0.993 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
Data File : FF007873.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2020 11:34
Operator : DD\AJ
Sample : L4631-03 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 13 00:48:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

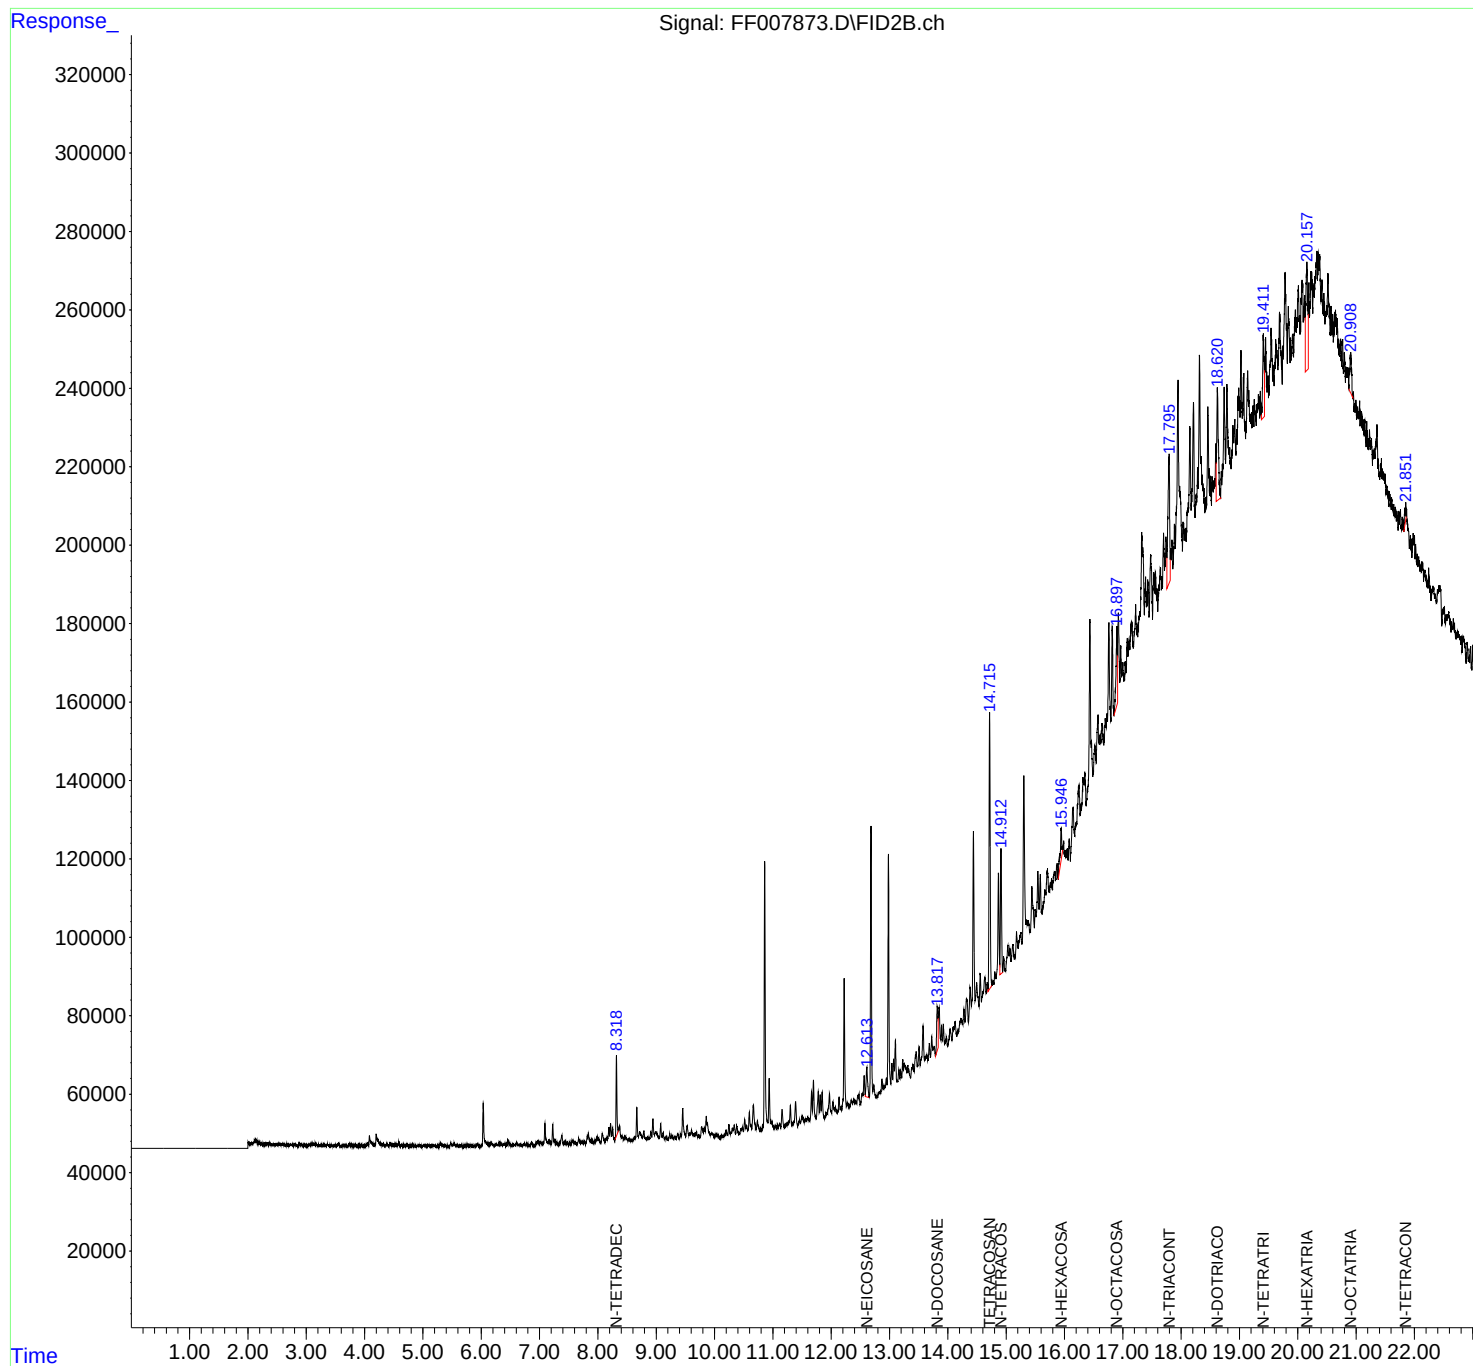


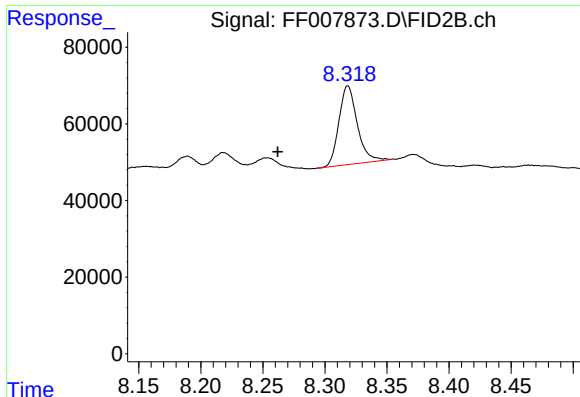

#4 N-TETRADECANE


R.T.: 8.318 min
Delta R.T.: 0.056 min
Response: 211080
Conc: 1.49 ug/ml

Instrument :
FID_F
ClientSampleId :

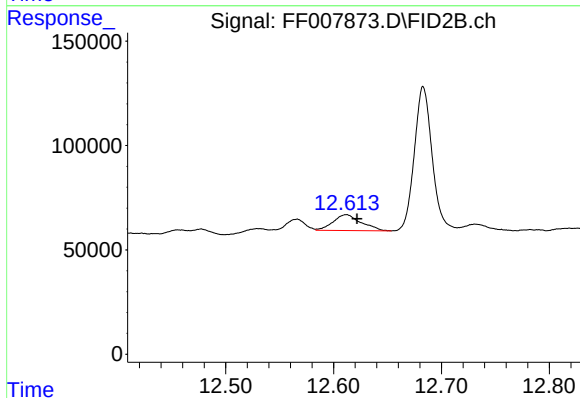


#7 N-EICOSANE

R.T.: 12.612 min
Delta R.T.: -0.010 min
Response: 137699
Conc: 0.93 ug/ml

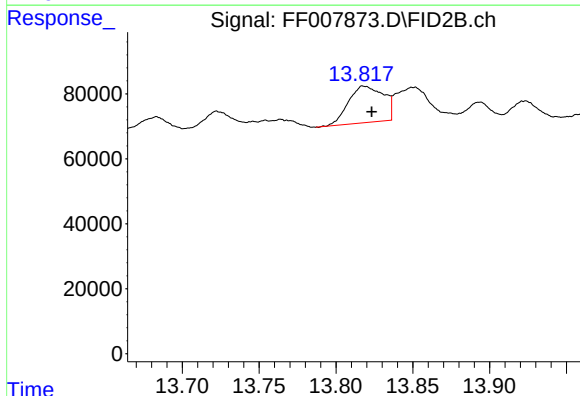


#8 N-DOCOSANE

R.T.: 13.818 min
Delta R.T.: -0.005 min
Response: 177881
Conc: 1.22 ug/ml

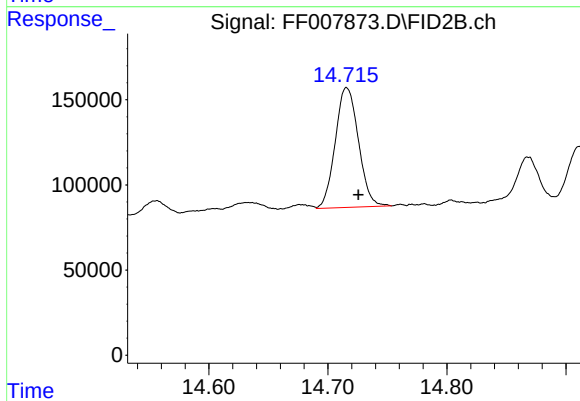

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.716 min
Delta R.T.: -0.010 min
Response: 951489
Conc: 7.45 ug/ml

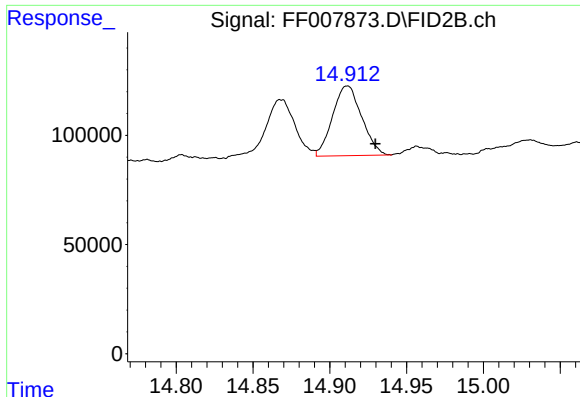

#10 N-TETRACOSANE


R.T.: 14.911 min
Delta R.T.: -0.018 min
Response: 421234
Conc: 2.91 ug/ml

Instrument :
FID_F
ClientSampleId :

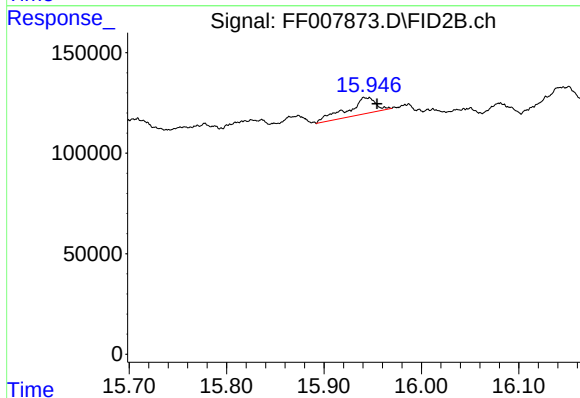


#11 N-HEXACOSANE

R.T.: 15.946 min
Delta R.T.: -0.008 min
Response: 164091
Conc: 1.17 ug/ml

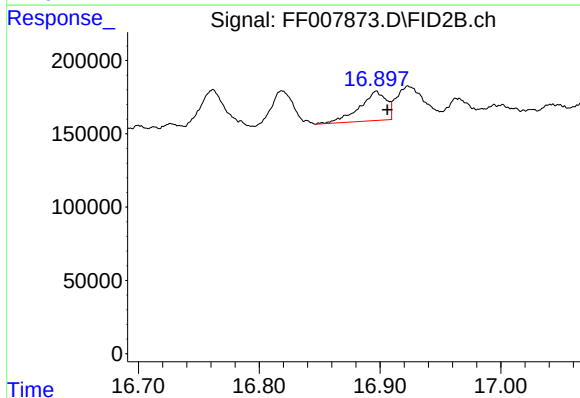


#12 N-OCTACOSANE

R.T.: 16.897 min
Delta R.T.: -0.009 min
Response: 306651
Conc: 2.26 ug/ml

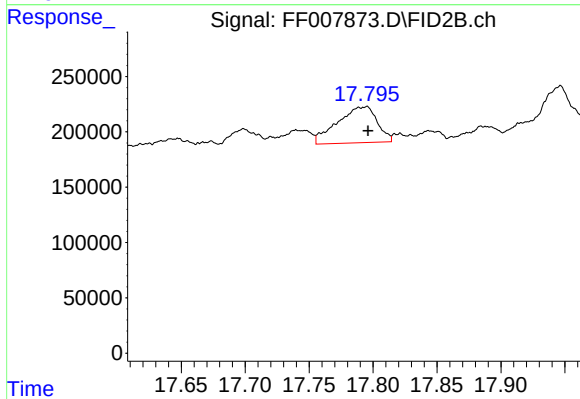

#13 N-TRIACONTANE


R.T.: 17.795 min
Delta R.T.: -0.001 min
Response: 706533
Conc: 5.46 ug/ml

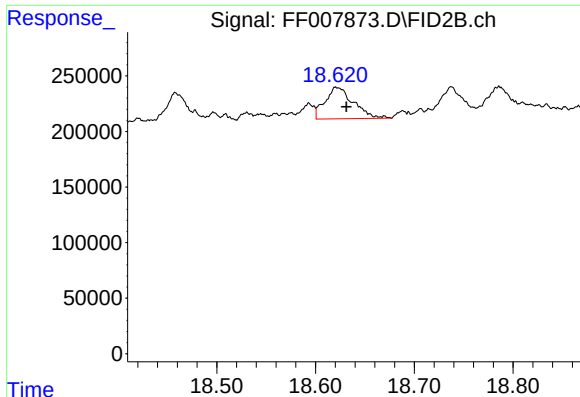

#14 N-DOTRIACONTANE


R.T.: 18.621 min
Delta R.T.: -0.010 min
Response: 565703
Conc: 4.88 ug/ml

Instrument :
FID_F
ClientSampleId :

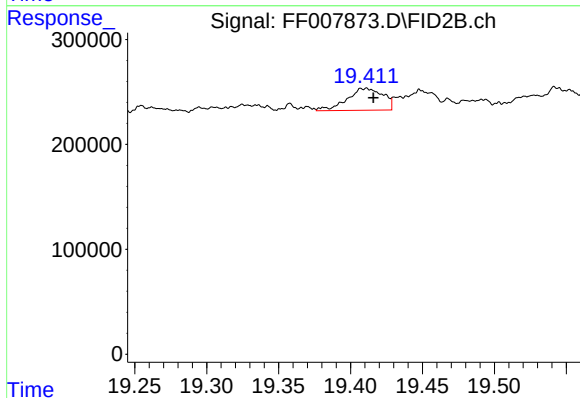


#15 N-TETRATRIACONTANE

R.T.: 19.411 min
Delta R.T.: -0.005 min
Response: 364194
Conc: 3.88 ug/ml

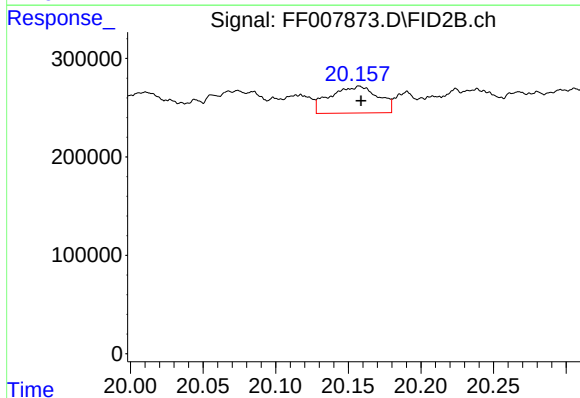


#16 N-HEXATRIACONTANE

R.T.: 20.158 min
Delta R.T.: 0.000 min
Response: 624123
Conc: 8.22 ug/ml

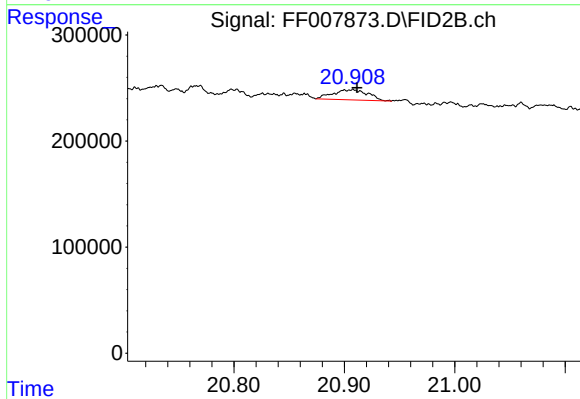

#17 N-OCTATRIACONTANE

R.T.: 20.908 min
Delta R.T.: -0.004 min
Response: 209514
Conc: 3.37 ug/ml

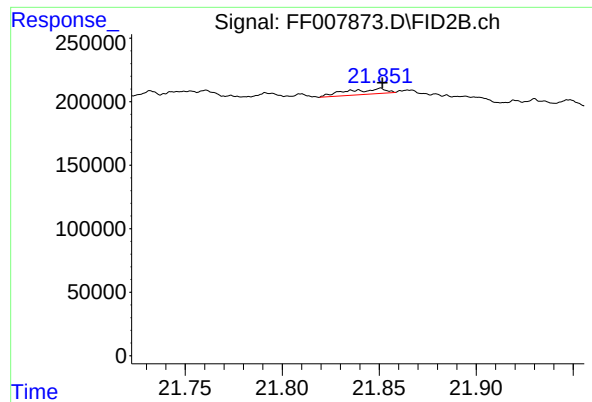

#18 N-TETRACONTANE

R.T.: 21.851 min
Delta R.T.: -0.001 min
Response: 60576
Conc: 0.99 ug/ml

Instrument :
FID_F
ClientSampleId :