

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
 Data File : FF007875.D
 Signal(s) : FID2B.ch
 Acq On : 12 Nov 2020 12:35
 Operator : DD\AJ
 Sample : L4702-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 13 00:48:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.721	3399999	26.618 ug/ml
Target Compounds			
4) N-TETRADECANE	8.256	1319266	9.342 ug/ml
5) N-HEXADECANE	9.859	1149704	7.911 ug/ml
6) N-OCTADECANE	11.303	434287	2.926 ug/ml
7) N-EICOSANE	12.613	616688	4.160 ug/ml
8) N-DOCOSANE	13.821	679510	4.664 ug/ml
10) N-TETRACOSANE	14.926	6607713	45.693 ug/ml
11) N-HEXACOSANE	15.925	1406470	10.021 ug/ml
12) N-OCTACOSANE	16.898	843915	6.222 ug/ml
13) N-TRIACONTANE	17.794	2706919	20.921 ug/ml
14) N-DOTRIACONTANE	18.601	3590501	30.972 ug/ml
15) N-TETRATRIACONTANE	19.410	2306597	24.557 ug/ml
16) N-HEXATRIACONTANE	20.152	2362190	31.098 ug/ml
17) N-OCTATRIACONTANE	20.857f	734288	11.818 ug/ml
18) N-TETRACONTANE	21.859	655645	10.746 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
Data File : FF007875.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2020 12:35
Operator : DD\AJ
Sample : L4702-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 13 00:48:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

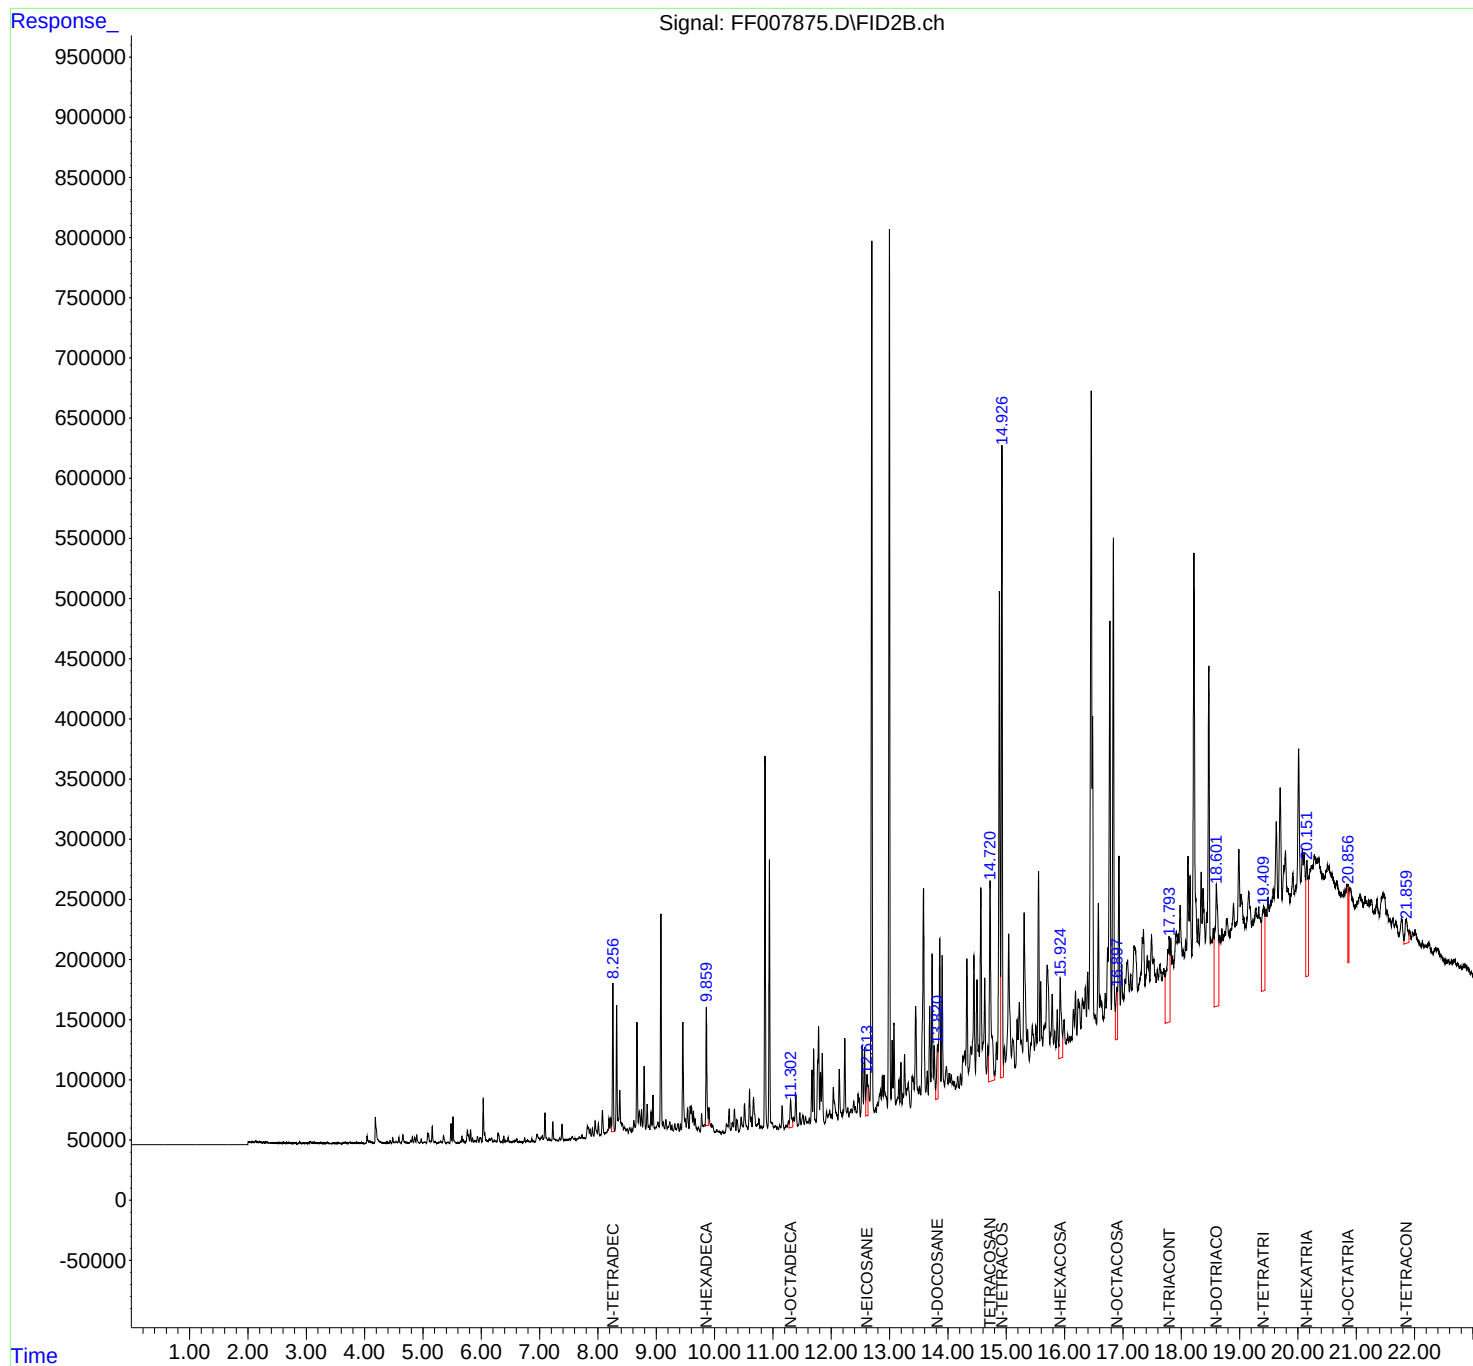


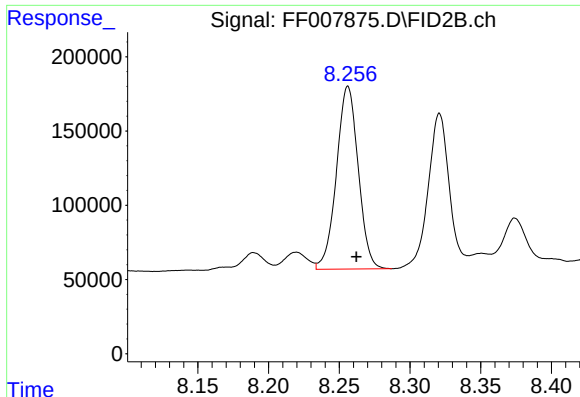

#4 N-TETRADECANE


R.T.: 8.256 min
Delta R.T.: -0.006 min
Response: 1319266
Conc: 9.34 ug/ml

Instrument :
FID_F
ClientSampleId :

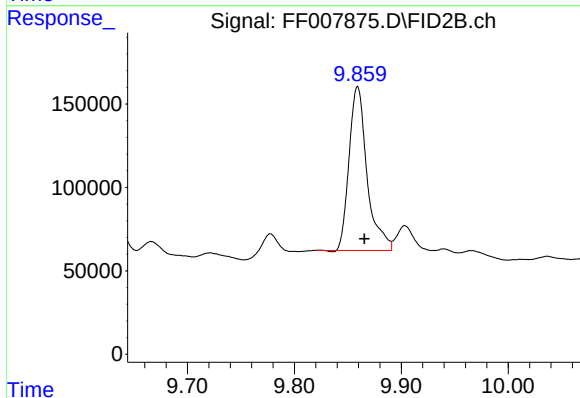


#5 N-HEXADECANE

R.T.: 9.859 min
Delta R.T.: -0.006 min
Response: 1149704
Conc: 7.91 ug/ml

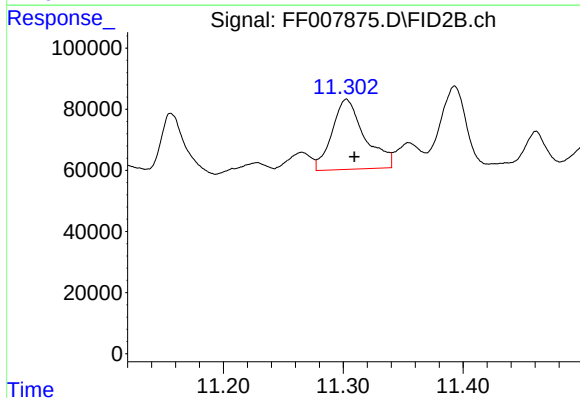


#6 N-OCTADECANE

R.T.: 11.303 min
Delta R.T.: -0.007 min
Response: 434287
Conc: 2.93 ug/ml

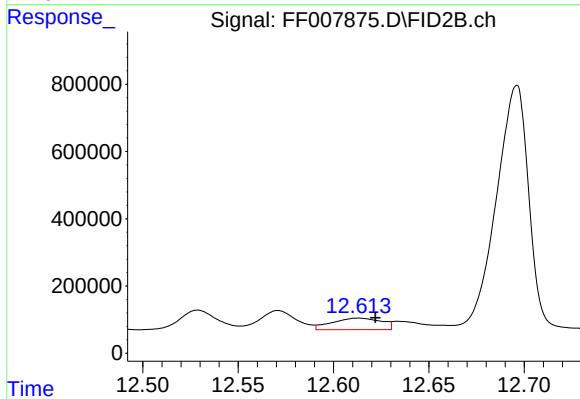

#7 N-EICOSANE


R.T.: 12.613 min
Delta R.T.: -0.009 min
Response: 616688
Conc: 4.16 ug/ml

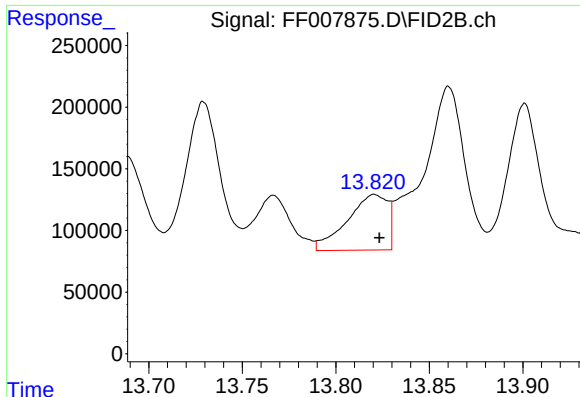

#8 N-DOCOSANE


R.T.: 13.821 min
Delta R.T.: -0.003 min
Response: 679510
Conc: 4.66 ug/ml

Instrument :
FID_F
ClientSampleId :

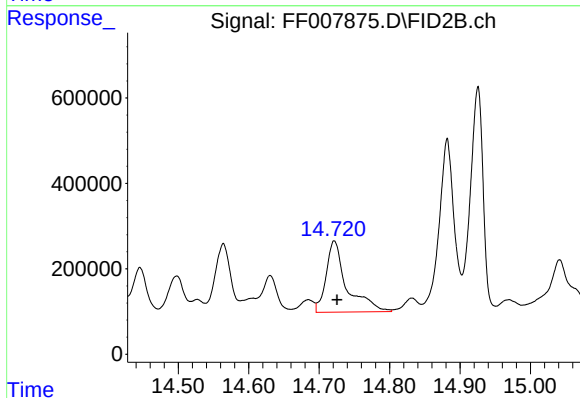


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.721 min
Delta R.T.: -0.004 min
Response: 3399999
Conc: 26.62 ug/ml

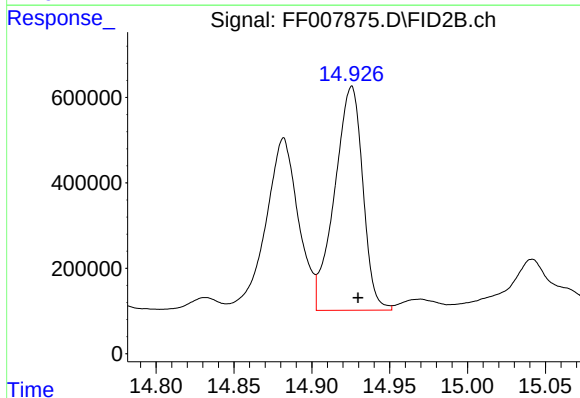


#10 N-TETRACOSANE

R.T.: 14.926 min
Delta R.T.: -0.004 min
Response: 6607713
Conc: 45.69 ug/ml

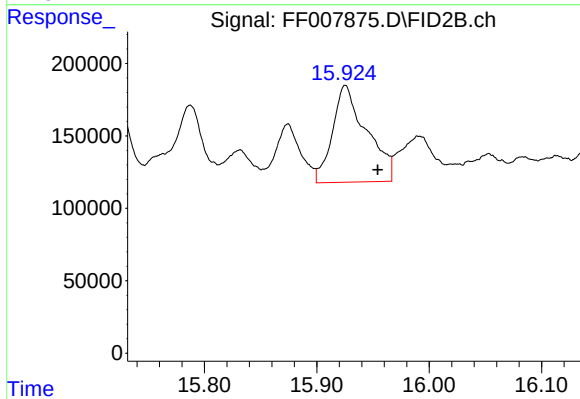

#11 N-HEXACOSANE


R.T.: 15.925 min
Delta R.T.: -0.029 min
Response: 1406470
Conc: 10.02 ug/ml

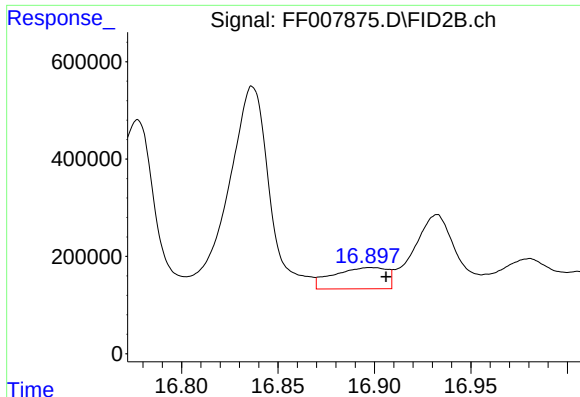

#12 N-OCTACOSANE


R.T.: 16.898 min
Delta R.T.: -0.008 min
Response: 843915
Conc: 6.22 ug/ml

Instrument :
FID_F
ClientSampleId :

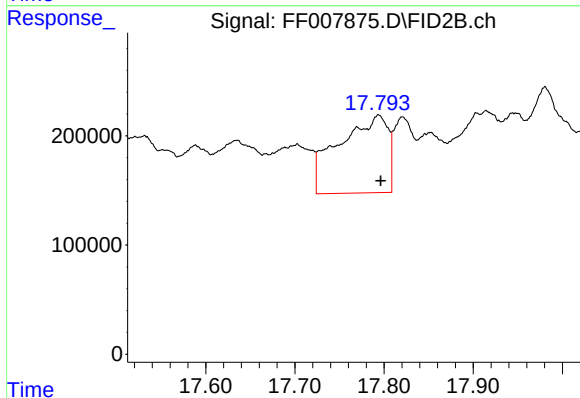


#13 N-TRIACONTANE

R.T.: 17.794 min
Delta R.T.: -0.002 min
Response: 2706919
Conc: 20.92 ug/ml

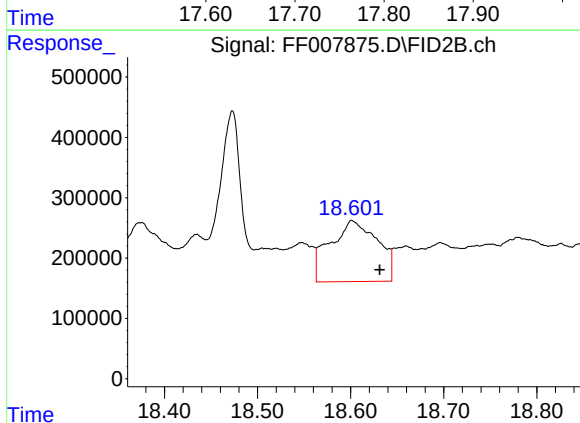


#14 N-DOTRIACONTANE

R.T.: 18.601 min
Delta R.T.: -0.030 min
Response: 3590501
Conc: 30.97 ug/ml

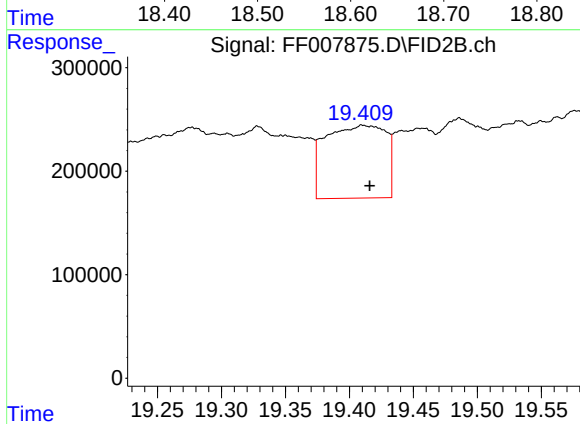

#15 N-TETRATRIACONTANE


R.T.: 19.410 min
Delta R.T.: -0.006 min
Response: 2306597
Conc: 24.56 ug/ml

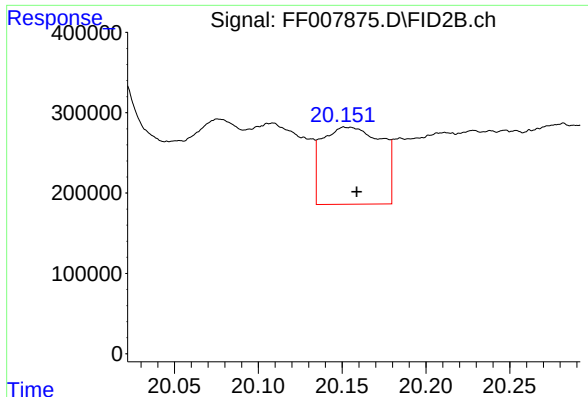

#16 N-HEXATRIACONTANE


R.T.: 20.152 min
Delta R.T.: -0.007 min
Response: 2362190
Conc: 31.10 ug/ml

Instrument :
FID_F
ClientSampleId :

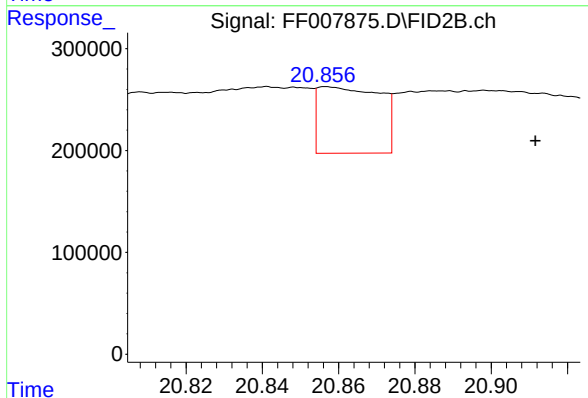

#17 N-OCTATRIACONTANE

R.T.: 20.857 min
Delta R.T.: -0.054 min
Response: 734288
Conc: 11.82 ug/ml

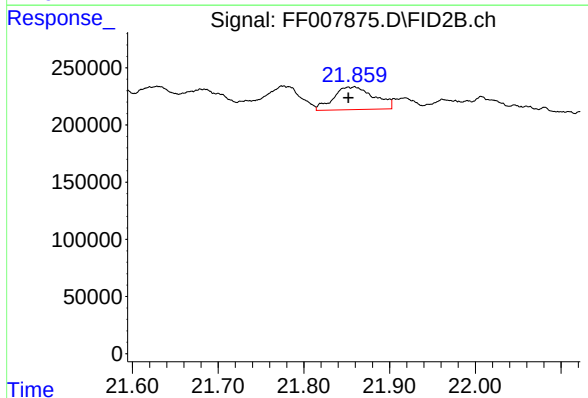

#18 N-TETRACONTANE

R.T.: 21.859 min
Delta R.T.: 0.007 min
Response: 655645
Conc: 10.75 ug/ml