

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
 Data File : FF007877.D
 Signal(s) : FID2B.ch
 Acq On : 12 Nov 2020 13:37
 Operator : DD\AJ
 Sample : L4715-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 13 00:49:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.720	2431299	19.034 ug/ml
Target Compounds			
4) N-TETRADECANE	8.225	91397	0.647 ug/ml
7) N-EICOSANE	12.688f	143939	0.971 ug/ml
10) N-TETRACOSANE	14.919	94175	0.651 ug/ml
13) N-TRIACONTANE	17.788	79669	0.616 ug/ml
14) N-DOTRIACONTANE	18.616	513342	4.428 ug/ml
16) N-HEXATRIACONTANE	20.150	129176	1.701 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
Data File : FF007877.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2020 13:37
Operator : DD\AJ
Sample : L4715-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 13 00:49:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

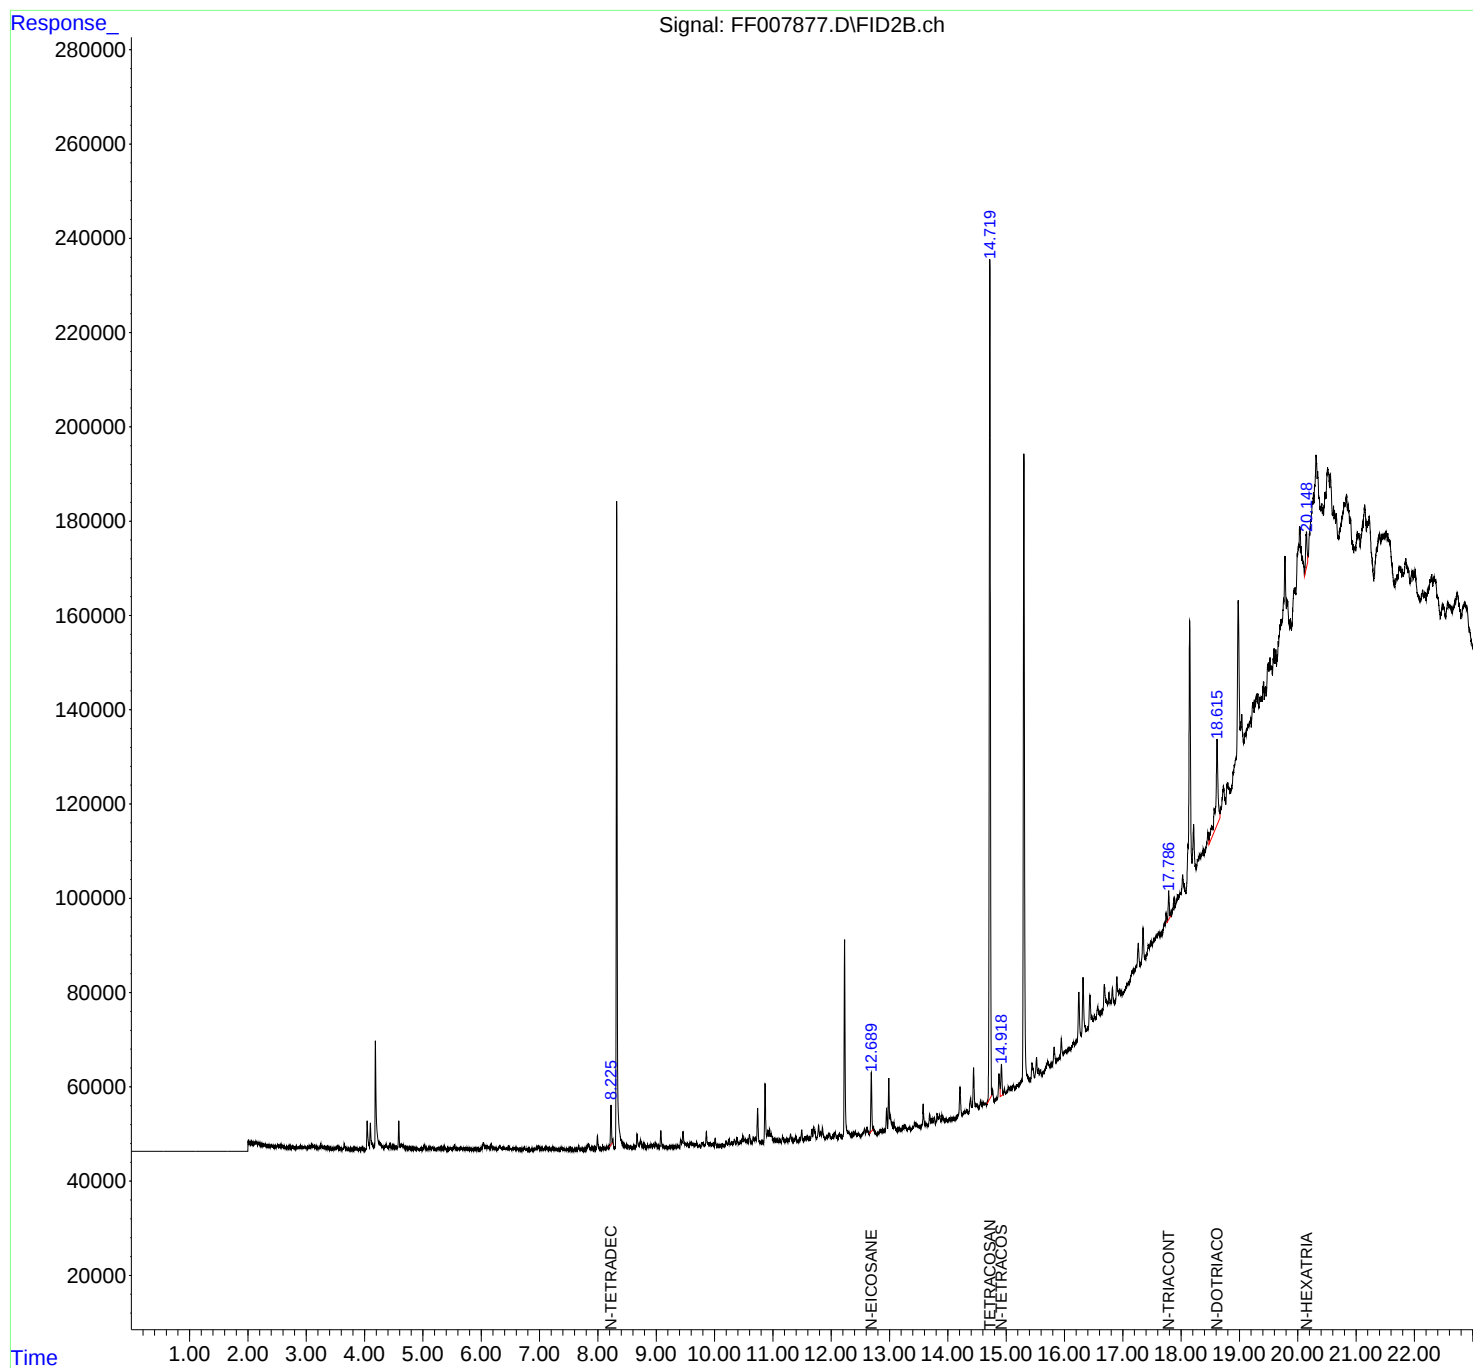


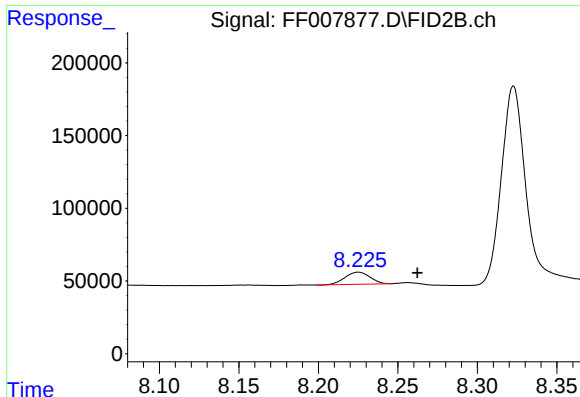

#4 N-TETRADECANE


R.T.: 8.225 min
Delta R.T.: -0.037 min
Response: 91397
Conc: 0.65 ug/ml

Instrument :
FID_F
ClientSampleId :

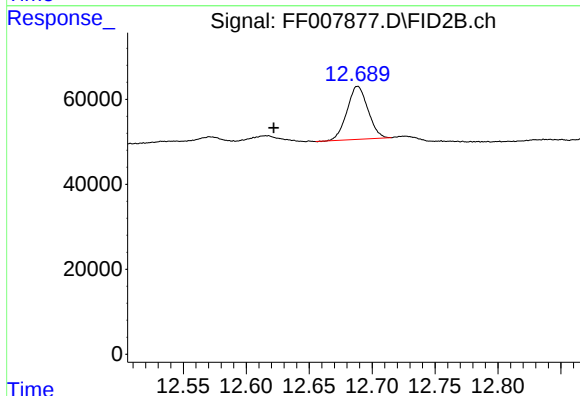


#7 N-EICOSANE

R.T.: 12.688 min
Delta R.T.: 0.067 min
Response: 143939
Conc: 0.97 ug/ml

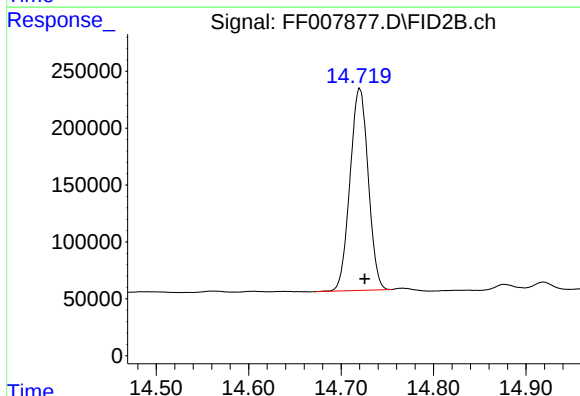


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.720 min
Delta R.T.: -0.006 min
Response: 2431299
Conc: 19.03 ug/ml

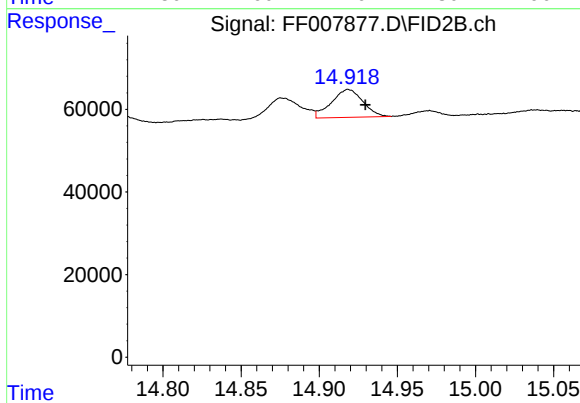

#10 N-TETRACOSANE


R.T.: 14.919 min
Delta R.T.: -0.011 min
Response: 94175
Conc: 0.65 ug/ml

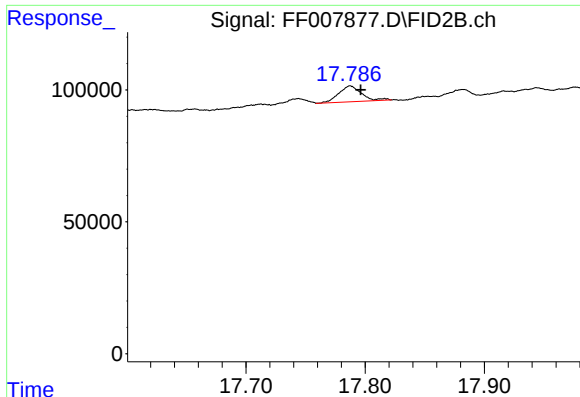

#13 N-TRIACONTANE


R.T.: 17.788 min
Delta R.T.: -0.009 min
Response: 79669
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :

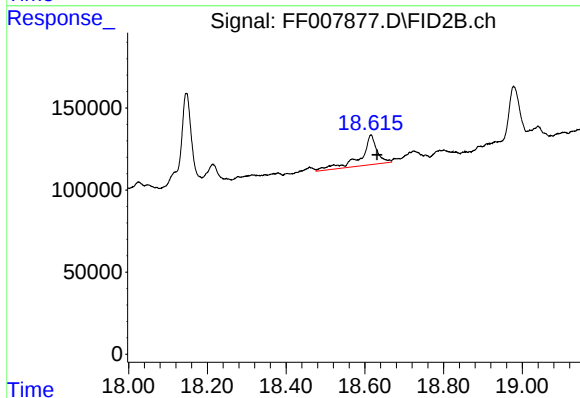

#14 N-DOTRIACONTANE

R.T.: 18.616 min
Delta R.T.: -0.016 min
Response: 513342
Conc: 4.43 ug/ml

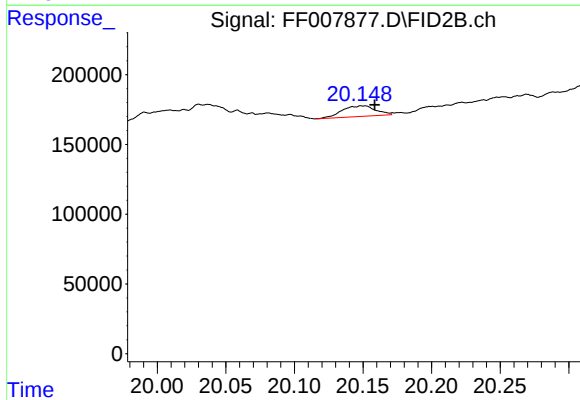

#16 N-HEXATRIACONTANE

R.T.: 20.150 min
Delta R.T.: -0.009 min
Response: 129176
Conc: 1.70 ug/ml