

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
 Data File : FF007885.D
 Signal(s) : FID2B.ch
 Acq On : 12 Nov 2020 17:50
 Operator : DD\AJ
 Sample : L4702-04 5X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 13 00:50:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.716	284349	2.226 ug/ml
Target Compounds			
4) N-TETRADECANE	8.255	273431	1.936 ug/ml
5) N-HEXADECANE	9.858	196171	1.350 ug/ml
7) N-EICOSANE	12.568f	96725	0.653 ug/ml
8) N-DOCOSANE	13.817	97820	0.671 ug/ml
10) N-TETRACOSANE	14.911	916008	6.334 ug/ml
11) N-HEXACOSANE	15.918	128120	0.913 ug/ml
12) N-OCTACOSANE	16.920	259949	1.917 ug/ml
13) N-TRIACONTANE	17.786	58822	0.455 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
Data File : FF007885.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2020 17:50
Operator : DD\AJ
Sample : L4702-04 5X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 13 00:50:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

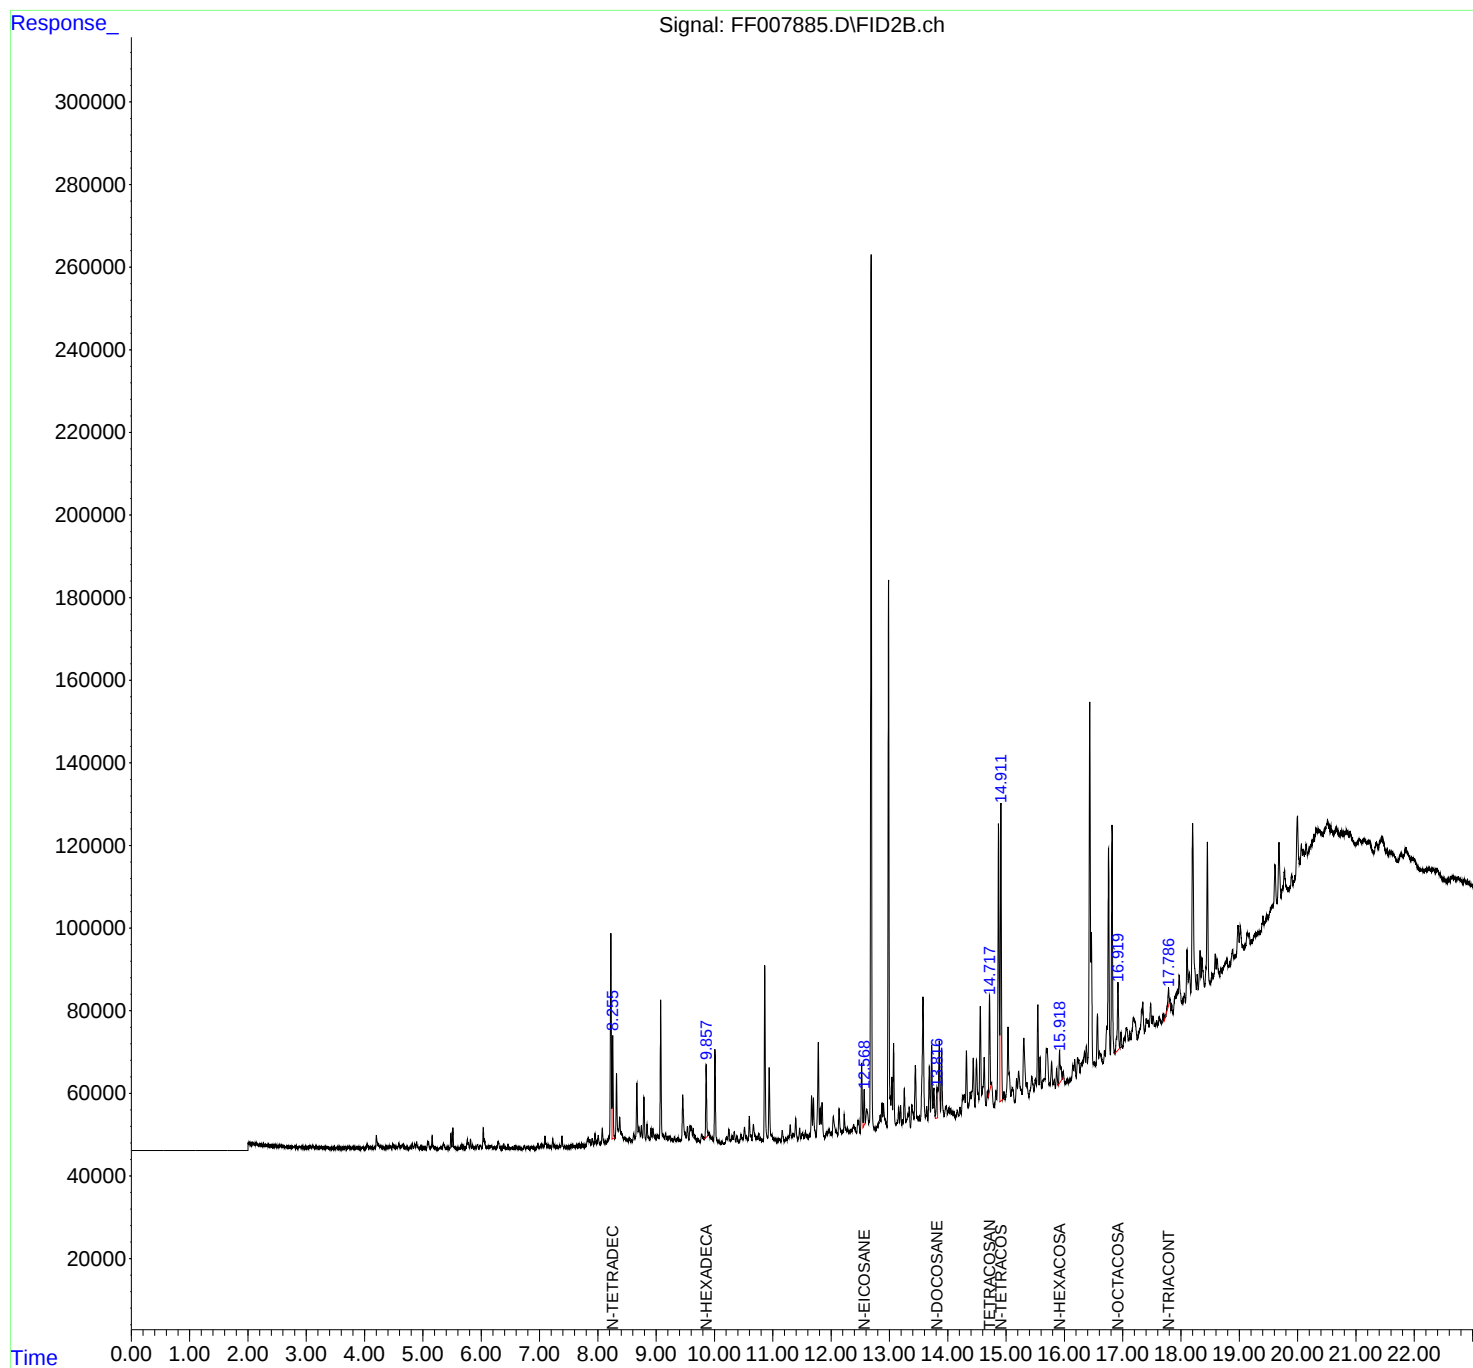


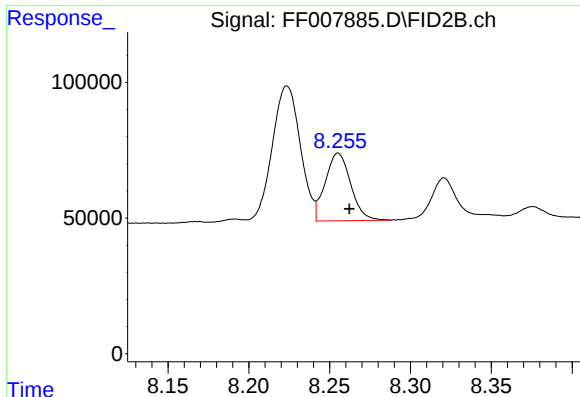

#4 N-TETRADECANE


R.T.: 8.255 min
Delta R.T.: -0.007 min
Response: 273431
Conc: 1.94 ug/ml

Instrument :
FID_F
ClientSampleId :

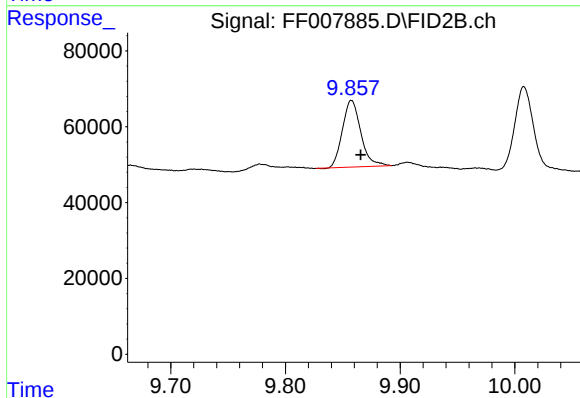


#5 N-HEXADECANE

R.T.: 9.858 min
Delta R.T.: -0.008 min
Response: 196171
Conc: 1.35 ug/ml

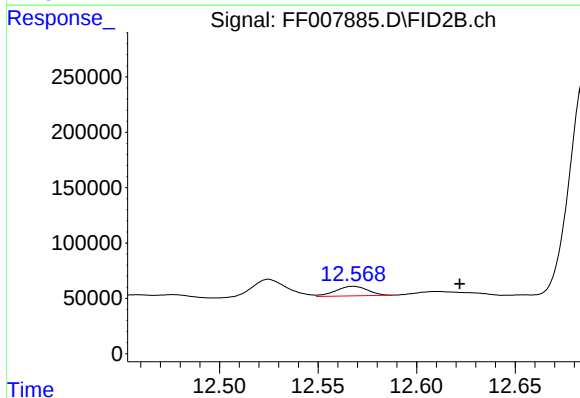


#7 N-EICOSANE

R.T.: 12.568 min
Delta R.T.: -0.054 min
Response: 96725
Conc: 0.65 ug/ml

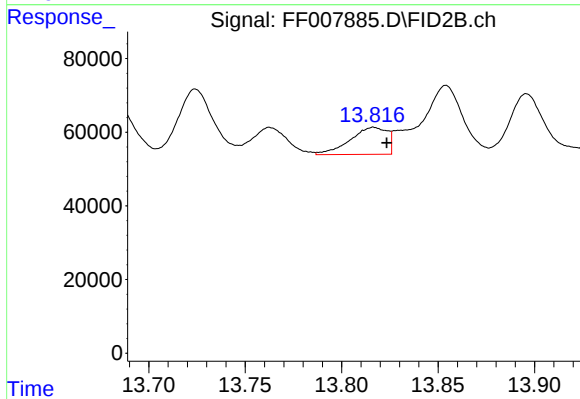

#8 N-DOCOSANE


R.T.: 13.817 min
Delta R.T.: -0.007 min
Response: 97820
Conc: 0.67 ug/ml

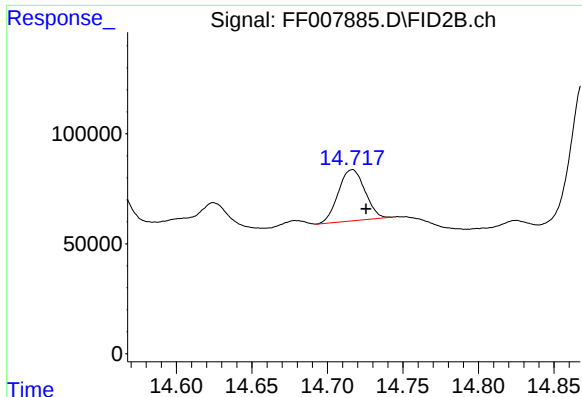

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.716 min
Delta R.T.: -0.009 min
Response: 284349
Conc: 2.23 ug/ml

Instrument :
FID_F
ClientSampleId :

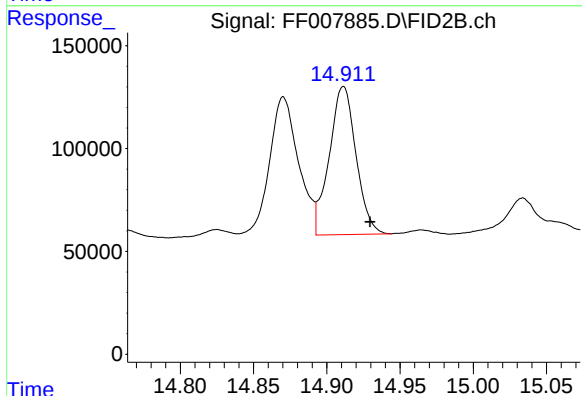


#10 N-TETRACOSANE

R.T.: 14.911 min
Delta R.T.: -0.018 min
Response: 916008
Conc: 6.33 ug/ml

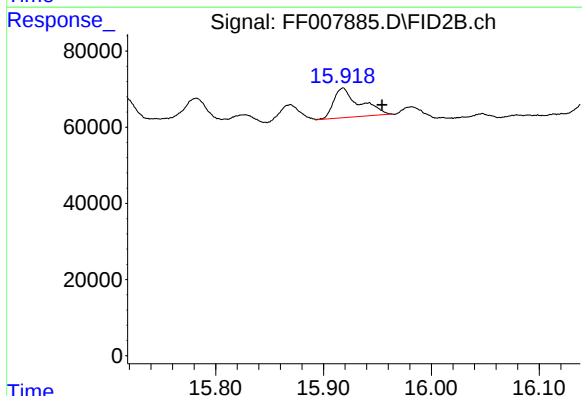


#11 N-HEXACOSANE

R.T.: 15.918 min
Delta R.T.: -0.036 min
Response: 128120
Conc: 0.91 ug/ml

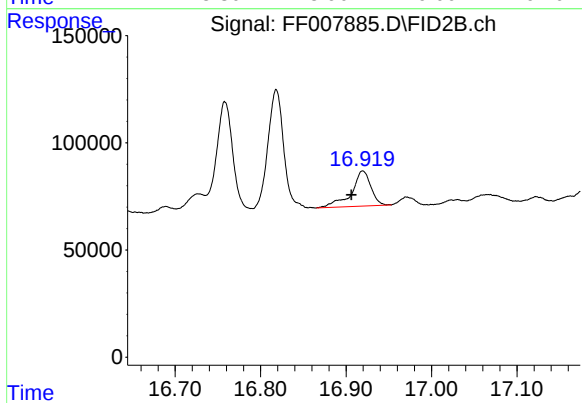

#12 N-OCTACOSANE

R.T.: 16.920 min
Delta R.T.: 0.013 min
Response: 259949
Conc: 1.92 ug/ml

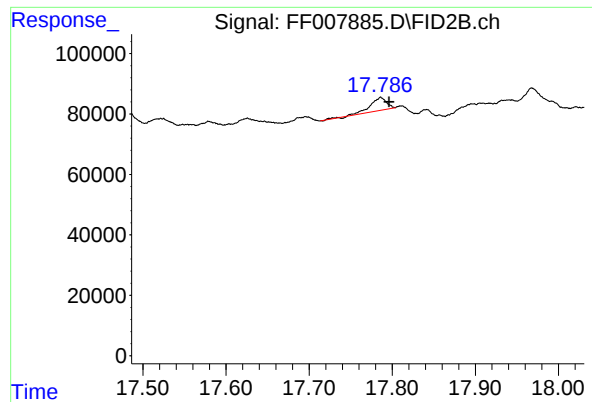

#13 N-TRIACONTANE

R.T.: 17.786 min
Delta R.T.: -0.010 min
Response: 58822
Conc: 0.45 ug/ml

Instrument :
FID_F
ClientSampleId :