

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
 Data File : FF007881.D
 Signal(s) : FID2B.ch
 Acq On : 12 Nov 2020 15:41
 Operator : DD\AJ
 Sample : L4702-02MSD
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 M-5(10-20)MSD

Integration File: autoint1.e
 Quant Time: Nov 13 00:50:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.718	2294560	17.963 ug/ml
Target Compounds			
2) N-DECANE	4.436	2661795	19.564 ug/ml
3) N-DODECANE	6.461	2750532	19.871 ug/ml
4) N-TETRADECANE	8.258	2978820	21.094 ug/ml
5) N-HEXADECANE	9.860	2907892	20.008 ug/ml
6) N-OCTADECANE	11.304	2685029	18.092 ug/ml
7) N-EICOSANE	12.616	2643829	17.836 ug/ml
8) N-DOCOSANE	13.817	2557194	17.552 ug/ml
10) N-TETRACOSANE	14.922	2466625	17.057 ug/ml
11) N-HEXACOSANE	15.946	2349937	16.743 ug/ml
12) N-OCTACOSANE	16.899	2276299	16.783 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111220\
Data File : FF007881.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2020 15:41
Operator : DD\AJ
Sample : L4702-02MSD
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
M-5(10-20)MSD

Integration File: autoint1.e
Quant Time: Nov 13 00:50:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

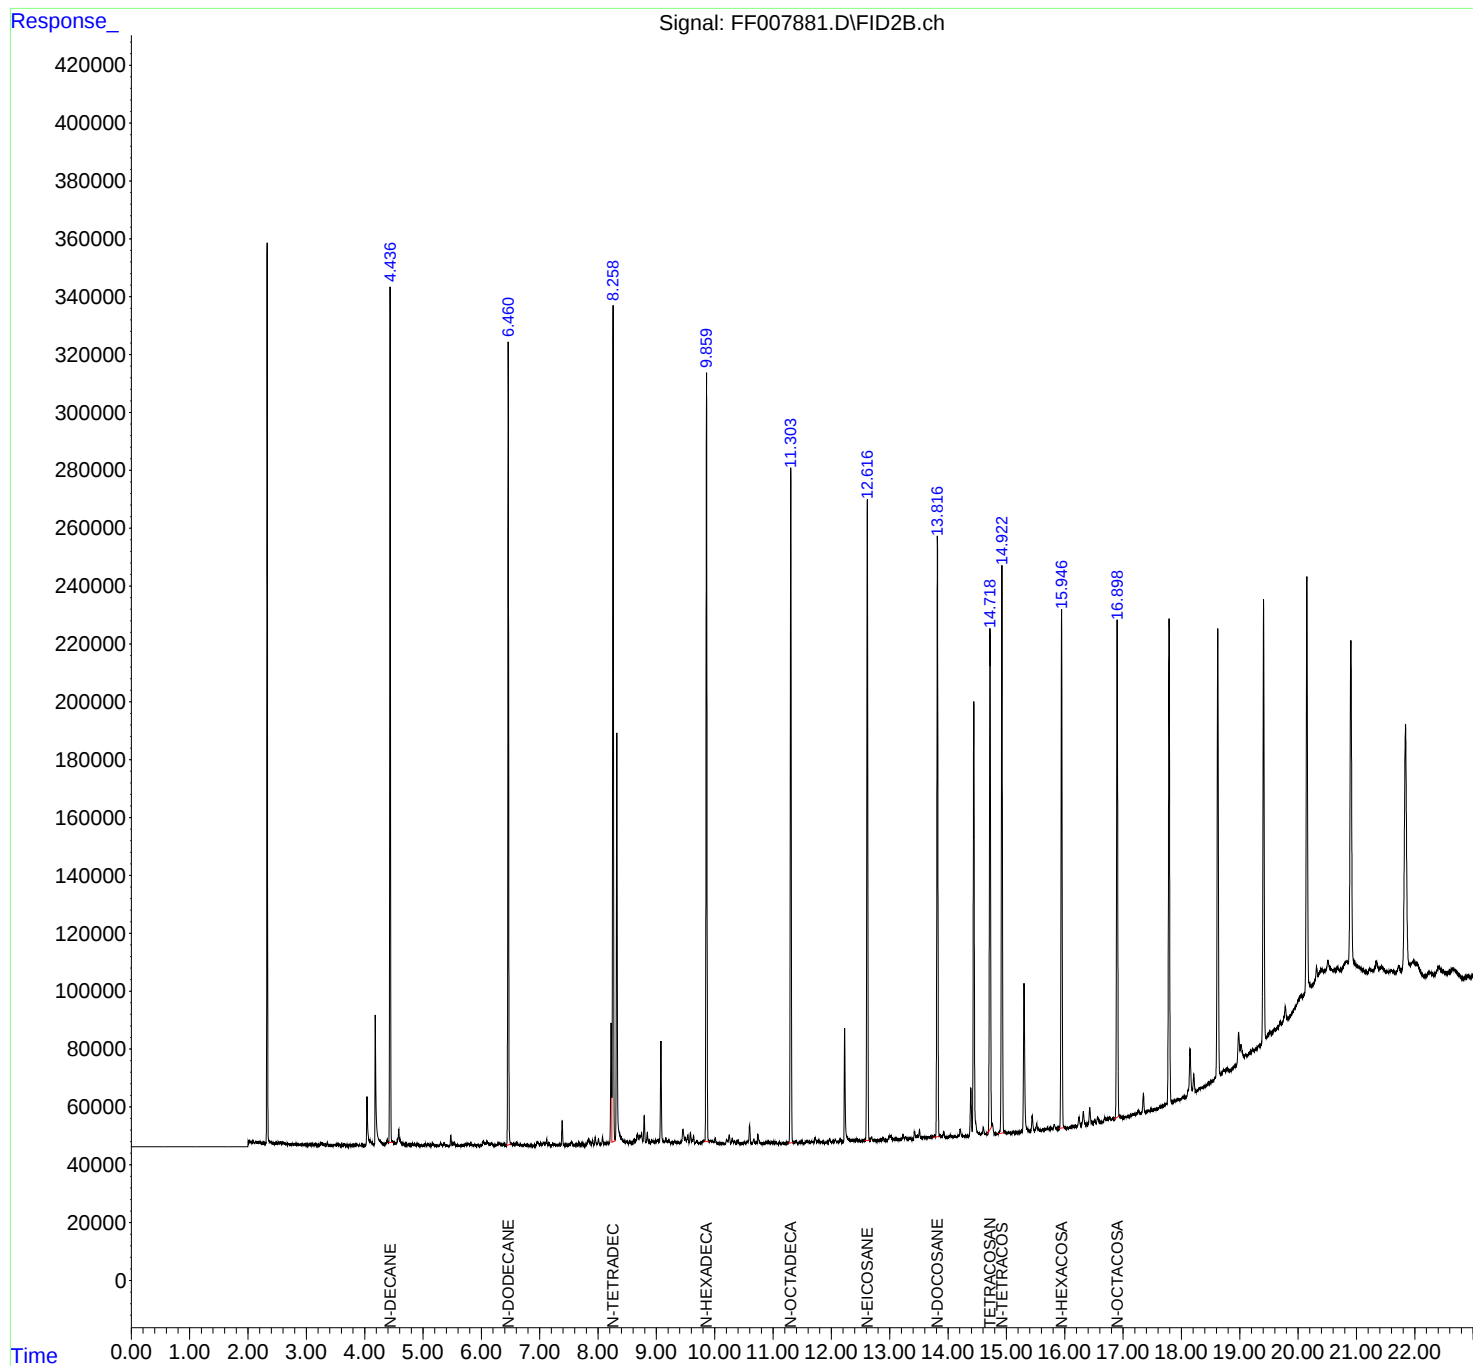


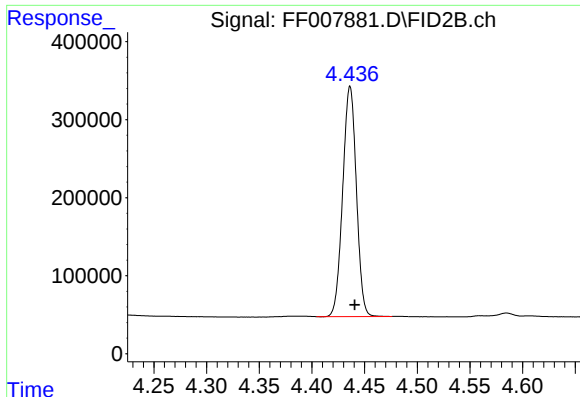

#2 N-DECANE


R.T.: 4.436 min
Delta R.T.: -0.004 min
Response: 2661795
Conc: 19.56 ug/ml

Instrument :
FID_F
ClientSampleId :
M-5(10-20)MSD

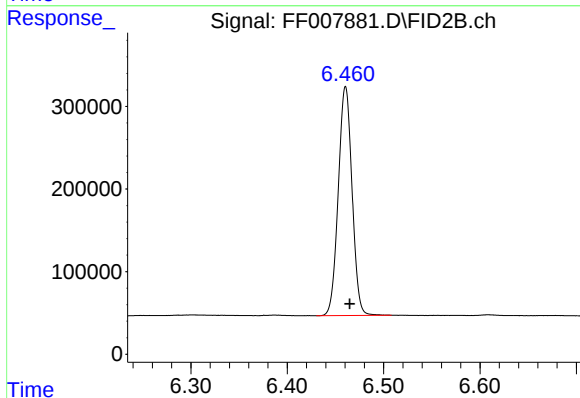


#3 N-DODECANE

R.T.: 6.461 min
Delta R.T.: -0.004 min
Response: 2750532
Conc: 19.87 ug/ml

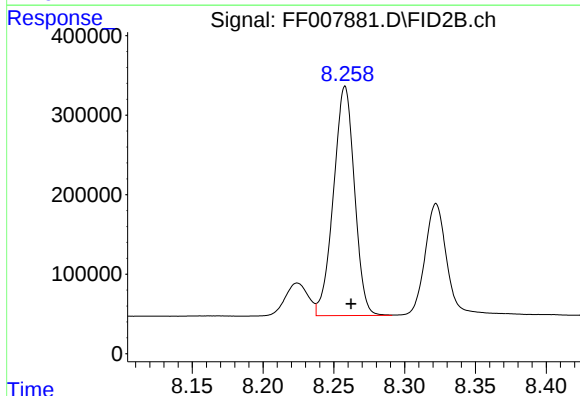


#4 N-TETRADECANE

R.T.: 8.258 min
Delta R.T.: -0.004 min
Response: 2978820
Conc: 21.09 ug/ml

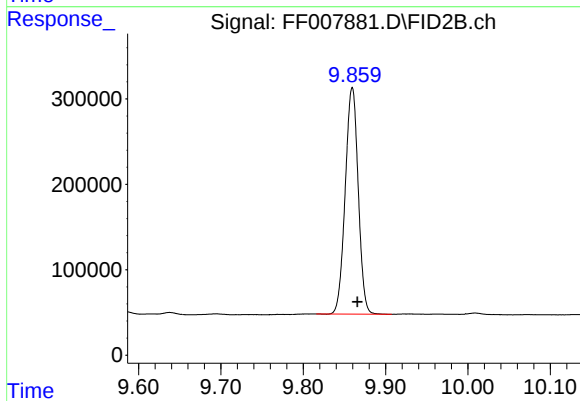

#5 N-HEXADECANE


R.T.: 9.860 min
Delta R.T.: -0.006 min
Response: 2907892
Conc: 20.01 ug/ml

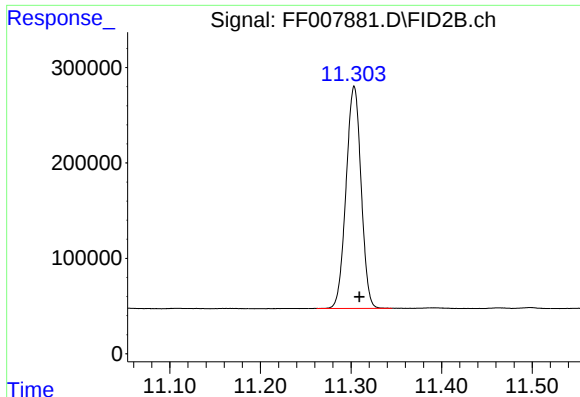

#6 N-OCTADECANE


R.T.: 11.304 min
Delta R.T.: -0.006 min
Response: 2685029
Conc: 18.09 ug/ml

Instrument :
FID_F
ClientSampleId :
M-5(10-20)MSD

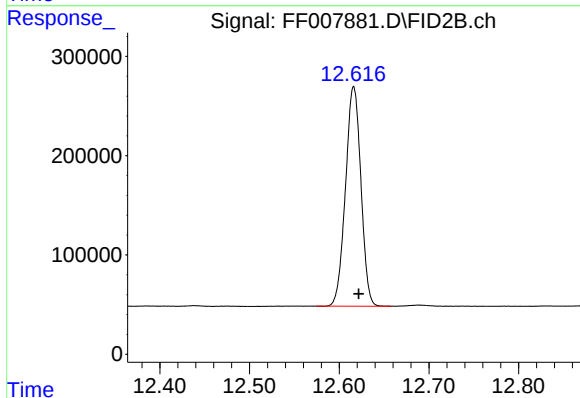


#7 N-EICOSANE

R.T.: 12.616 min
Delta R.T.: -0.006 min
Response: 2643829
Conc: 17.84 ug/ml

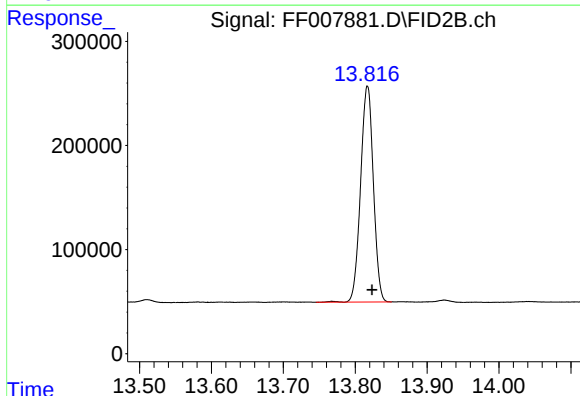


#8 N-DOCOSANE

R.T.: 13.817 min
Delta R.T.: -0.006 min
Response: 2557194
Conc: 17.55 ug/ml

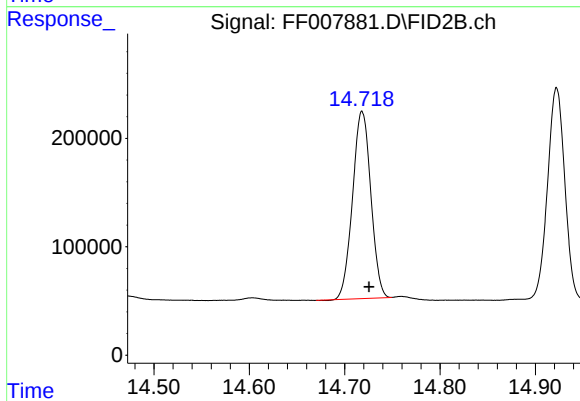

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.718 min
Delta R.T.: -0.007 min
Response: 2294560
Conc: 17.96 ug/ml

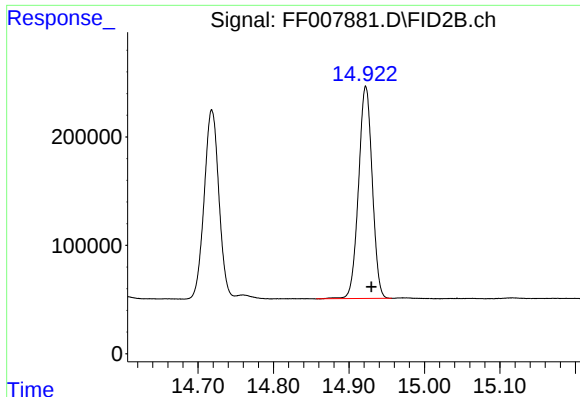

#10 N-TETRACOSANE


R.T.: 14.922 min
Delta R.T.: -0.007 min
Response: 2466625
Conc: 17.06 ug/ml

Instrument :
FID_F
ClientSampleId :
M-5(10-20)MSD

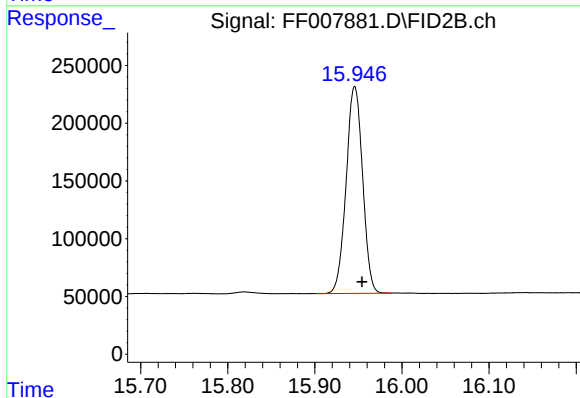

#11 N-HEXACOSANE

R.T.: 15.946 min
Delta R.T.: -0.009 min
Response: 2349937
Conc: 16.74 ug/ml

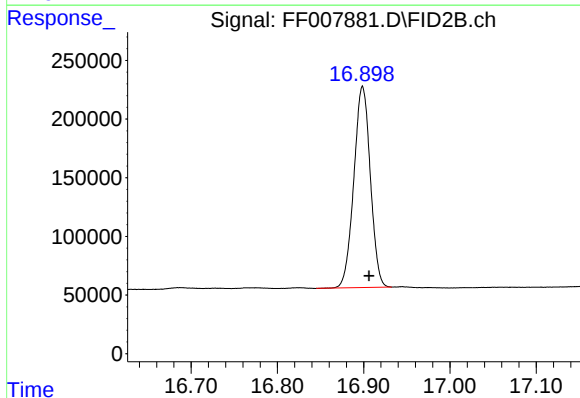

#12 N-OCTACOSANE

R.T.: 16.899 min
Delta R.T.: -0.007 min
Response: 2276299
Conc: 16.78 ug/ml