

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
Data File : FF016694.D
Signal(s) : FID2B.ch
Acq On : 13 Nov 2025 22:27
Operator : YP\AJ
Sample : Q3610-09
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AU-713-TPH-09

Integration File: Sample.e
Quant Time: Nov 14 05:51:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.053	1081979	10.356 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
Data File : FF016694.D
Signal(s) : FID2B.ch
Acq On : 13 Nov 2025 22:27
Operator : YP\AJ
Sample : Q3610-09
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AU-713-TPH-09

Integration File: Sample.e
Quant Time: Nov 14 05:51:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

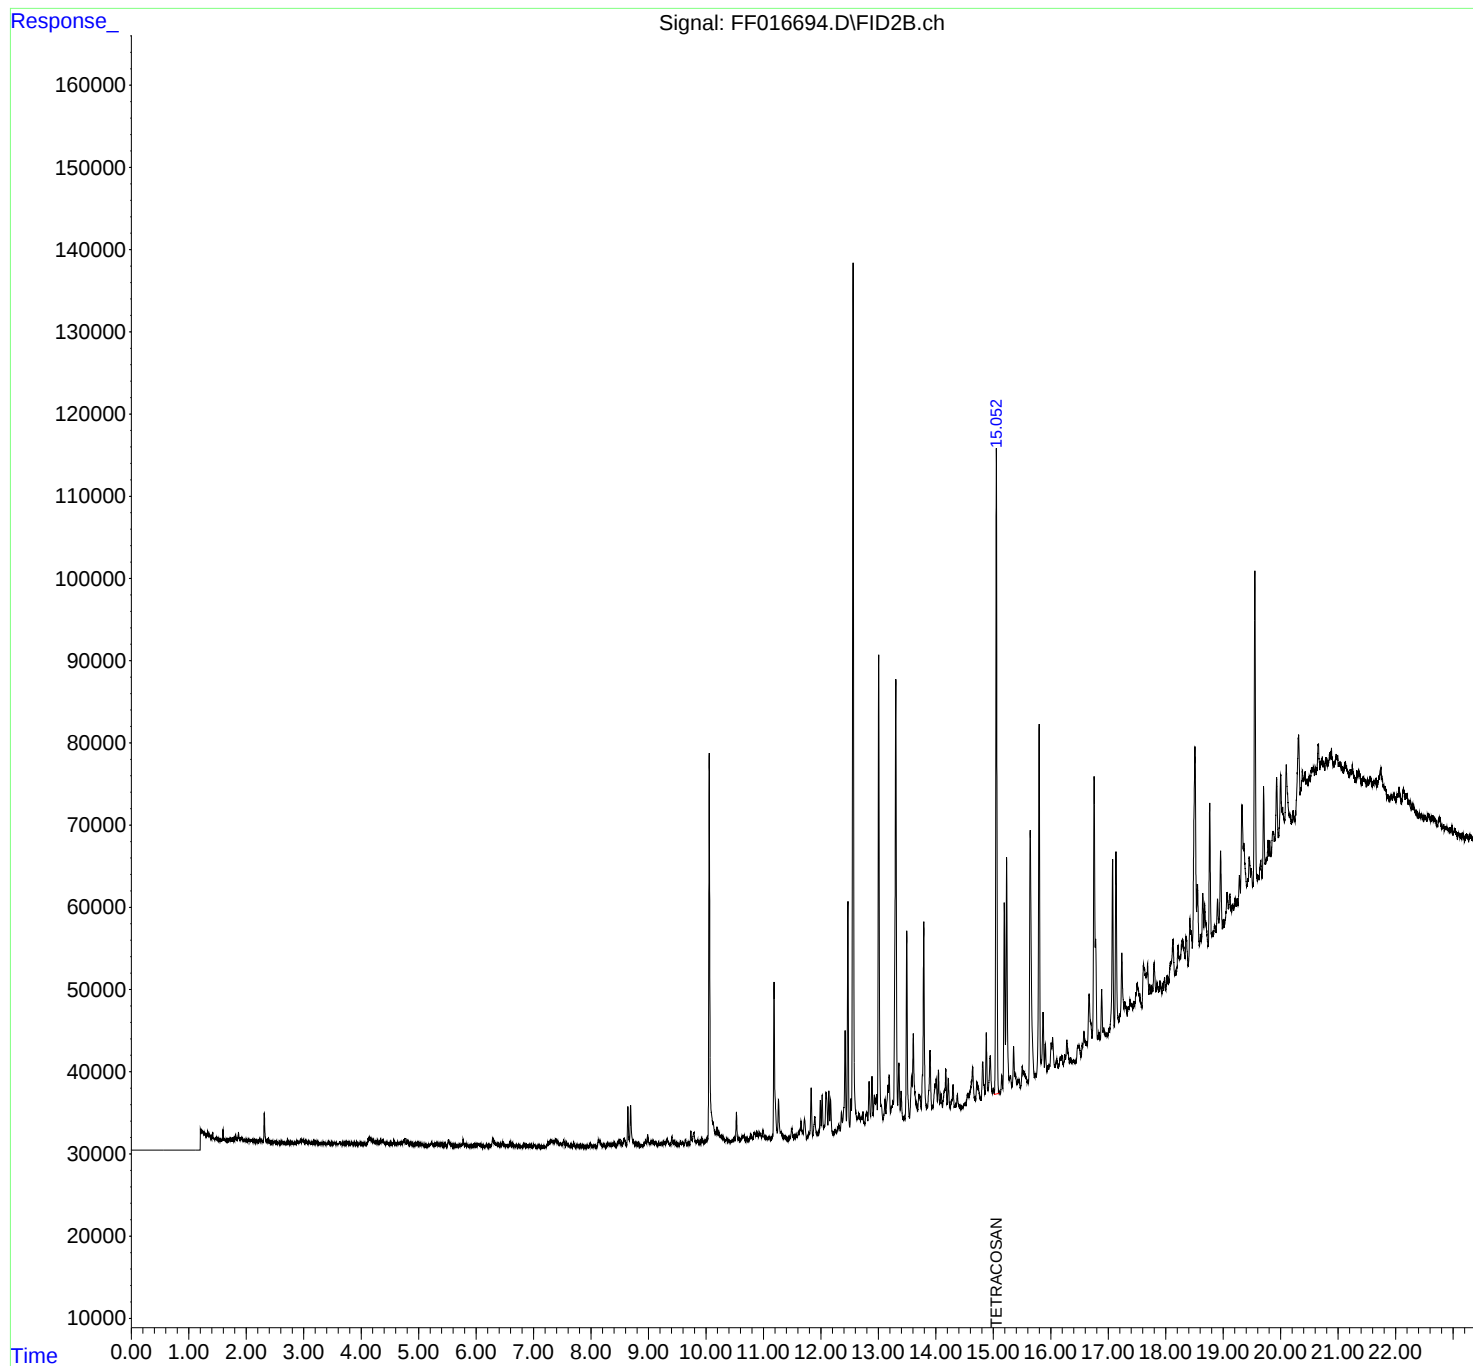

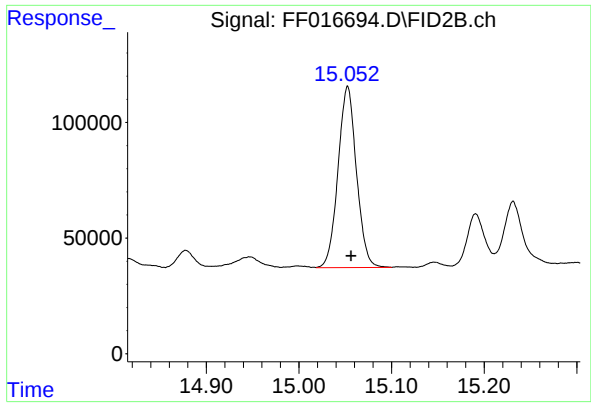

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.053 min
Delta R.T.: -0.004 min
Response: 1081979
Conc: 10.36 ug/ml

Instrument :
FID_F
ClientSampleId :
AU-713-TPH-09