

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
 Data File : FF016697.D
 Signal(s) : FID2B.ch
 Acq On : 13 Nov 2025 23:55
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: Sample.e
 Quant Time: Nov 14 05:52:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
 Quant Title :
 QLast Update : Wed Oct 29 12:48:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.057	5151239	49.306 ug/ml
Target Compounds			
2) N-DECANE	4.571	5733267	51.816 ug/ml
3) N-DODECANE	6.750	5793555	52.154 ug/ml
4) N-TETRADECANE	8.583	5821869	52.114 ug/ml
5) N-HEXADECANE	10.193	5822200	51.819 ug/ml
6) N-OCTADECANE	11.639	5970574	51.018 ug/ml
7) N-EICOSANE	12.952	6107037	50.014 ug/ml
8) N-DOCOSANE	14.154	5906762	49.551 ug/ml
10) N-TETRACOSANE	15.261	5824625	49.157 ug/ml
11) N-HEXACOSANE	16.286	5562937	48.424 ug/ml
12) N-OCTACOSANE	17.240	5433556	47.681 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
Data File : FF016697.D
Signal(s) : FID2B.ch
Acq On : 13 Nov 2025 23:55
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: Sample.e
Quant Time: Nov 14 05:52:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

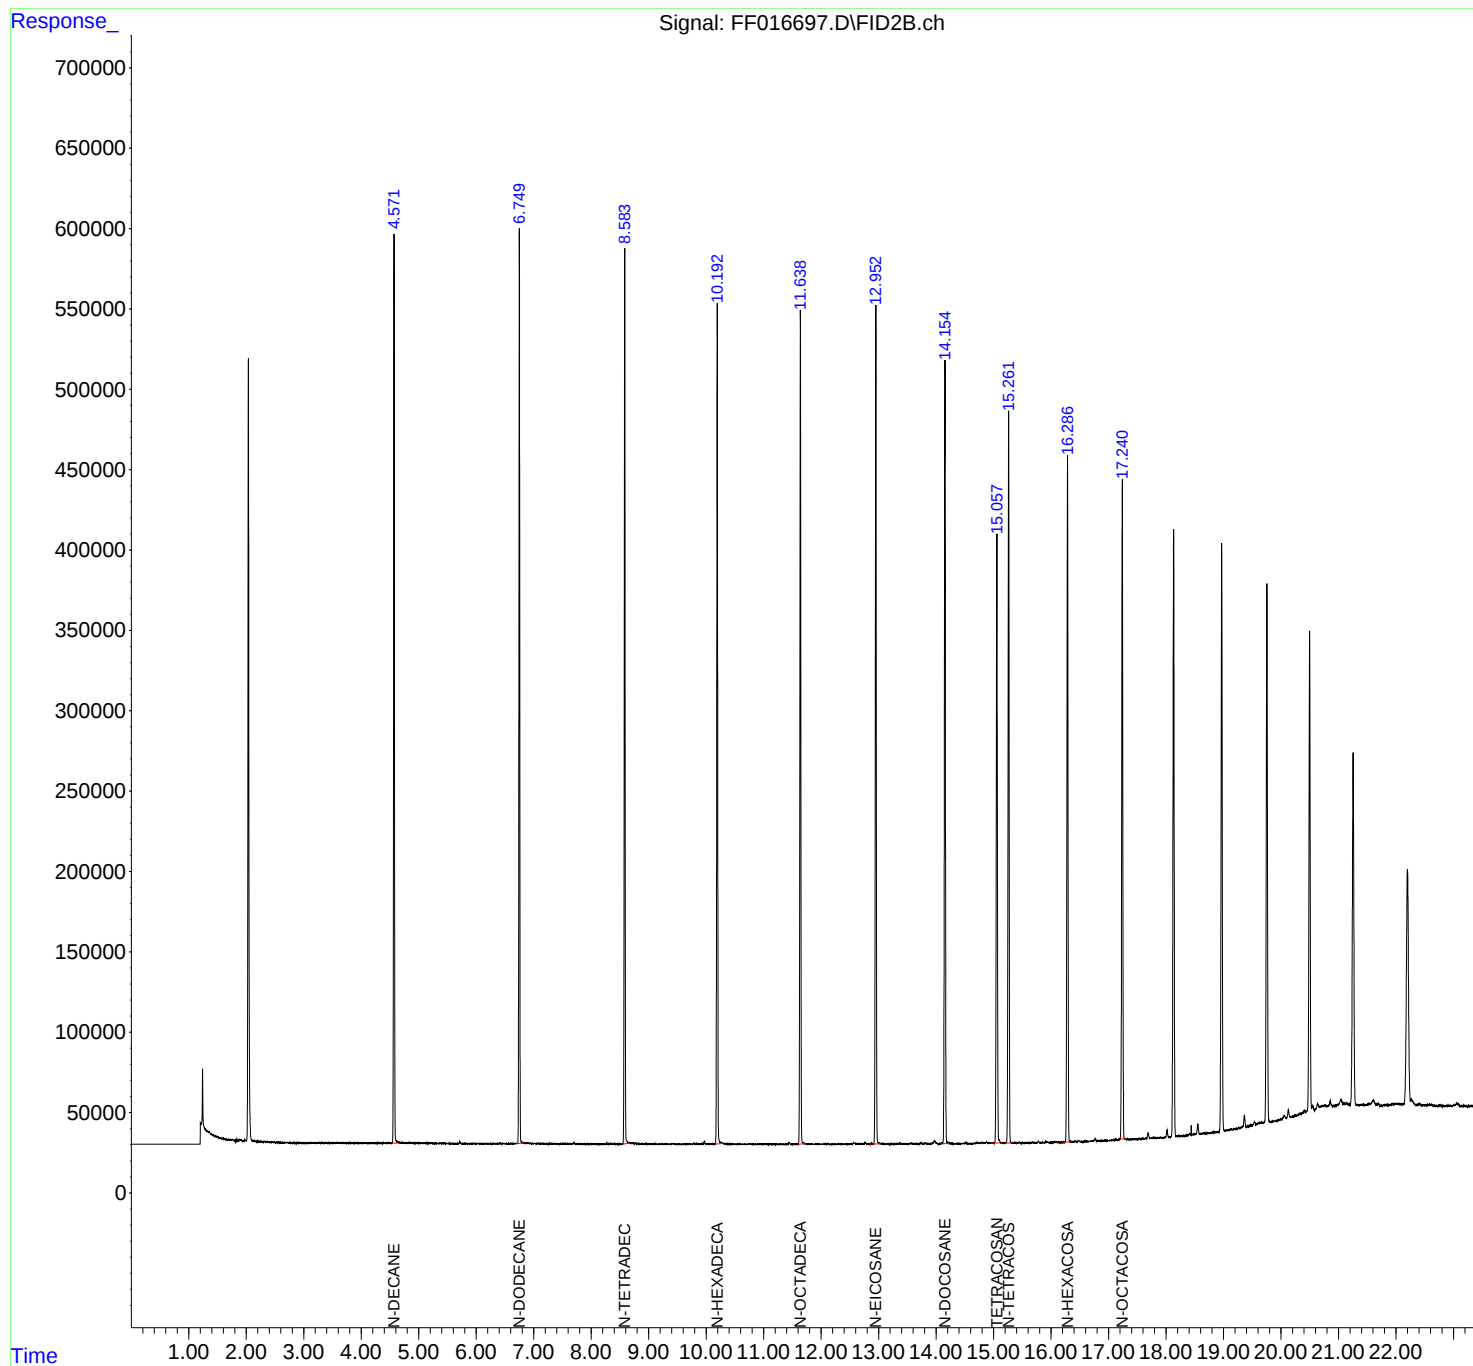


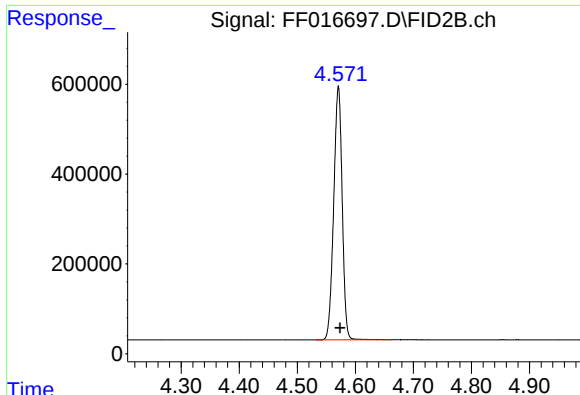

#2 N-DECANE


R.T.: 4.571 min
Delta R.T.: -0.003 min
Response: 5733267
Conc: 51.82 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

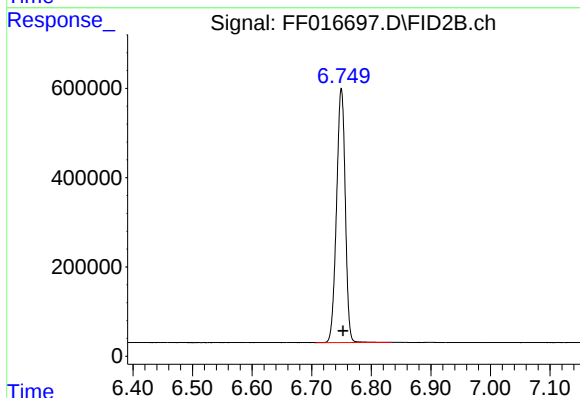


#3 N-DODECANE

R.T.: 6.750 min
Delta R.T.: -0.003 min
Response: 5793555
Conc: 52.15 ug/ml

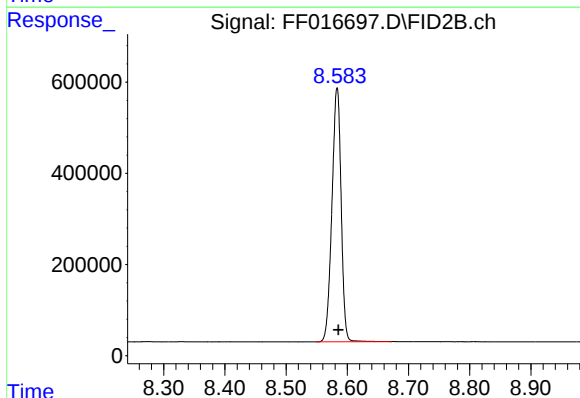


#4 N-TETRADECANE

R.T.: 8.583 min
Delta R.T.: -0.002 min
Response: 5821869
Conc: 52.11 ug/ml

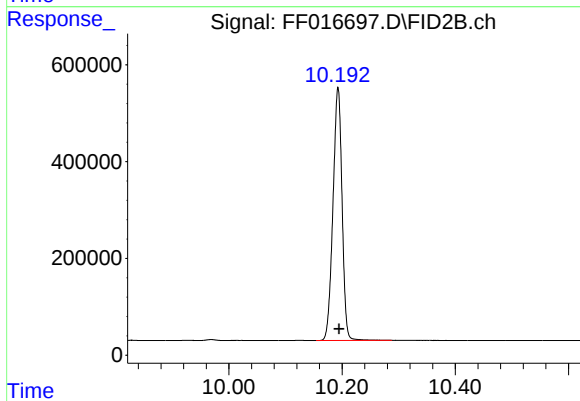

#5 N-HEXADECANE


R.T.: 10.193 min
Delta R.T.: -0.002 min
Response: 5822200
Conc: 51.82 ug/ml

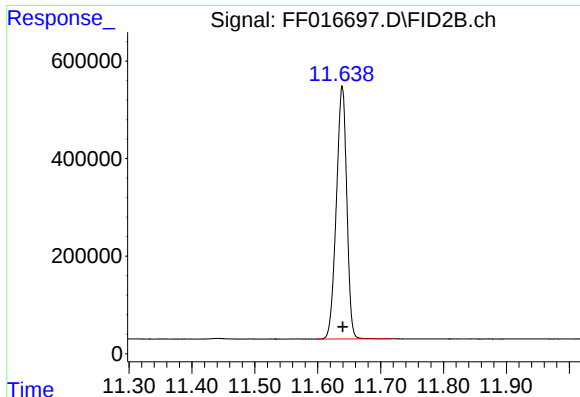

#6 N-OCTADECANE


R.T.: 11.639 min
Delta R.T.: -0.001 min
Response: 5970574
Conc: 51.02 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

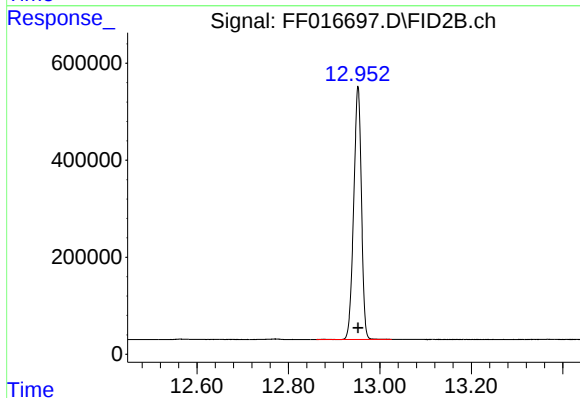


#7 N-EICOSANE

R.T.: 12.952 min
Delta R.T.: 0.000 min
Response: 6107037
Conc: 50.01 ug/ml

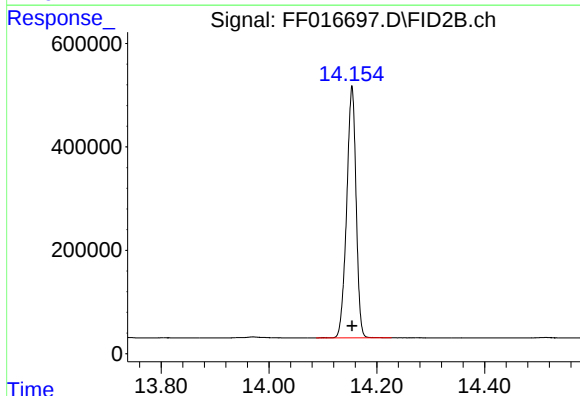


#8 N-DOCOSANE

R.T.: 14.154 min
Delta R.T.: 0.000 min
Response: 5906762
Conc: 49.55 ug/ml

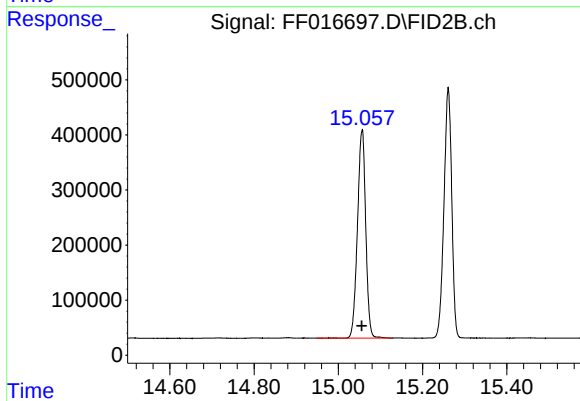

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.057 min
Delta R.T.: 0.000 min
Response: 5151239
Conc: 49.31 ug/ml

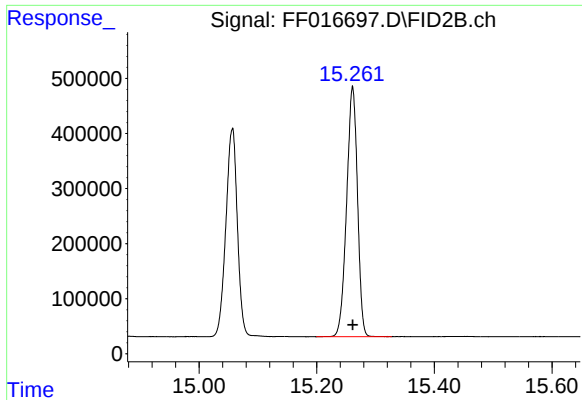

#10 N-TETRACOSANE


R.T.: 15.261 min
Delta R.T.: 0.000 min
Response: 5824625
Conc: 49.16 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

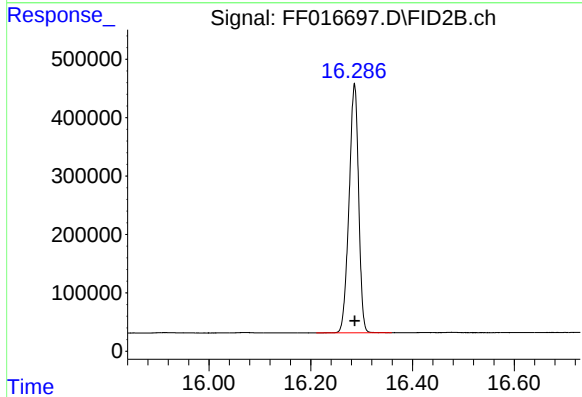

#11 N-HEXACOSANE

R.T.: 16.286 min
Delta R.T.: 0.000 min
Response: 5562937
Conc: 48.42 ug/ml

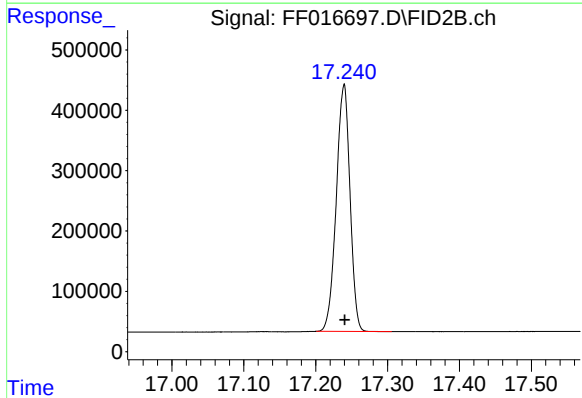

#12 N-OCTACOSANE

R.T.: 17.240 min
Delta R.T.: 0.000 min
Response: 5433556
Conc: 47.68 ug/ml