

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111418\
 Data File : FF002684.D
 Signal(s) : FID2B.ch
 Acq On : 14 Nov 2018 15:00
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 15 00:48:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.648	4117354	52.708 ug/ml
Target Compounds			
2) N-DECANE	4.370	6612643	52.944 ug/ml
3) N-DODECANE	6.395	6539295	53.952 ug/ml
4) N-TETRADECANE	8.191	6312121	54.643 ug/ml
5) N-HEXADECANE	9.793	5998650	54.863 ug/ml
6) N-OCTADECANE	11.236	5684311	54.759 ug/ml
7) N-EICOSANE	12.547	5264649	54.374 ug/ml
8) N-DOCOSANE	13.749	4897722	53.494 ug/ml
10) N-TETRACOSANE	14.852	4654078	52.241 ug/ml
11) N-HEXACOSANE	15.876	4611940	50.819 ug/ml
12) N-OCTACOSANE	16.827	4815111	50.484 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111418\
Data File : FF002684.D
Signal(s) : FID2B.ch
Acq On : 14 Nov 2018 15:00
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 15 00:48:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

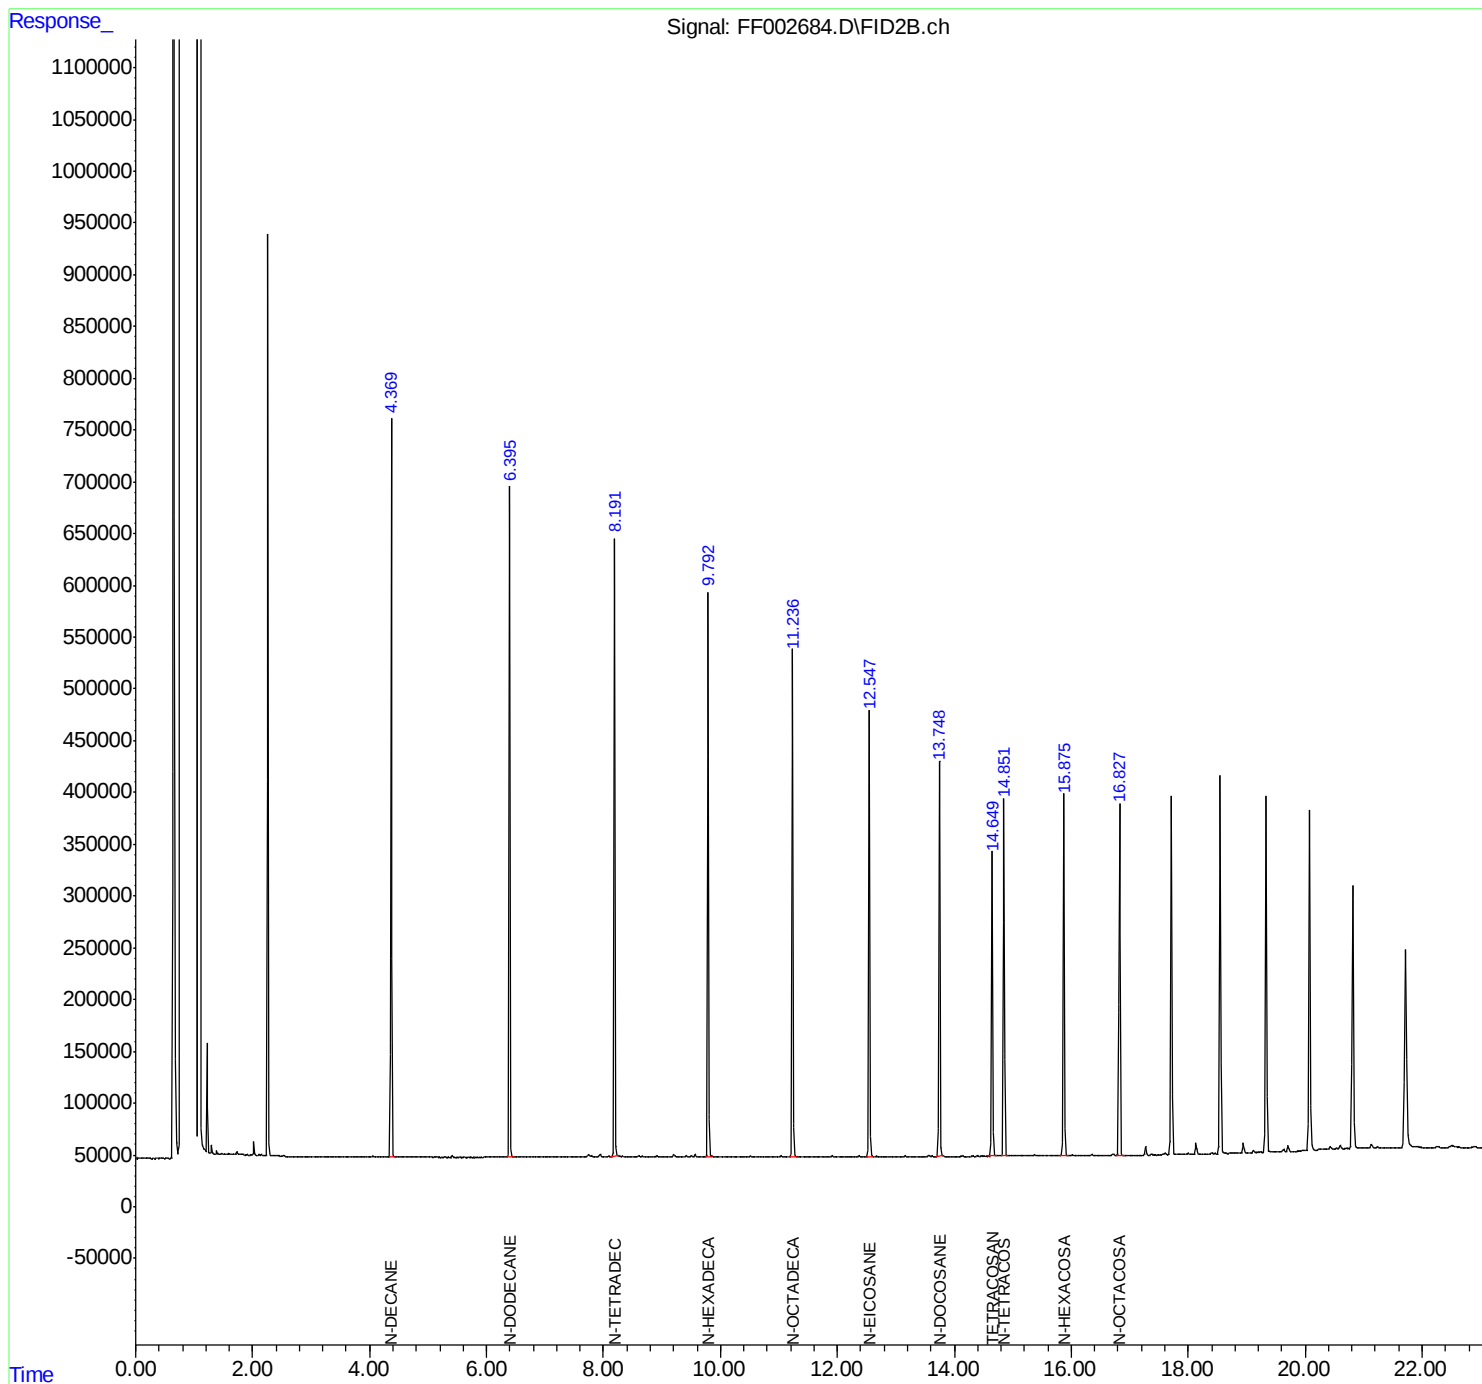

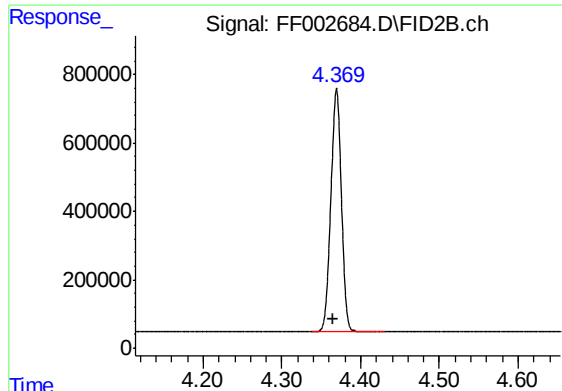


#2 N-DECANE

R.T.: 4.370 min
Delta R.T.: 0.004 min
Response: 6612643
Conc: 52.94 ug/ml

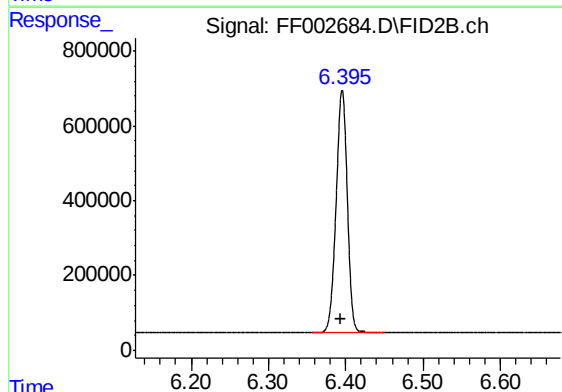


#3 N-DODECANE

R.T.: 6.395 min
Delta R.T.: 0.002 min
Response: 6539295
Conc: 53.95 ug/ml

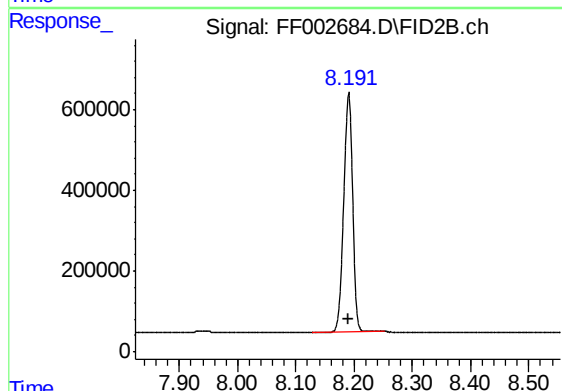


#4 N-TETRADECANE

R.T.: 8.191 min
Delta R.T.: 0.001 min
Response: 6312121
Conc: 54.64 ug/ml

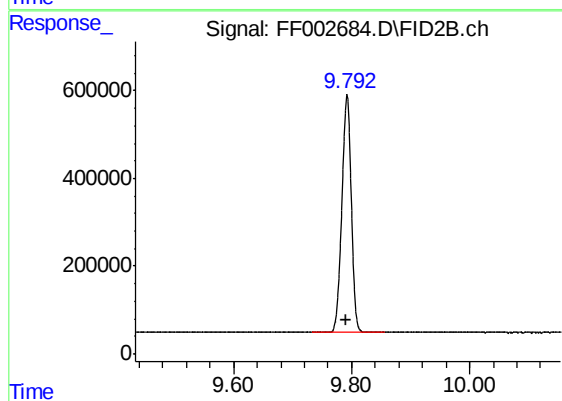


#5 N-HEXADECANE

R.T.: 9.793 min
Delta R.T.: 0.001 min
Response: 5998650
Conc: 54.86 ug/ml

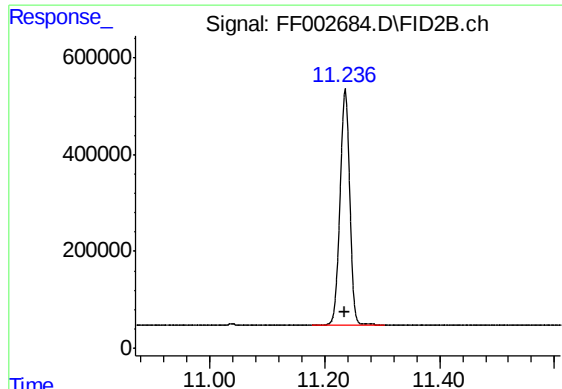


#6 N-OCTADECANE

R.T.: 11.236 min
Delta R.T.: 0.000 min
Response: 5684311
Conc: 54.76 ug/ml

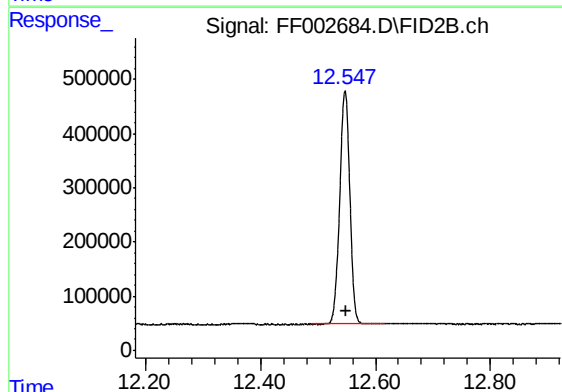


#7 N-EICOSANE

R.T.: 12.547 min
Delta R.T.: 0.000 min
Response: 5264649
Conc: 54.37 ug/ml

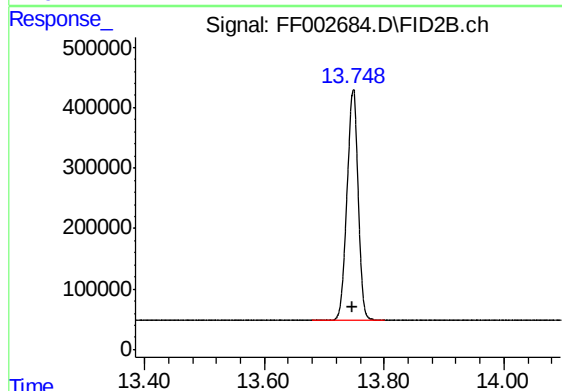


#8 N-DOCOSANE

R.T.: 13.749 min
Delta R.T.: 0.001 min
Response: 4897722
Conc: 53.49 ug/ml

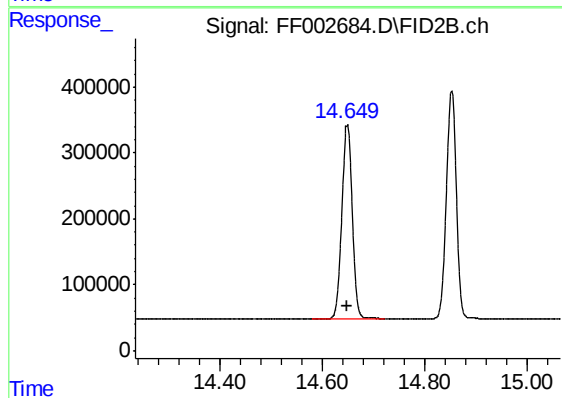


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.648 min
Delta R.T.: 0.000 min
Response: 4117354
Conc: 52.71 ug/ml

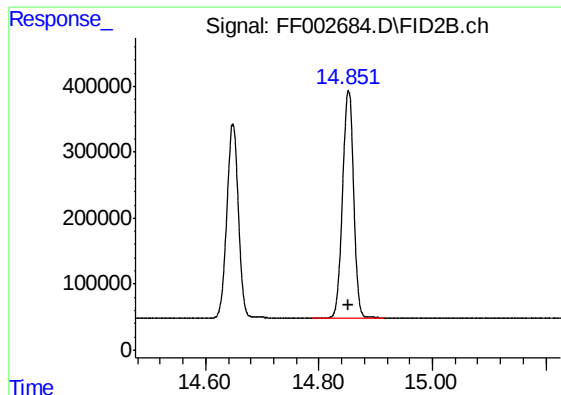


#10 N-TETRACOSANE

R.T.: 14.852 min
Delta R.T.: -0.001 min
Response: 4654078
Conc: 52.24 ug/ml

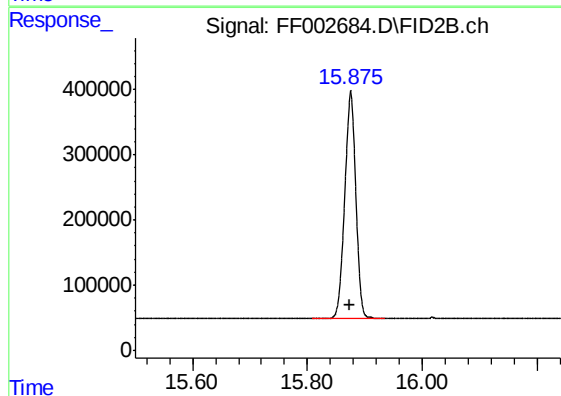

#11 N-HEXACOSANE

R.T.: 15.876 min
Delta R.T.: 0.000 min
Response: 4611940
Conc: 50.82 ug/ml

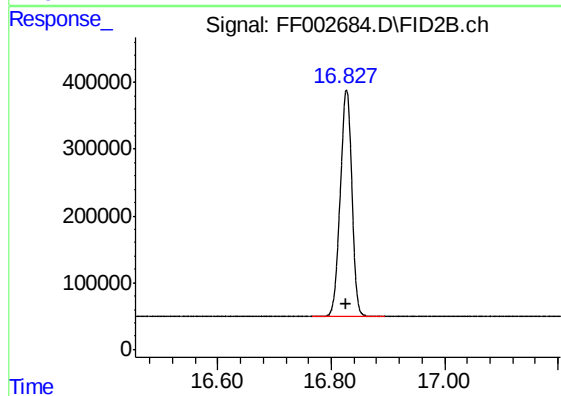

#12 N-OCTACOSANE

R.T.: 16.827 min
Delta R.T.: 0.000 min
Response: 4815111
Conc: 50.48 ug/ml