

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111422\
 Data File : FF011688.D
 Signal(s) : FID2B.ch
 Acq On : 14 Nov 2022 08:38
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 14 13:00:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.045	169892	1.432 ug/ml
Target Compounds			
8) N-DOCOSANE	14.136	822402	6.093 ug/ml
10) N-TETRACOSANE	15.228	2782417	20.518 ug/ml
11) N-HEXACOSANE	16.275	633158	4.739 ug/ml
12) N-OCTACOSANE	17.227	439101	3.314 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111422\
Data File : FF011688.D
Signal(s) : FID2B.ch
Acq On : 14 Nov 2022 08:38
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 13:00:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

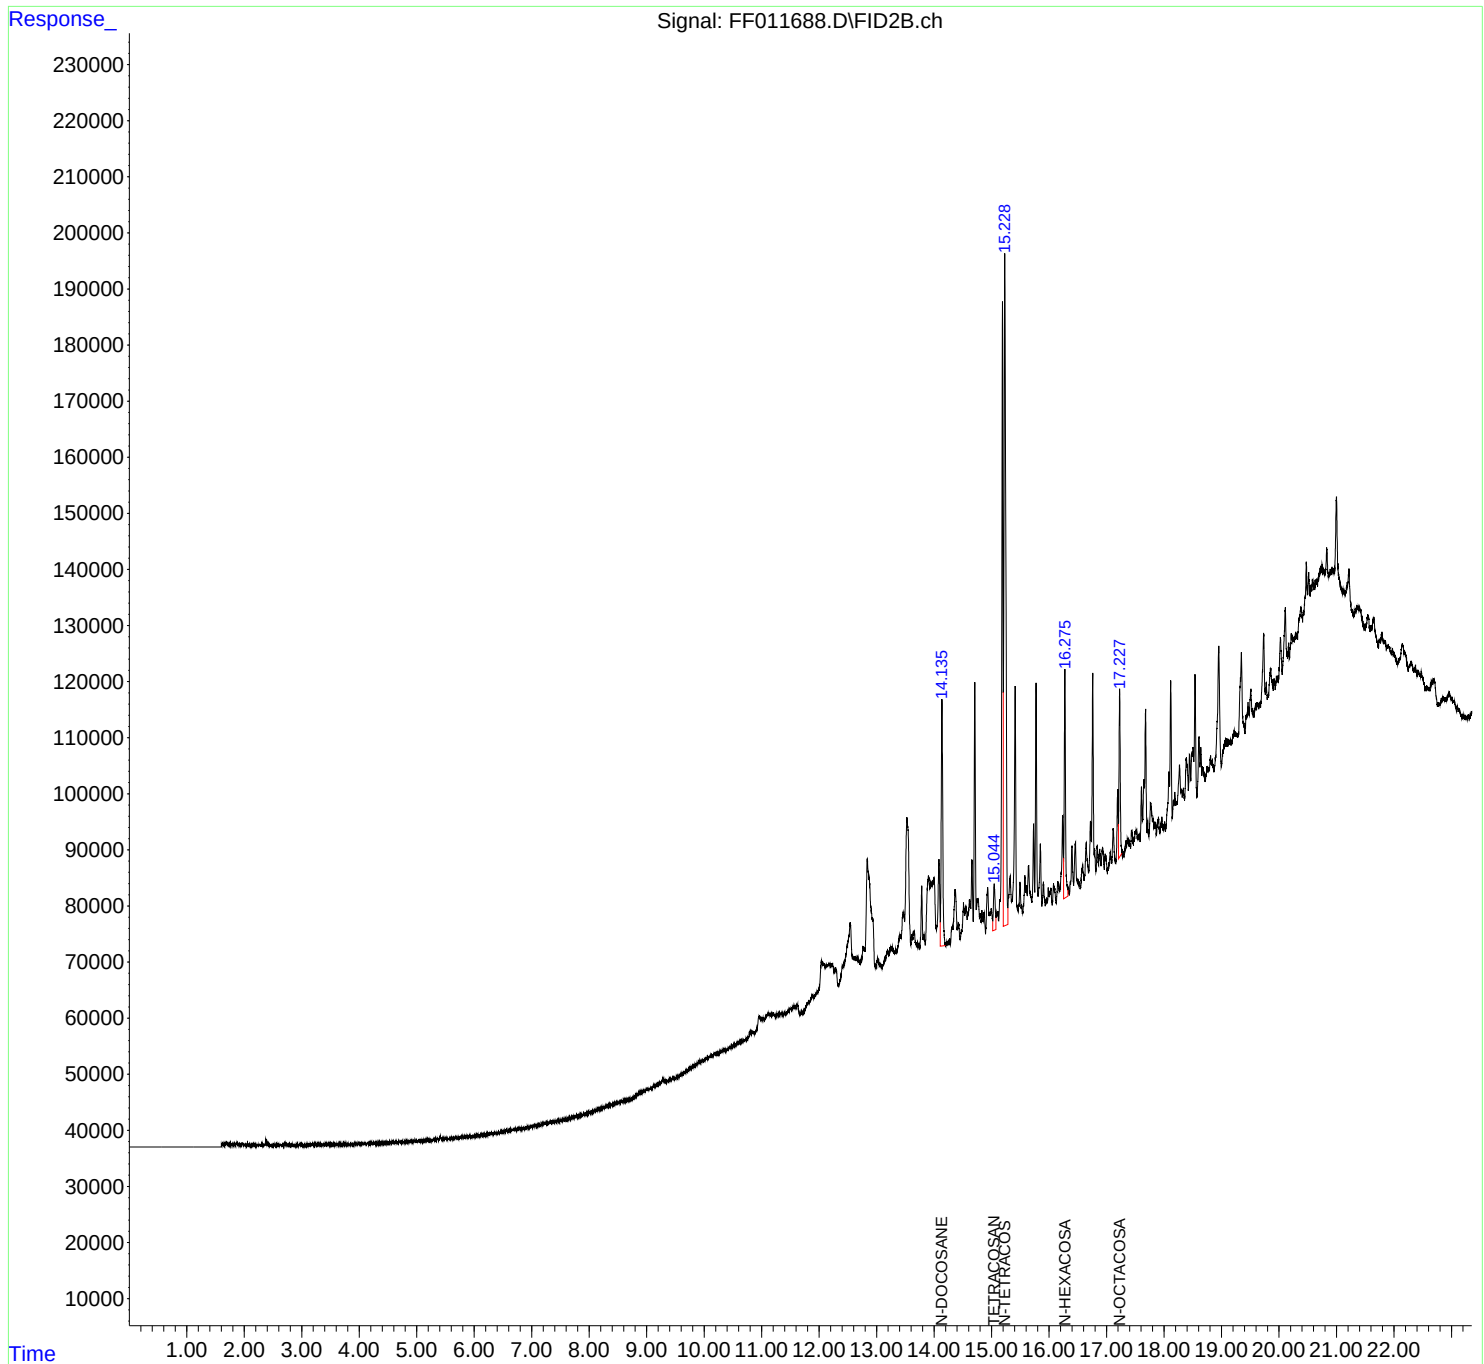


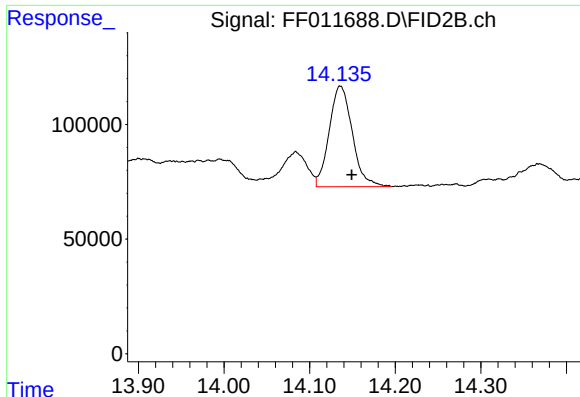

#8 N-DOCOSANE


R.T.: 14.136 min
Delta R.T.: -0.013 min
Response: 822402
Conc: 6.09 ug/ml

Instrument :
FID_F
ClientSampleId :

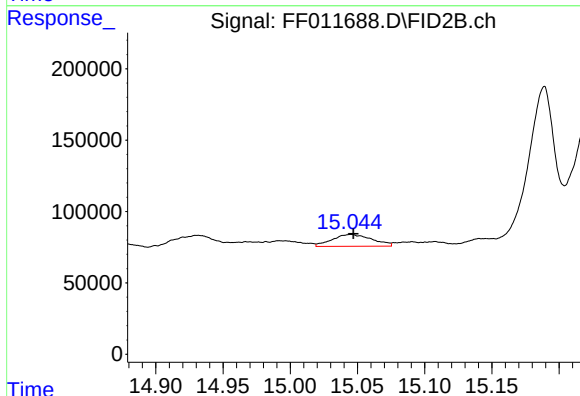


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.045 min
Delta R.T.: -0.002 min
Response: 169892
Conc: 1.43 ug/ml

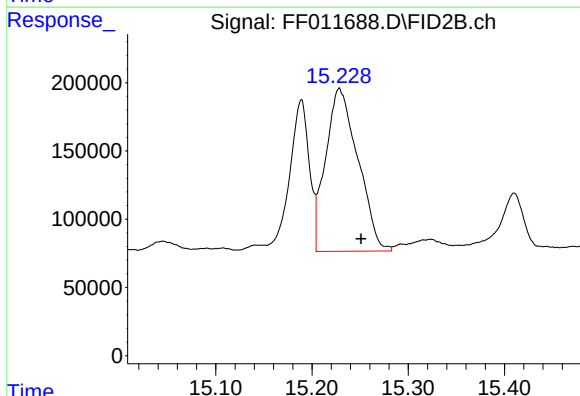


#10 N-TETRACOSANE

R.T.: 15.228 min
Delta R.T.: -0.023 min
Response: 2782417
Conc: 20.52 ug/ml

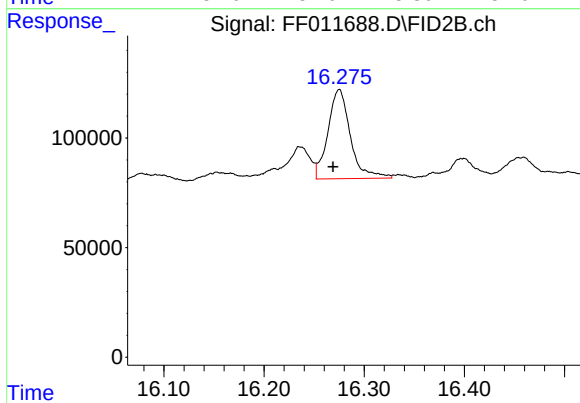

#11 N-HEXACOSANE

R.T.: 16.275 min
Delta R.T.: 0.006 min
Response: 633158
Conc: 4.74 ug/ml

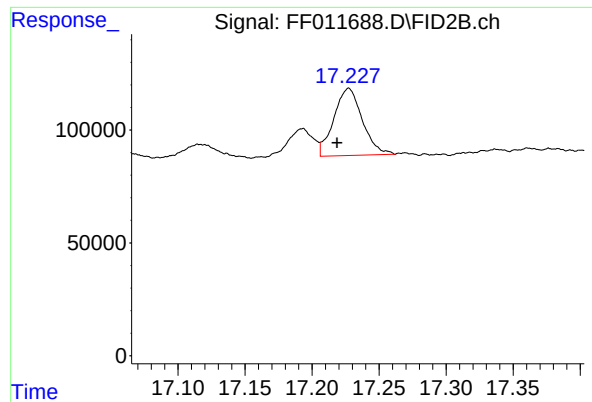

#12 N-OCTACOSANE

R.T.: 17.227 min
Delta R.T.: 0.009 min
Response: 439101
Conc: 3.31 ug/ml

Instrument :
FID_F
ClientSampleId :