

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111422\
 Data File : FF011722.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2022 05:38
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 15 07:10:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.057	2306138	19.437 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.230	47768	0.361 ug/ml
13) N-TRIACONTANE	18.116	127201	0.964 ug/ml
14) N-DOTRIACONTANE	18.950	178171	1.324 ug/ml
15) N-TETRATRIACONTANE	19.733	228484	1.735 ug/ml
16) N-HEXATRIACONTANE	20.472	150855	1.225 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111422\
Data File : FF011722.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2022 05:38
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 15 07:10:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

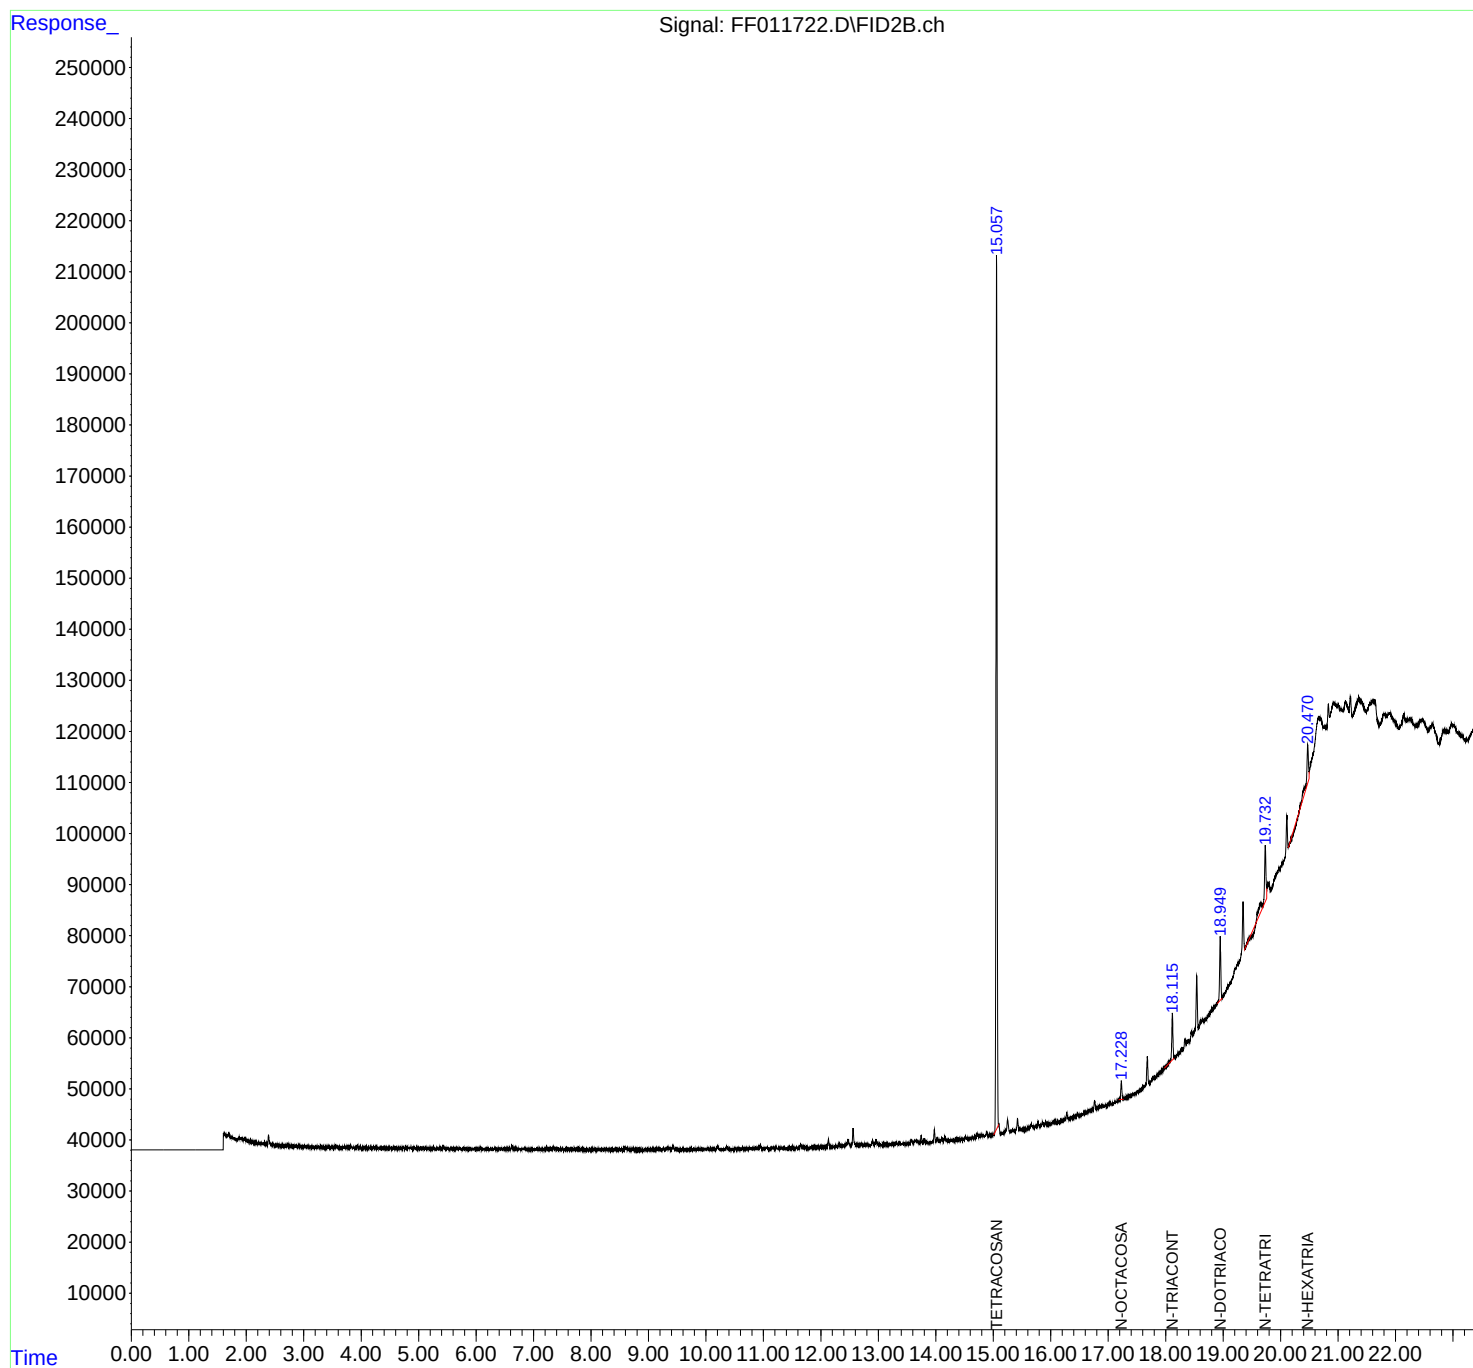


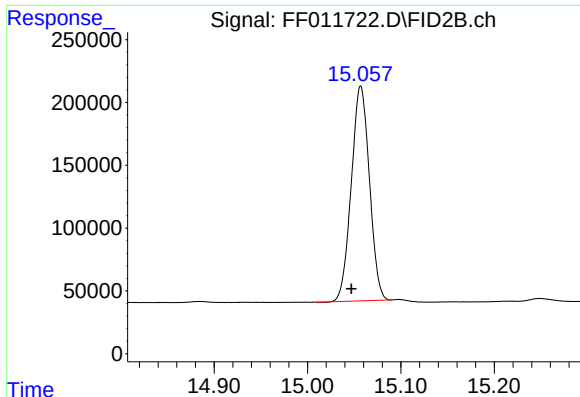

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.057 min
Delta R.T.: 0.010 min
Response: 2306138
Conc: 19.44 ug/ml

Instrument :
FID_F
ClientSampleId :

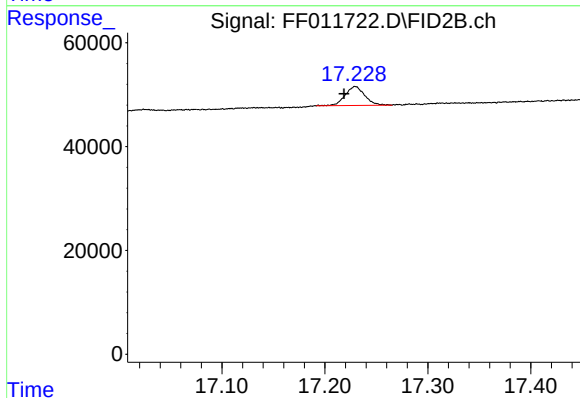


#12 N-OCTACOSANE

R.T.: 17.230 min
Delta R.T.: 0.011 min
Response: 47768
Conc: 0.36 ug/ml

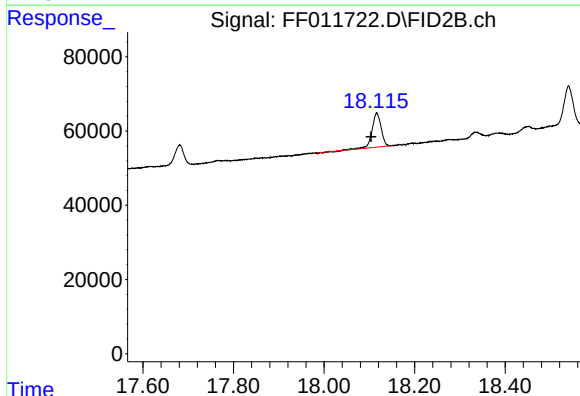


#13 N-TRIACONTANE

R.T.: 18.116 min
Delta R.T.: 0.013 min
Response: 127201
Conc: 0.96 ug/ml

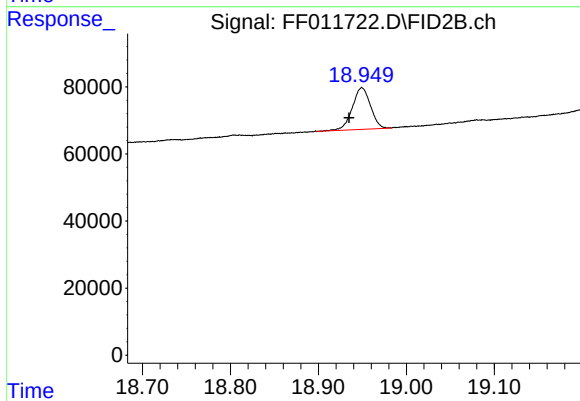

#14 N-DOTRIACONTANE


R.T.: 18.950 min
Delta R.T.: 0.014 min
Response: 178171
Conc: 1.32 ug/ml

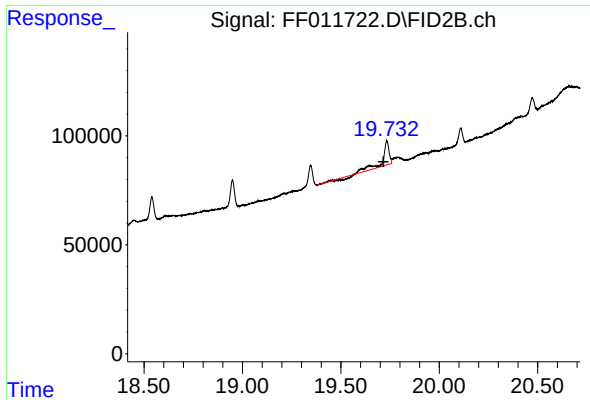

#15 N-TETRATRIACONTANE

R.T.: 19.733 min
Delta R.T.: 0.017 min
Response: 228484
Conc: 1.73 ug/ml

Instrument :
FID_F
ClientSampleId :

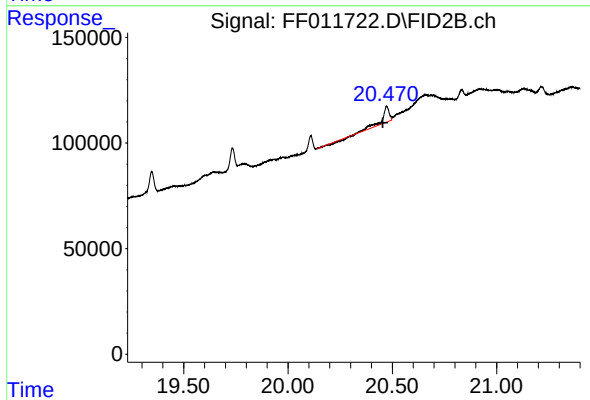

#16 N-HEXATRIACONTANE

R.T.: 20.472 min
Delta R.T.: 0.018 min
Response: 150855
Conc: 1.22 ug/ml