

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111422\
Data File : FF011691.D
Signal(s) : FID2B.ch
Acq On : 14 Nov 2022 11:33
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 14 13:01:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.767	2990032	22.247 ug/ml
12) N-OCTACOSANE	17.233	2720848	20.538 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111422\
Data File : FF011691.D
Signal(s) : FID2B.ch
Acq On : 14 Nov 2022 11:33
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 14 13:01:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

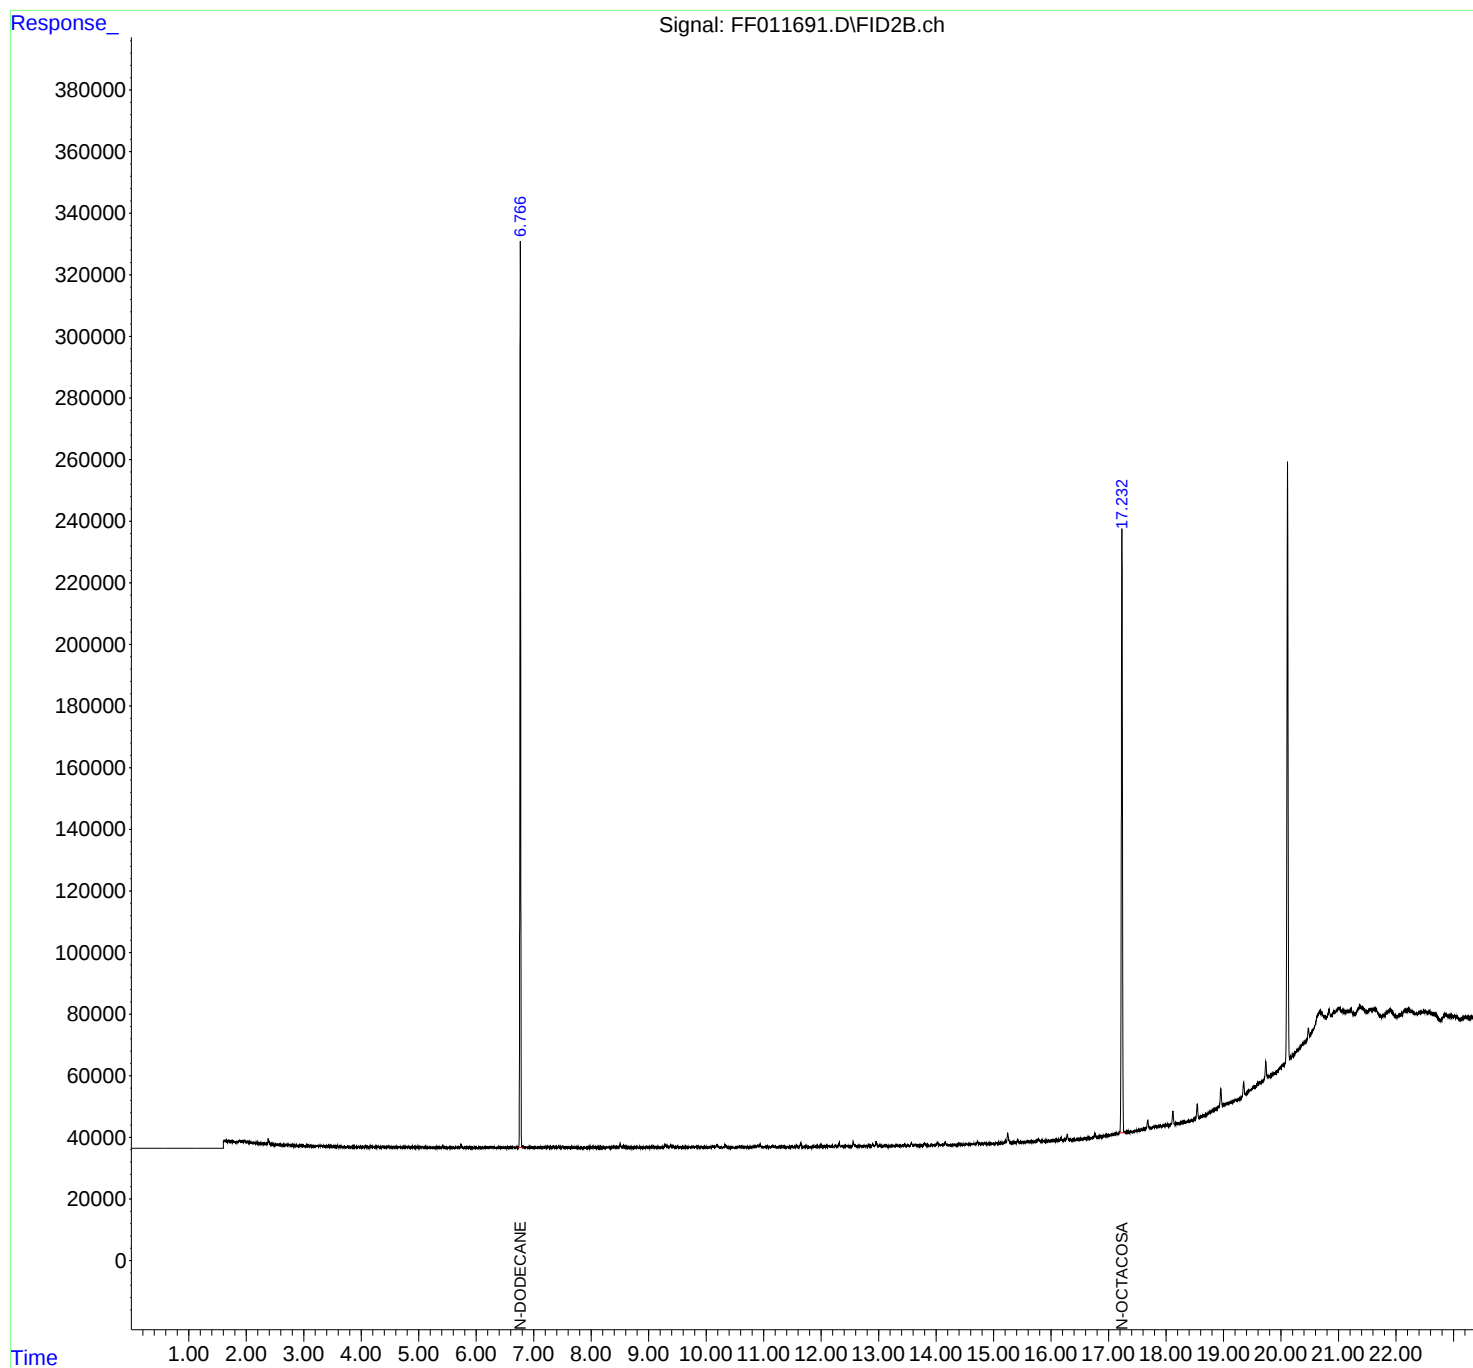


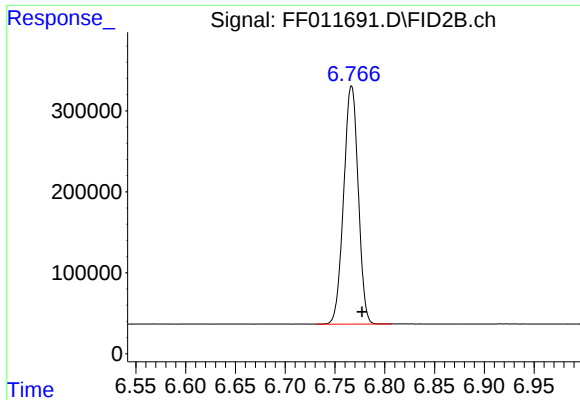

#3 N-DODECANE


R.T.: 6.767 min
Delta R.T.: -0.011 min
Response: 2990032
Conc: 22.25 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

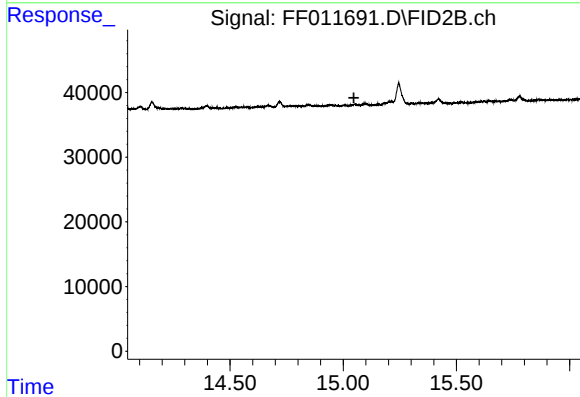

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.047 min
Response: 0
Conc: N.D.

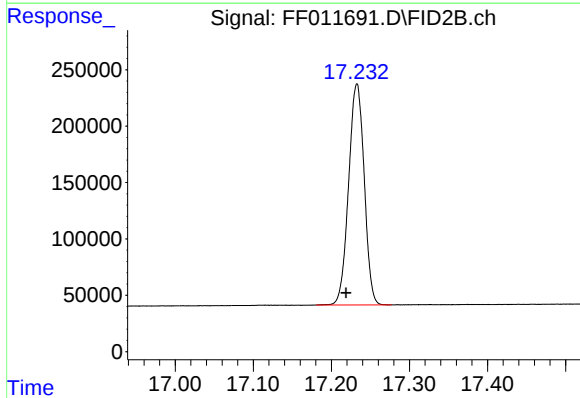

#12 N-OCTACOSANE

R.T.: 17.233 min
Delta R.T.: 0.014 min
Response: 2720848
Conc: 20.54 ug/ml