

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF111422\  
Data File : FF011698.D  
Signal(s) : FID2B.ch  
Acq On : 14 Nov 2022 14:58  
Operator : YP\AJ  
Sample : N5578-11RE  
Misc :  
ALS Vial : 62 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
CAC-HPT-2-GW-(20-23)RE

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/15/2022  
Supervised By :Ankita Jodhani 11/15/2022

Integration File: autoint1.e  
Quant Time: Nov 15 04:48:03 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF110422.M  
Quant Title :  
QLast Update : Fri Nov 04 14:11:34 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.057 | 549768   | 4.634 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF111422\  
Data File : FF011698.D  
Signal(s) : FID2B.ch  
Acq On : 14 Nov 2022 14:58  
Operator : YP\AJ  
Sample : N5578-11RE  
Misc :  
ALS Vial : 62 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
CAC-HPT-2-GW-(20-23)RE


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/15/2022  
Supervised By :Ankita Jodhani 11/15/2022

Integration File: autoint1.e  
Quant Time: Nov 15 04:48:03 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF110422.M  
Quant Title :  
QLast Update : Fri Nov 04 14:11:34 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

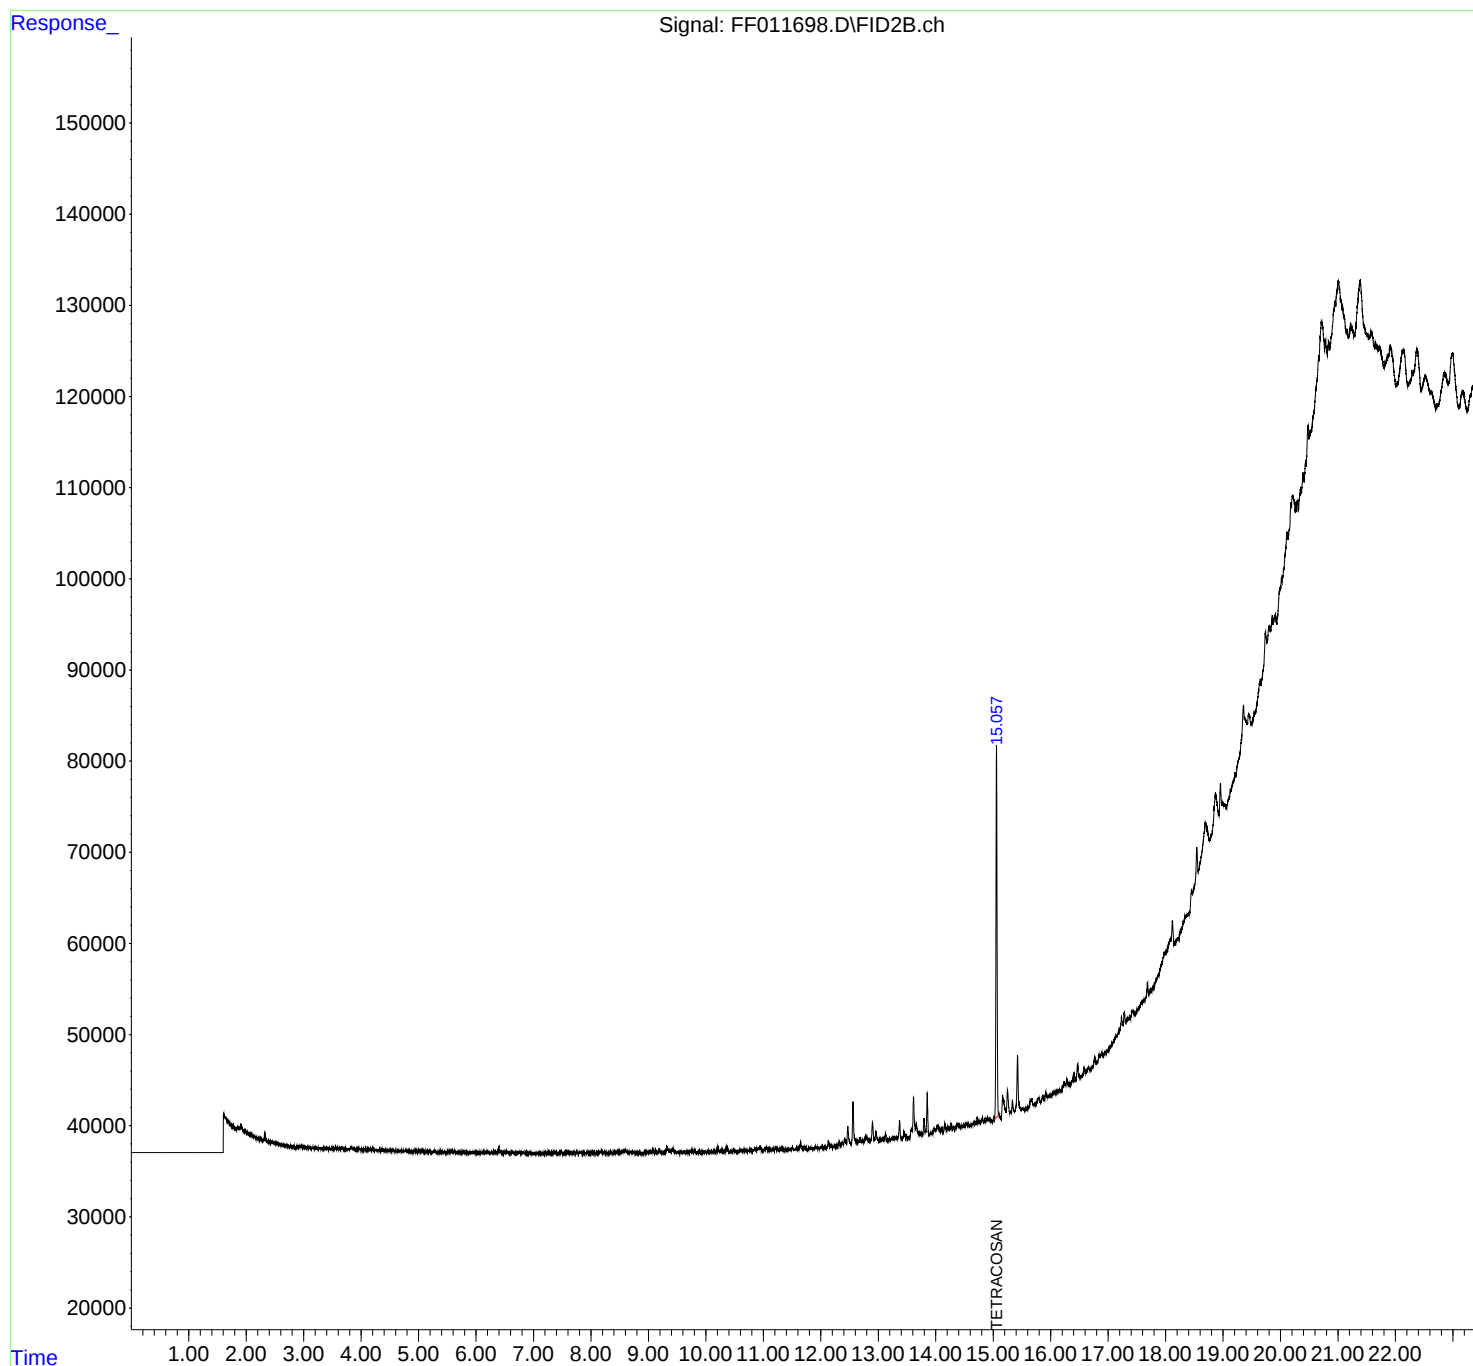

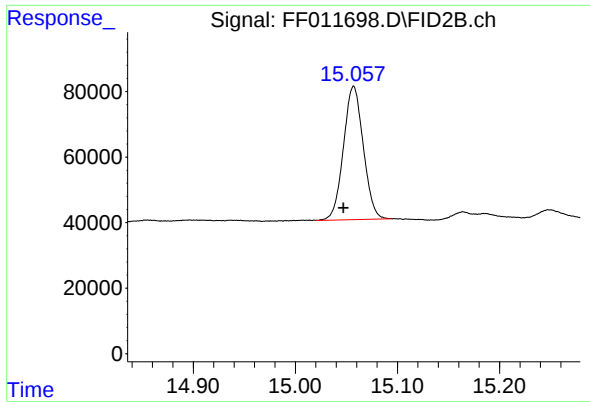

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.057 min  
Delta R.T.: 0.010 min  
Response: 549768  
Conc: 4.63 ug/ml

Instrument : FID\_F  
ClientSampleId : CAC-HPT-2-GW-(20-23)RE

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/15/2022  
Supervised By :Ankita Jodhani 11/15/2022