

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111422\
 Data File : FF011707.D
 Signal(s) : FID2B.ch
 Acq On : 14 Nov 2022 19:53
 Operator : YP\AJ
 Sample : PB149018BS
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB149018BS

Integration File: autoint1.e
 Quant Time: Nov 15 04:49:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	2015471	16.987 ug/ml
Target Compounds			
2) N-DECANE	4.614	2277619	17.257 ug/ml
3) N-DODECANE	6.775	2334147	17.367 ug/ml
4) N-TETRADECANE	8.600	2366565	17.488 ug/ml
5) N-HEXADECANE	10.205	2398041	17.443 ug/ml
6) N-OCTADECANE	11.648	2424430	17.527 ug/ml
7) N-EICOSANE	12.958	2366612	17.112 ug/ml
8) N-DOCOSANE	14.155	2309830	17.113 ug/ml
10) N-TETRACOSANE	15.258	2306245	17.006 ug/ml
11) N-HEXACOSANE	16.279	2224632	16.651 ug/ml
12) N-OCTACOSANE	17.229	2166364	16.352 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111422\
Data File : FF011707.D
Signal(s) : FID2B.ch
Acq On : 14 Nov 2022 19:53
Operator : YP\AJ
Sample : PB149018BS
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB149018BS

Integration File: autoint1.e
Quant Time: Nov 15 04:49:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

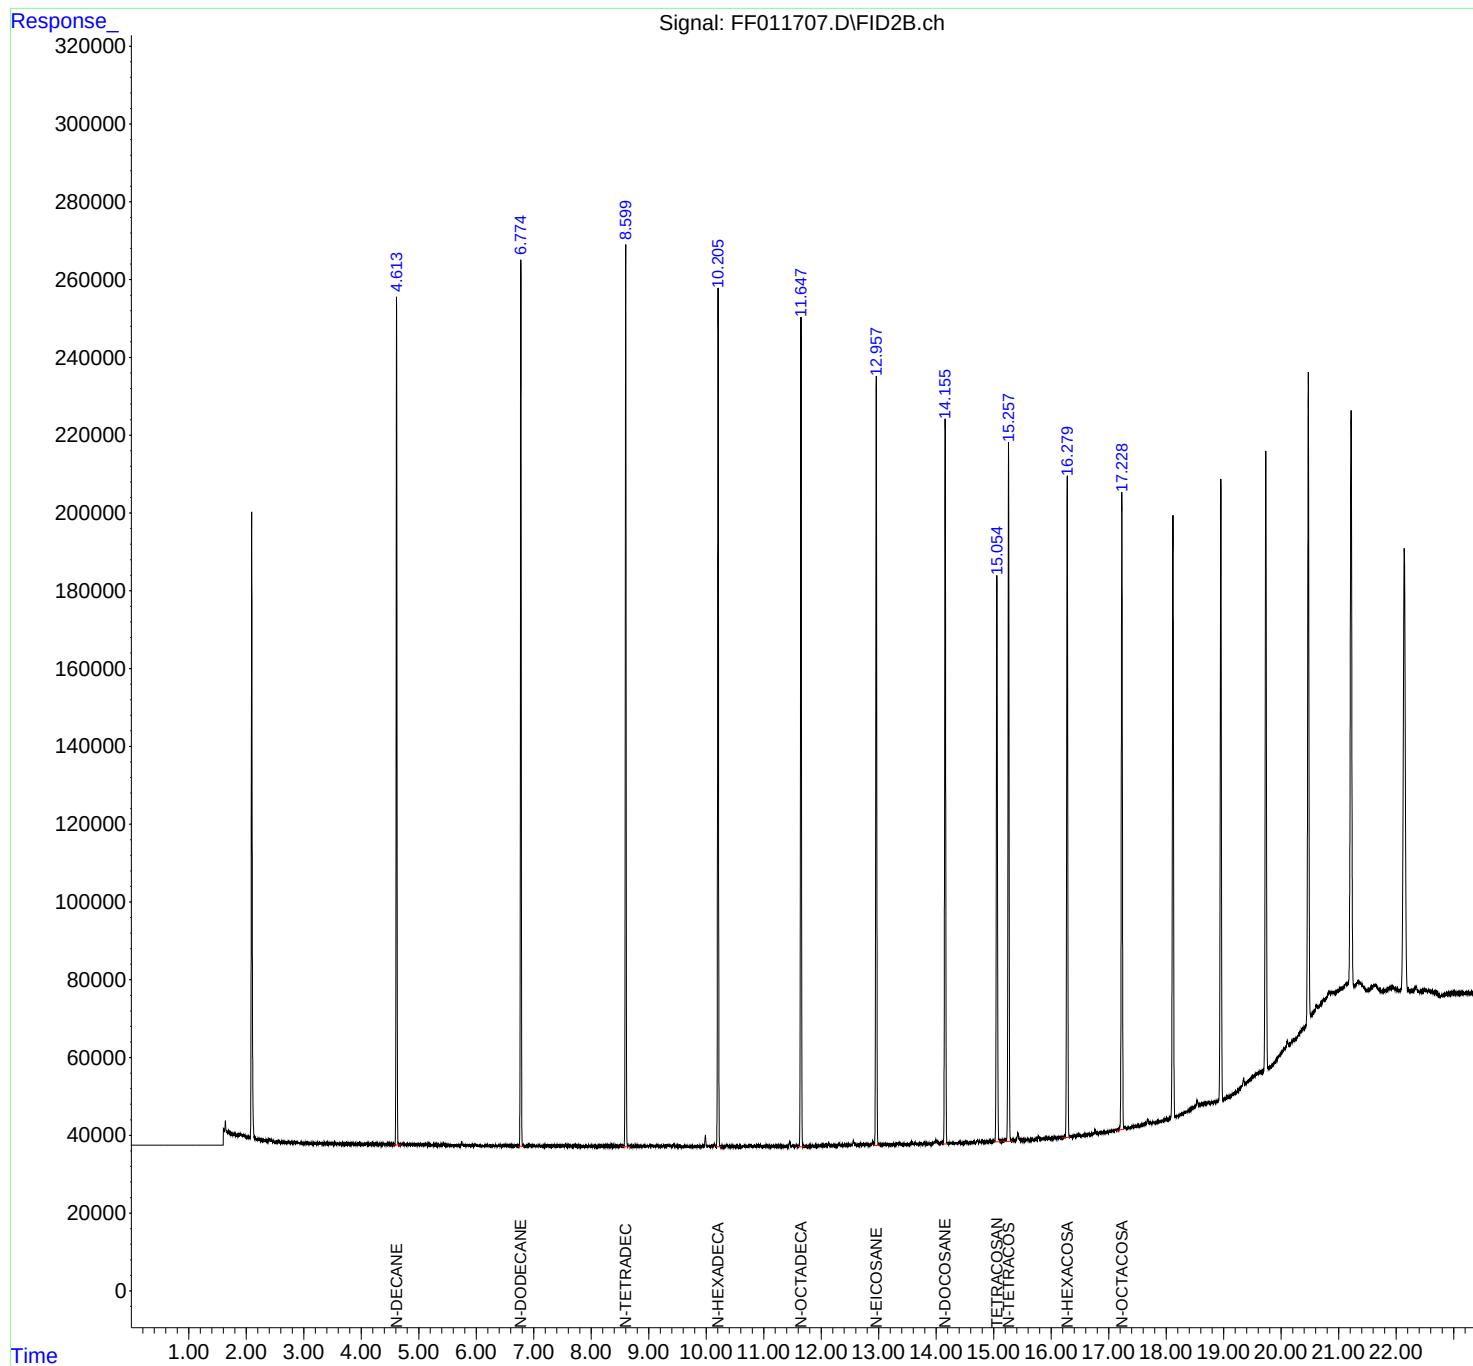


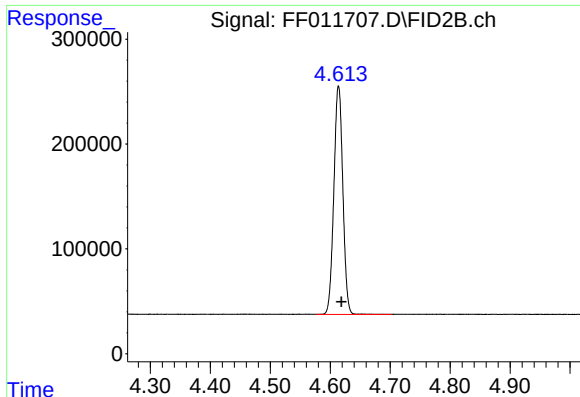

#2 N-DECANE


R.T.: 4.614 min
Delta R.T.: -0.004 min
Response: 2277619
Conc: 17.26 ug/ml

Instrument :
FID_F
ClientSampleId :
PB149018BS

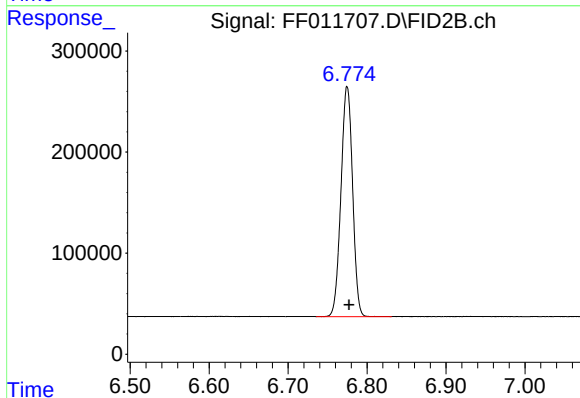


#3 N-DODECANE

R.T.: 6.775 min
Delta R.T.: -0.002 min
Response: 2334147
Conc: 17.37 ug/ml

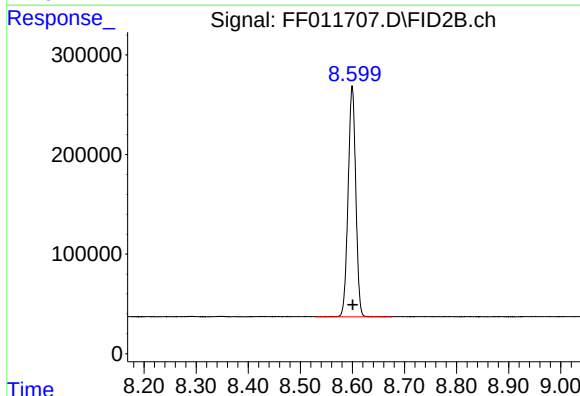


#4 N-TETRADECANE

R.T.: 8.600 min
Delta R.T.: -0.001 min
Response: 2366565
Conc: 17.49 ug/ml

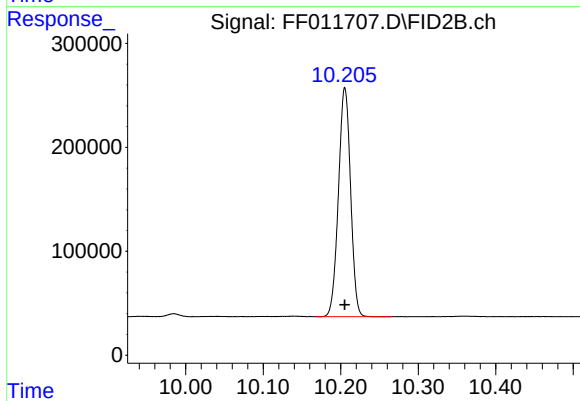

#5 N-HEXADECANE


R.T.: 10.205 min
Delta R.T.: 0.000 min
Response: 2398041
Conc: 17.44 ug/ml

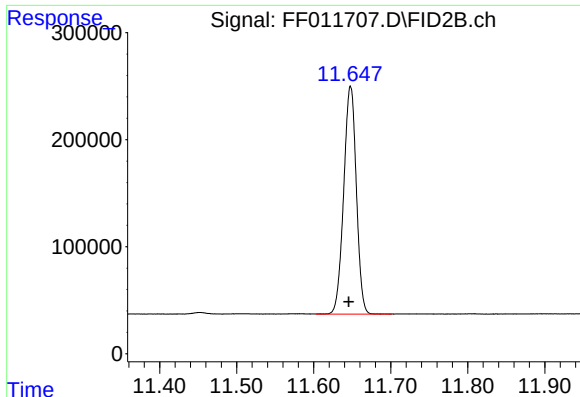

#6 N-OCTADECANE


R.T.: 11.648 min
Delta R.T.: 0.002 min
Response: 2424430
Conc: 17.53 ug/ml

Instrument :
FID_F
ClientSampleId :
PB149018BS

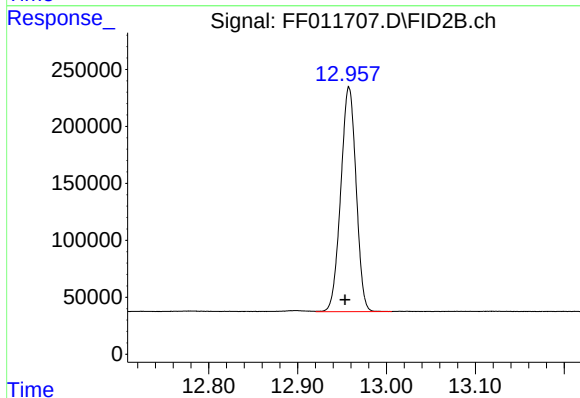


#7 N-EICOSANE

R.T.: 12.958 min
Delta R.T.: 0.004 min
Response: 2366612
Conc: 17.11 ug/ml

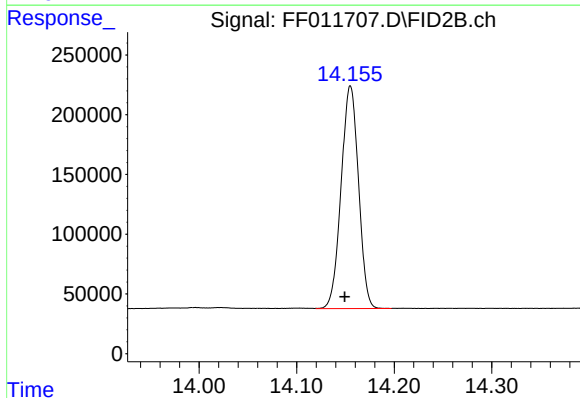


#8 N-DOCOSANE

R.T.: 14.155 min
Delta R.T.: 0.006 min
Response: 2309830
Conc: 17.11 ug/ml

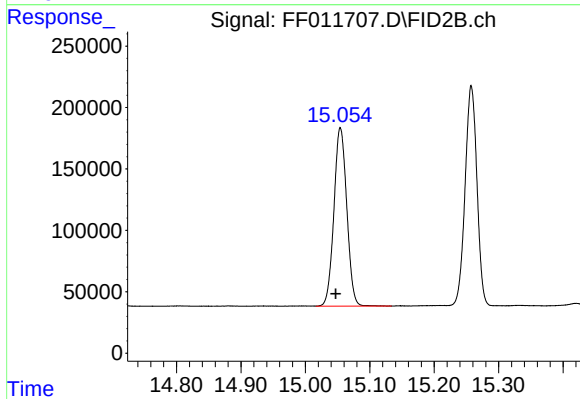

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.054 min
Delta R.T.: 0.007 min
Response: 2015471
Conc: 16.99 ug/ml

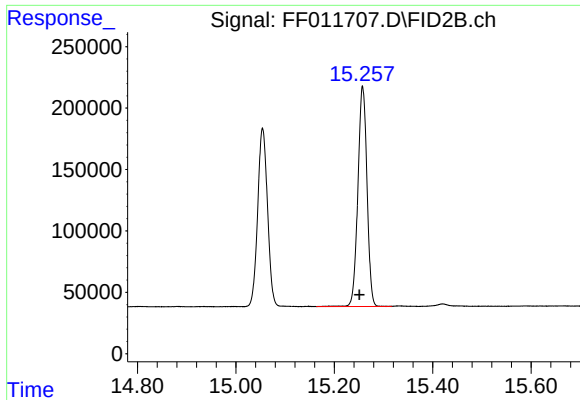

#10 N-TETRACOSANE


R.T.: 15.258 min
Delta R.T.: 0.007 min
Response: 2306245
Conc: 17.01 ug/ml

Instrument :
FID_F
ClientSampleId :
PB149018BS

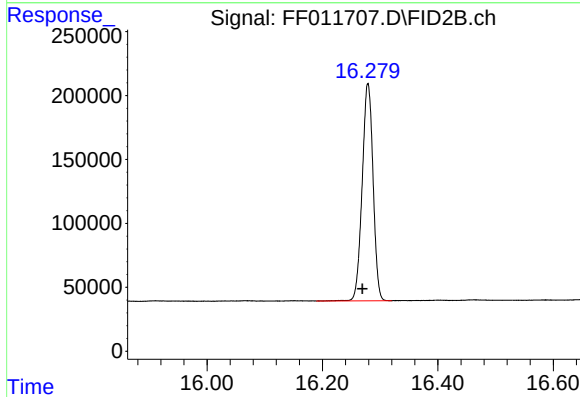

#11 N-HEXACOSANE

R.T.: 16.279 min
Delta R.T.: 0.010 min
Response: 2224632
Conc: 16.65 ug/ml

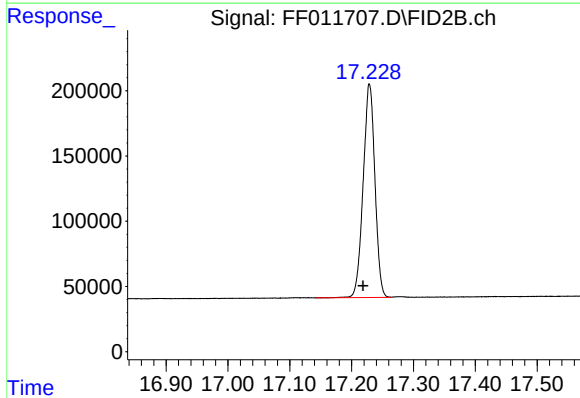

#12 N-OCTACOSANE

R.T.: 17.229 min
Delta R.T.: 0.010 min
Response: 2166364
Conc: 16.35 ug/ml