

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111425\
Data File : FF016705.D
Signal(s) : FID2B.ch
Acq On : 14 Nov 2025 11:08
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 13:24:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	18.125	100332	0.893 ug/ml
14)	N-DOTRIACONTANE	18.960	168650	1.573 ug/ml
15)	N-TETRATRIACONTANE	19.748	141718	1.442 ug/ml
16)	N-HEXATRIACONTANE	20.492	97363	1.139 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111425\
Data File : FF016705.D
Signal(s) : FID2B.ch
Acq On : 14 Nov 2025 11:08
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 13:24:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

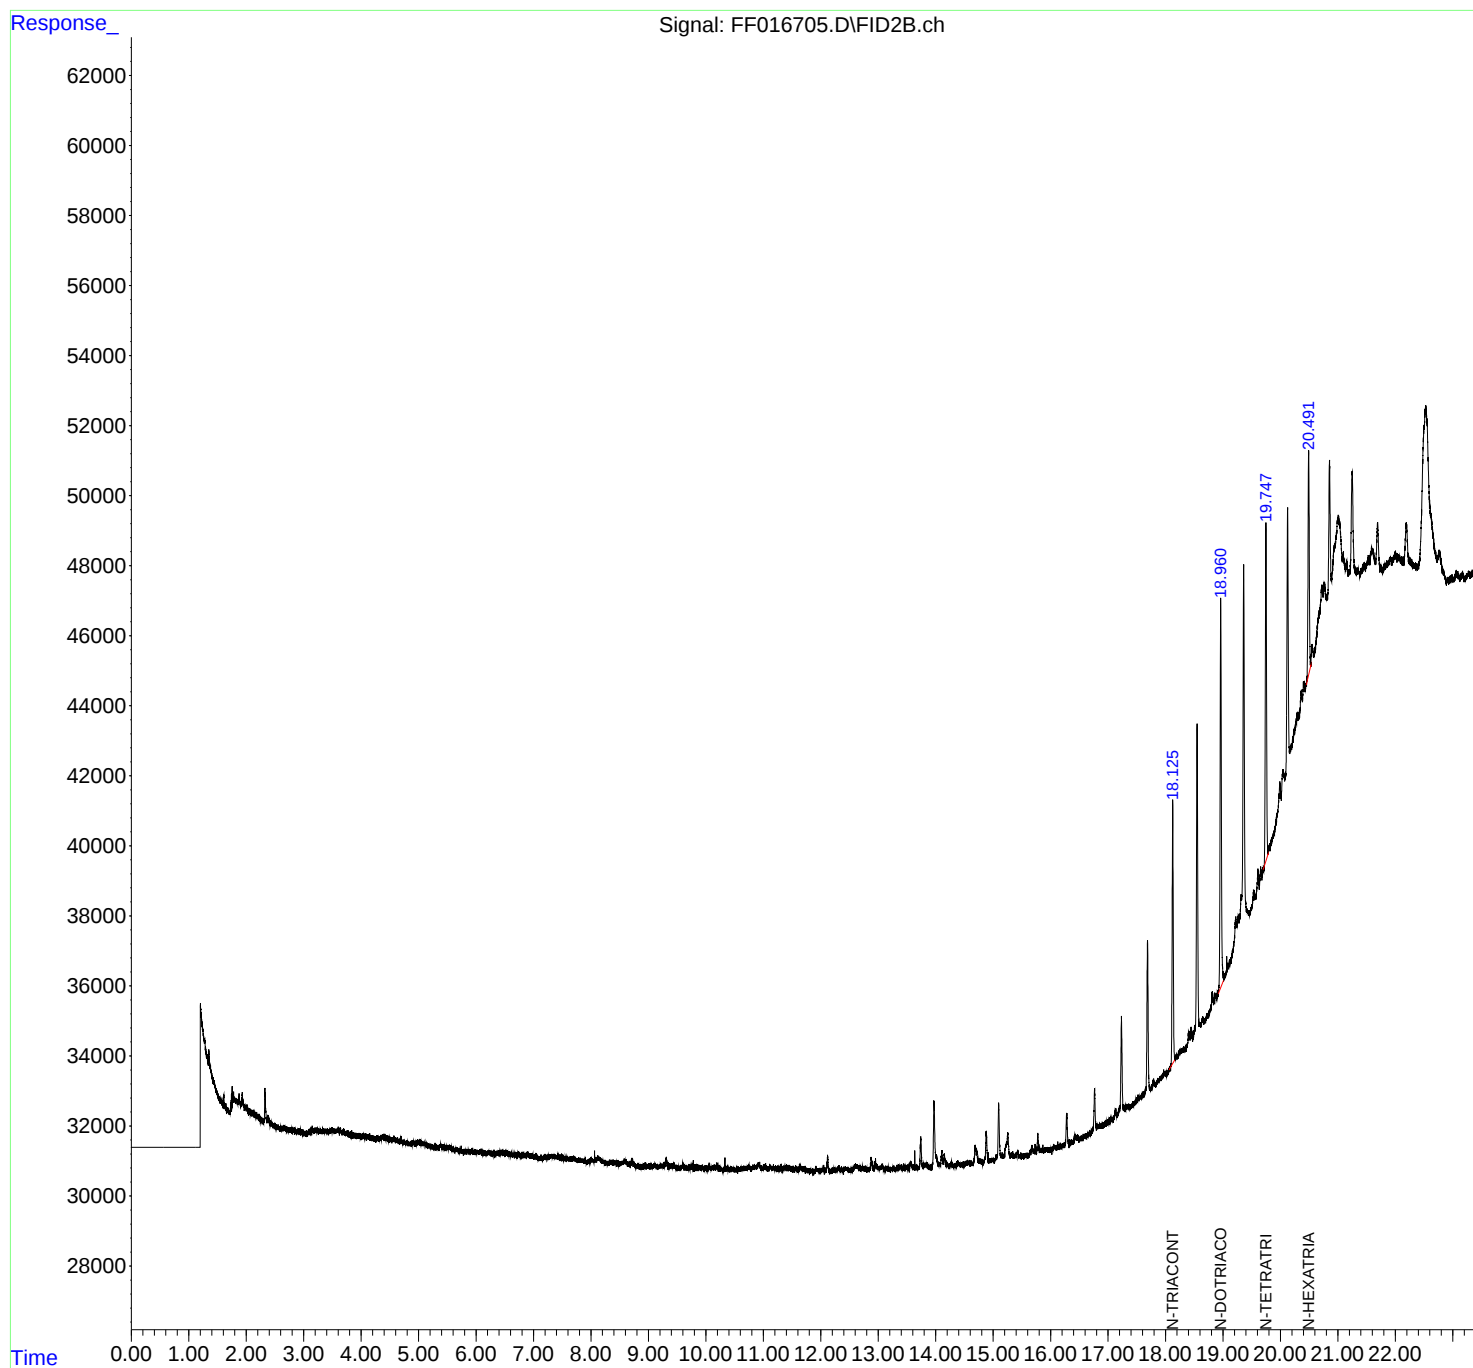


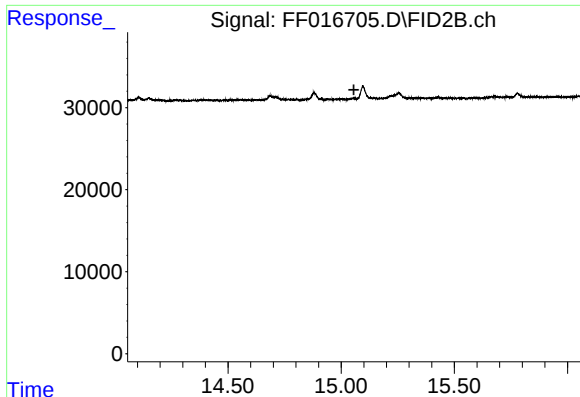

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.056 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

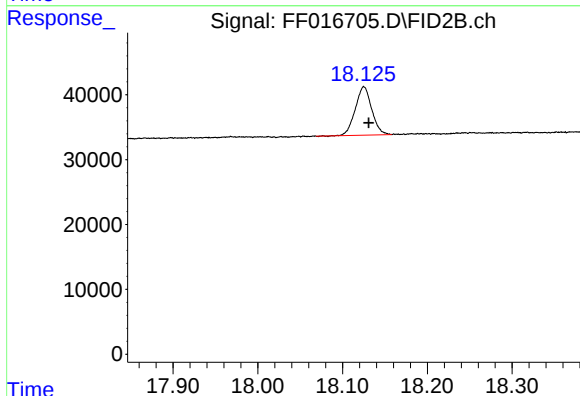


#13 N-TRIACONTANE

R.T.: 18.125 min
Delta R.T.: -0.006 min
Response: 100332
Conc: 0.89 ug/ml

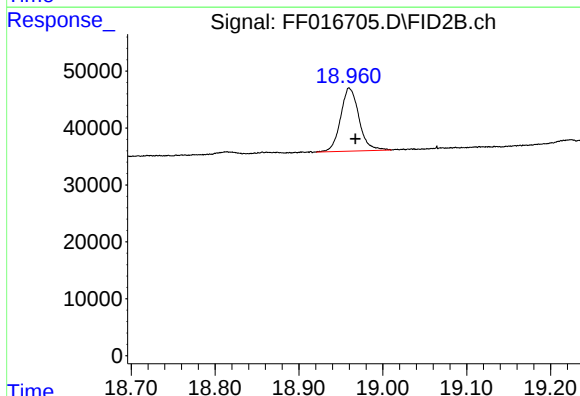


#14 N-DOTRIACONTANE

R.T.: 18.960 min
Delta R.T.: -0.007 min
Response: 168650
Conc: 1.57 ug/ml

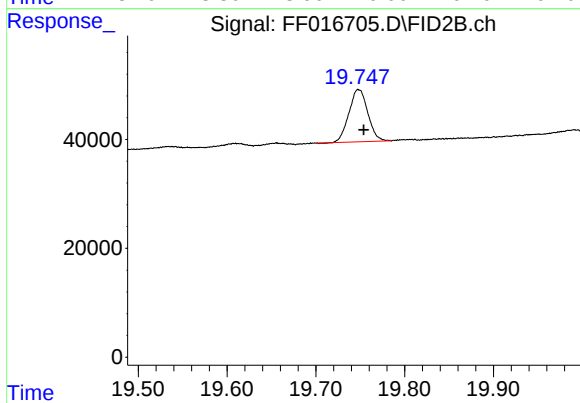

#15 N-TETRATRIACONTANE

R.T.: 19.748 min
Delta R.T.: -0.006 min
Response: 141718
Conc: 1.44 ug/ml

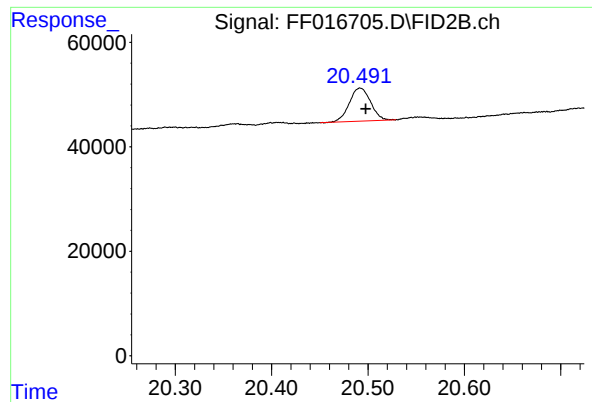

#16 N-HEXATRIACONTANE

R.T.: 20.492 min
Delta R.T.: -0.006 min
Response: 97363
Conc: 1.14 ug/ml

Instrument :

FID_F

ClientSampleId :