

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111425\
Data File : FF016711.D
Signal(s) : FID2B.ch
Acq On : 14 Nov 2025 14:48
Operator : YP\AJ
Sample : Q3610-10RE
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 15:02:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.051	816687	7.817 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.958	67749	0.632 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111425\
Data File : FF016711.D
Signal(s) : FID2B.ch
Acq On : 14 Nov 2025 14:48
Operator : YP\AJ
Sample : Q3610-10RE
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 15:02:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

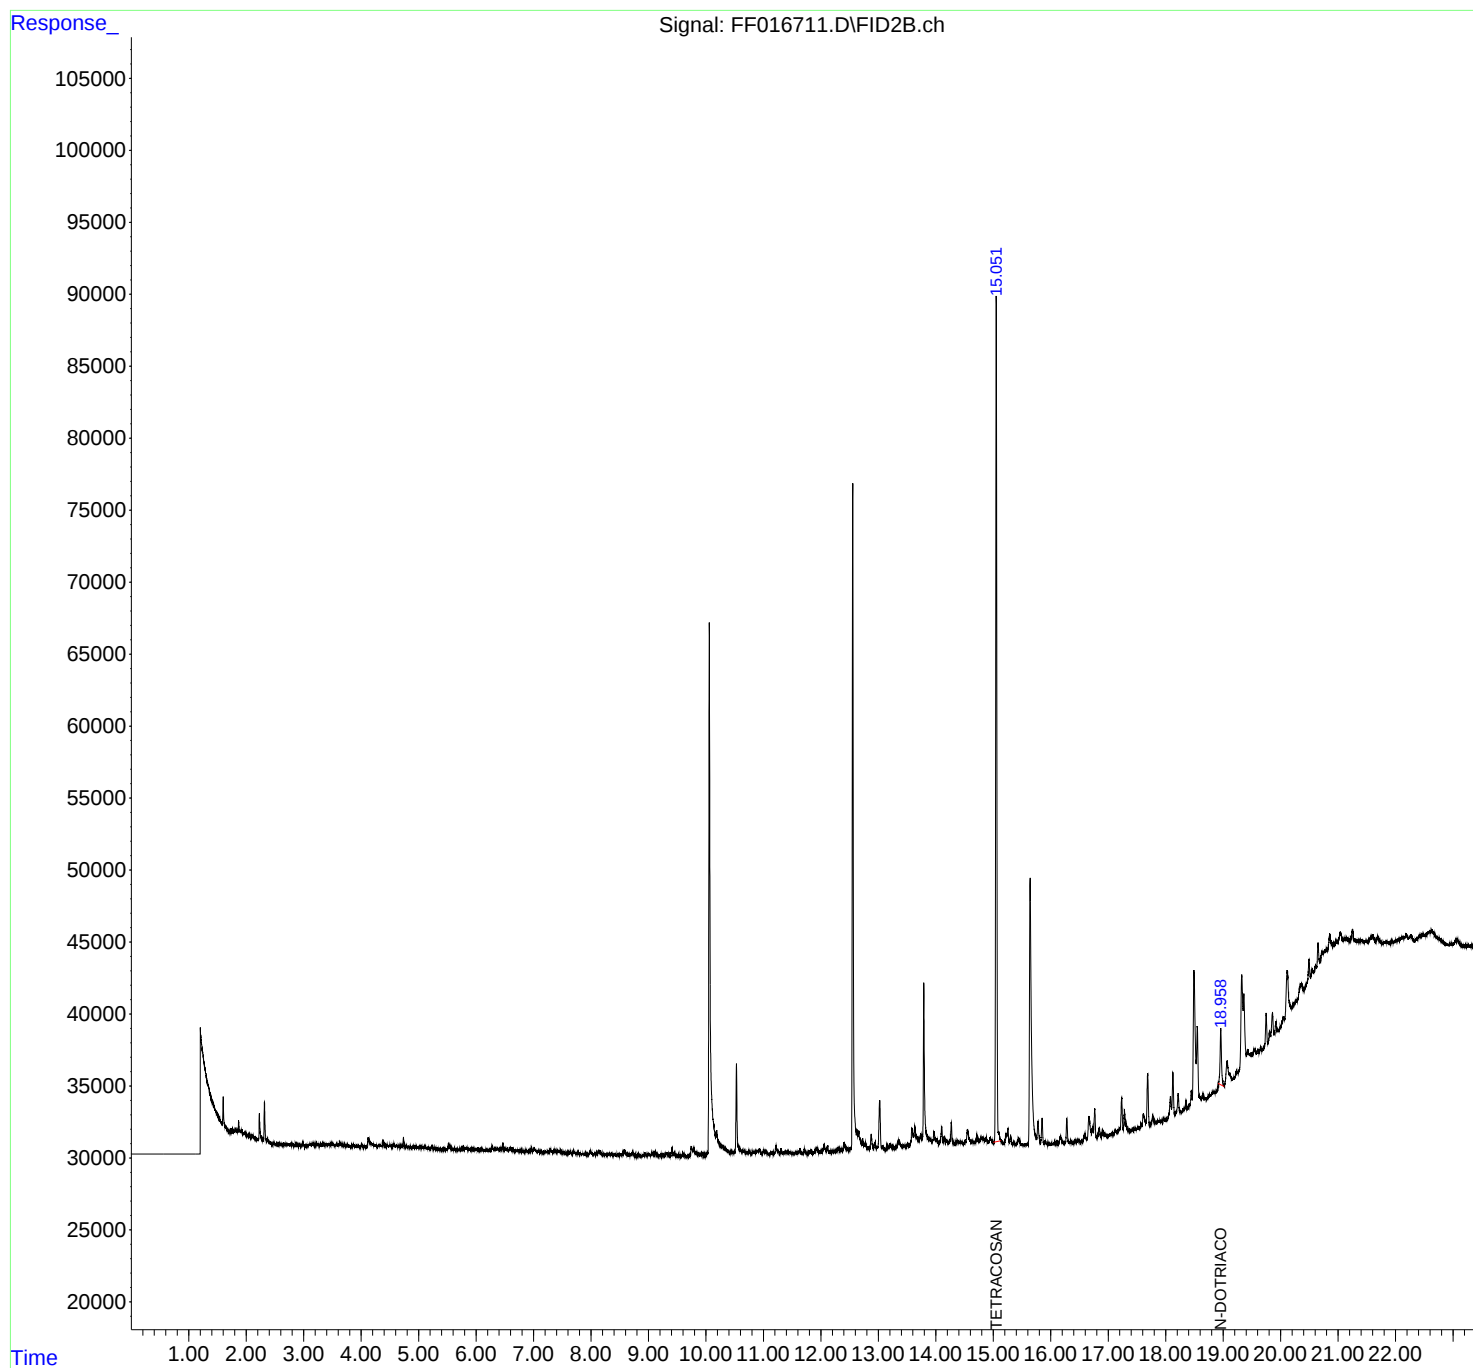


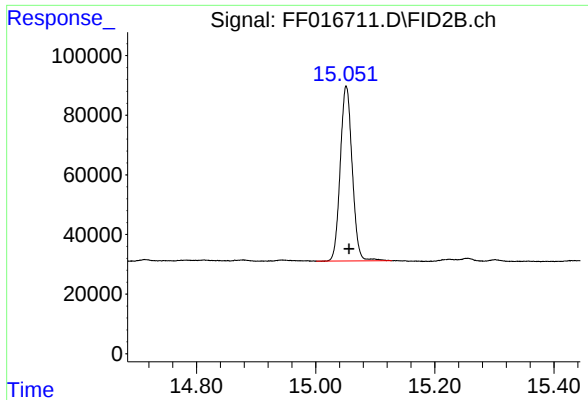

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.051 min
Delta R.T.: -0.005 min
Response: 816687
Conc: 7.82 ug/ml

Instrument :
FID_F
ClientSampleId :

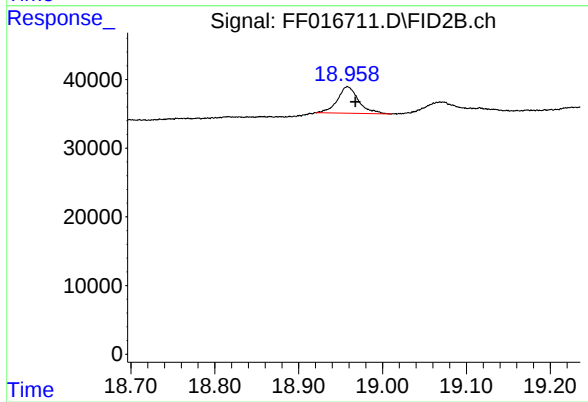

#14 N-DOTRIACONTANE

R.T.: 18.958 min
Delta R.T.: -0.009 min
Response: 67749
Conc: 0.63 ug/ml