

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111518\
Data File : FF002697.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2018 09:18
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 15 12:35:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.689	117586	1.383 ug/ml
Target Compounds				
3)	N-DODECANE	6.364	8349	0.062 ug/ml
4)	N-TETRADECANE	8.183	87419	0.683 ug/ml
5)	N-HEXADECANE	9.808	34721	0.288 ug/ml
6)	N-OCTADECANE	11.207	76762	0.672 ug/ml
7)	N-EICOSANE	12.584	72232	0.683 ug/ml
8)	N-DOCOSANE	13.776	60063	0.601 ug/ml
10)	N-TETRACOSANE	14.850	122625	1.269 ug/ml
11)	N-HEXACOSANE	15.873	135960	1.388 ug/ml
12)	N-OCTACOSANE	16.824	124333	1.203 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111518\
Data File : FF002697.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2018 09:18
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 15 12:35:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

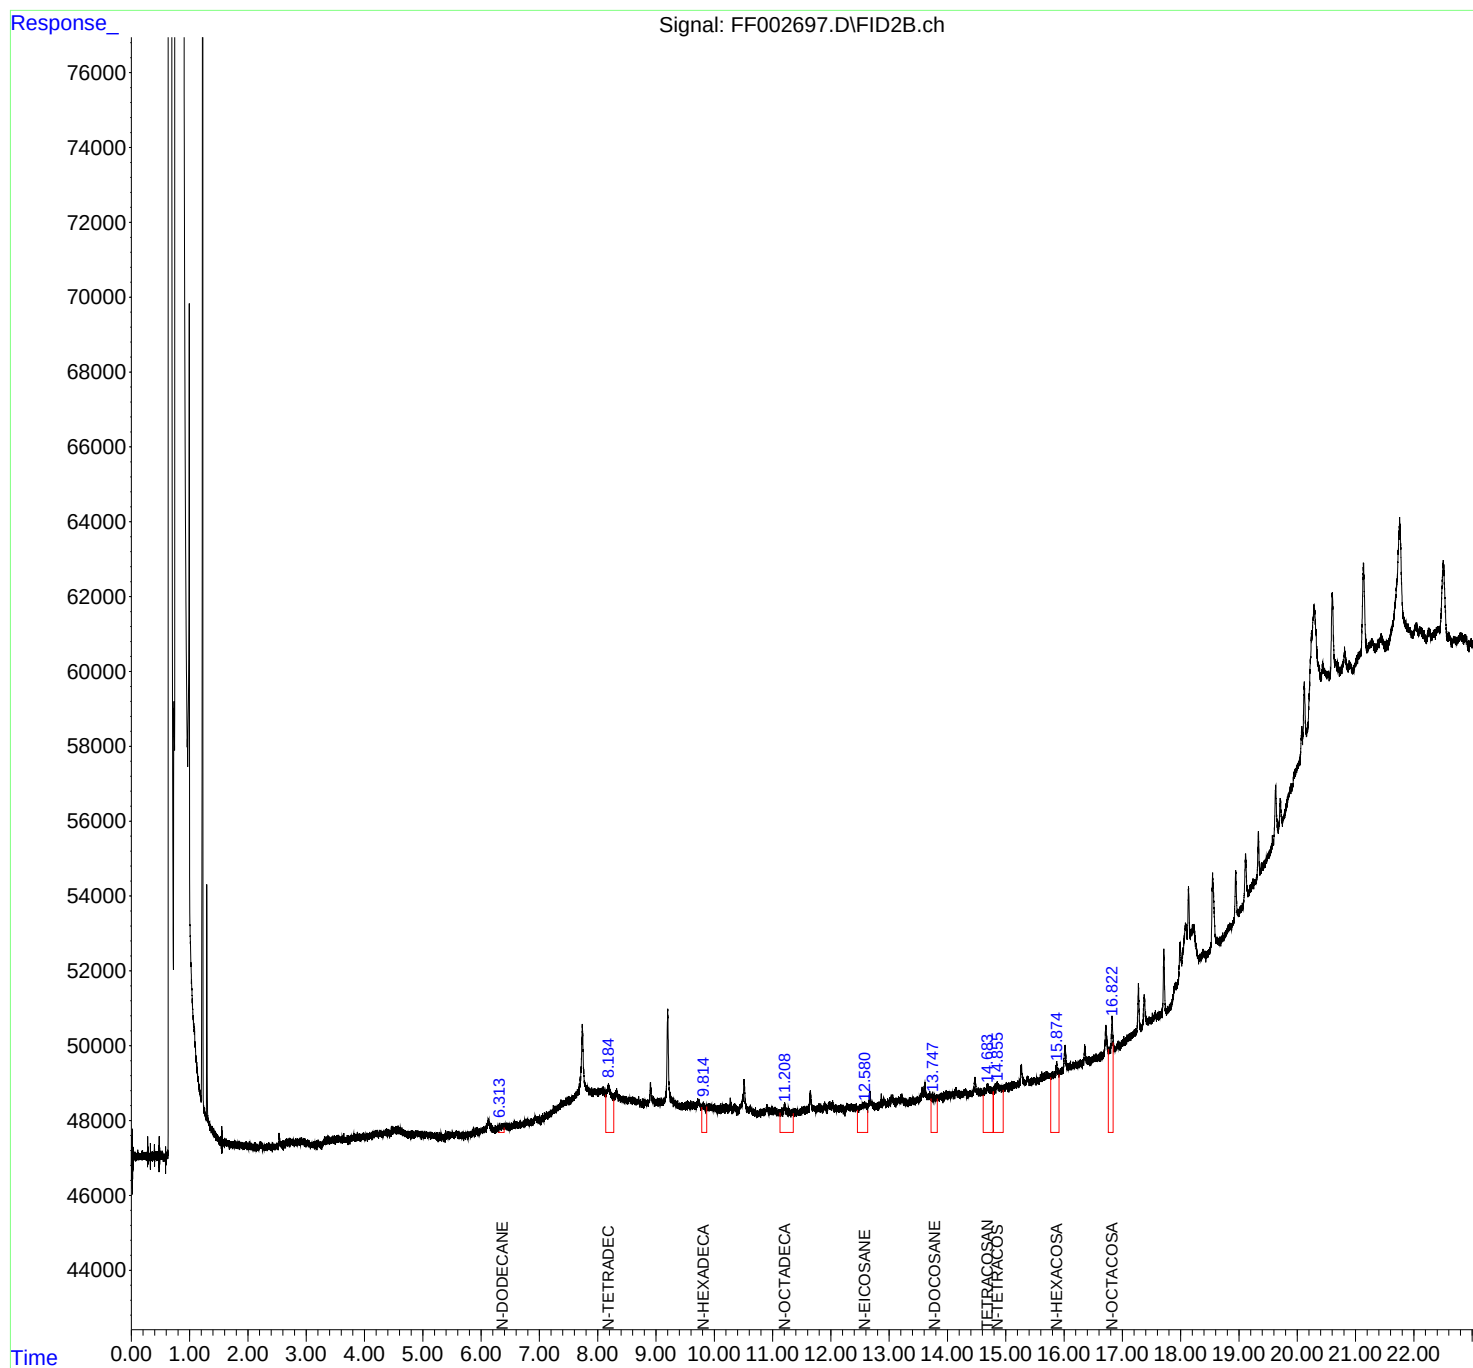

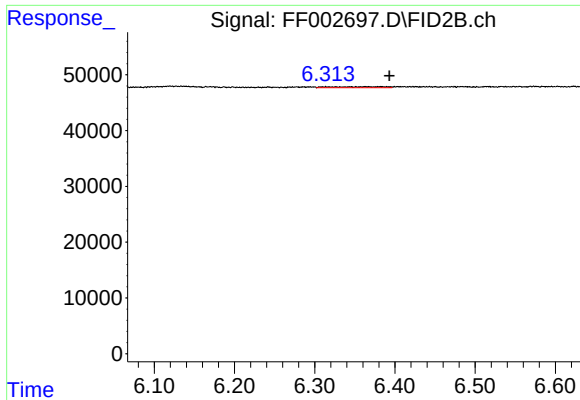


#3 N-DODECANE

R.T.: 6.364 min
Delta R.T.: -0.029 min
Response: 8349
Conc: 0.06 ug/ml

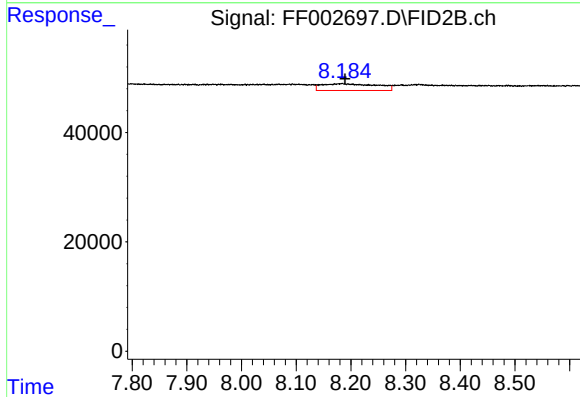


#4 N-TETRADECANE

R.T.: 8.183 min
Delta R.T.: -0.007 min
Response: 87419
Conc: 0.68 ug/ml

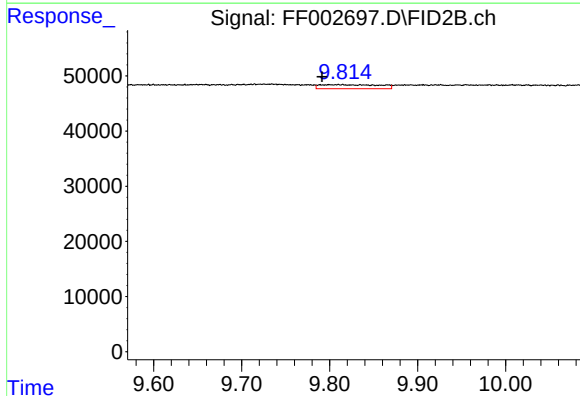


#5 N-HEXADECANE

R.T.: 9.808 min
Delta R.T.: 0.017 min
Response: 34721
Conc: 0.29 ug/ml

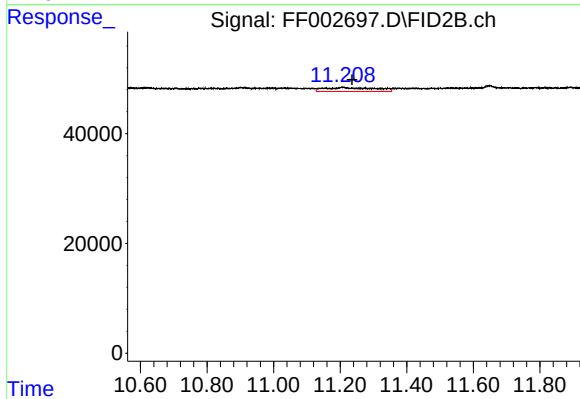


#6 N-OCTADECANE

R.T.: 11.207 min
Delta R.T.: -0.028 min
Response: 76762
Conc: 0.67 ug/ml

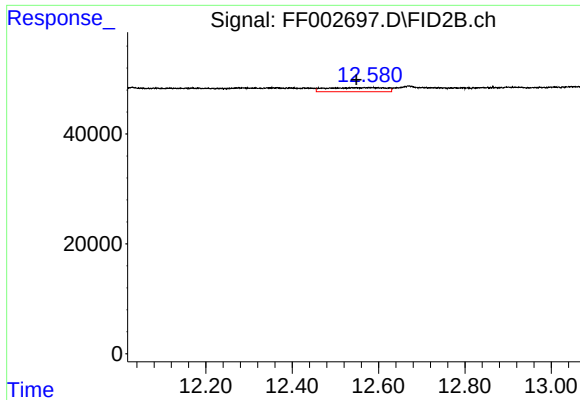


#7 N-EICOSANE

R.T.: 12.584 min
Delta R.T.: 0.036 min
Response: 72232
Conc: 0.68 ug/ml

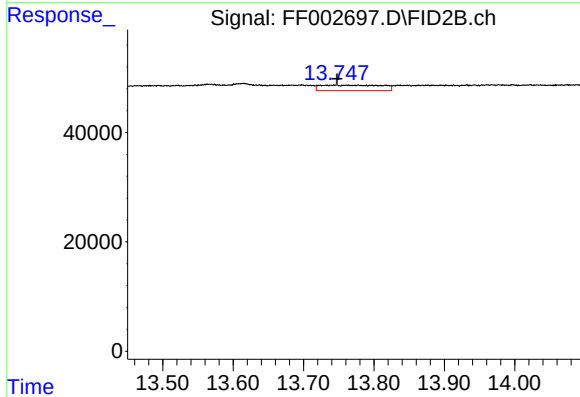


#8 N-DOCOSANE

R.T.: 13.776 min
Delta R.T.: 0.029 min
Response: 60063
Conc: 0.60 ug/ml

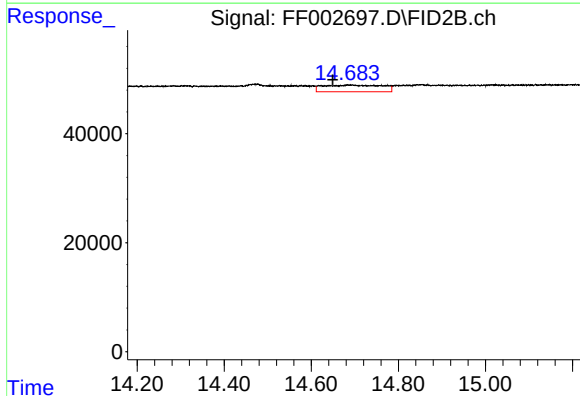


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.689 min
Delta R.T.: 0.040 min
Response: 117586
Conc: 1.38 ug/ml

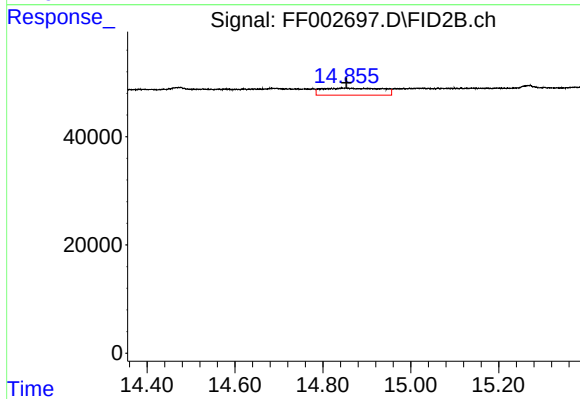


#10 N-TETRACOSANE

R.T.: 14.850 min
Delta R.T.: -0.004 min
Response: 122625
Conc: 1.27 ug/ml

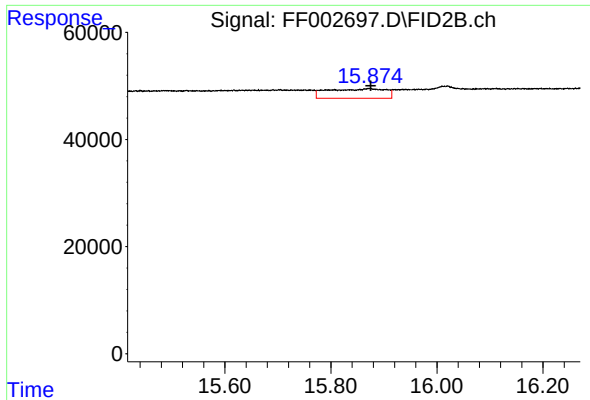

#11 N-HEXACOSANE

R.T.: 15.873 min
Delta R.T.: -0.002 min
Response: 135960
Conc: 1.39 ug/ml

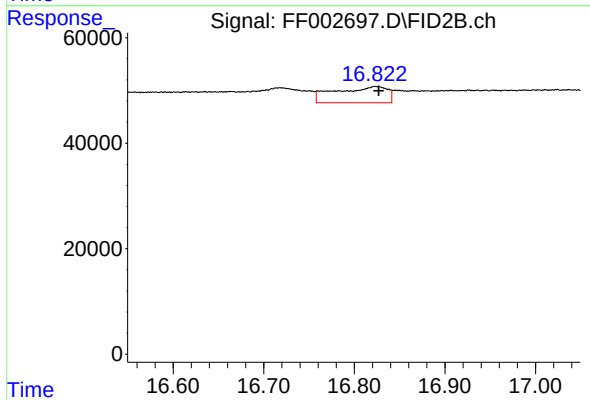

#12 N-OCTACOSANE

R.T.: 16.824 min
Delta R.T.: -0.003 min
Response: 124333
Conc: 1.20 ug/ml