

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111518\
 Data File : FF002701.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2018 11:18
 Operator : AJ\SJ
 Sample : J5925-05 50X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 15 12:35:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.646	97366	1.145 ug/ml
Target Compounds				
3)	N-DODECANE	6.388	68134	0.507 ug/ml
4)	N-TETRADECANE	8.204	247993	1.937 ug/ml
5)	N-HEXADECANE	9.794	564346	4.688 ug/ml
6)	N-OCTADECANE	11.226	175059	1.533 ug/ml
7)	N-EICOSANE	12.545	209149	1.976 ug/ml
8)	N-DOCOSANE	13.759	67909	0.679 ug/ml
10)	N-TETRACOSANE	14.853	15592	0.161 ug/ml
11)	N-HEXACOSANE	15.873	11148	0.114 ug/ml
12)	N-OCTACOSANE	16.824	38904	0.376 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111518\
Data File : FF002701.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2018 11:18
Operator : AJ\SJ
Sample : J5925-05 50X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 15 12:35:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

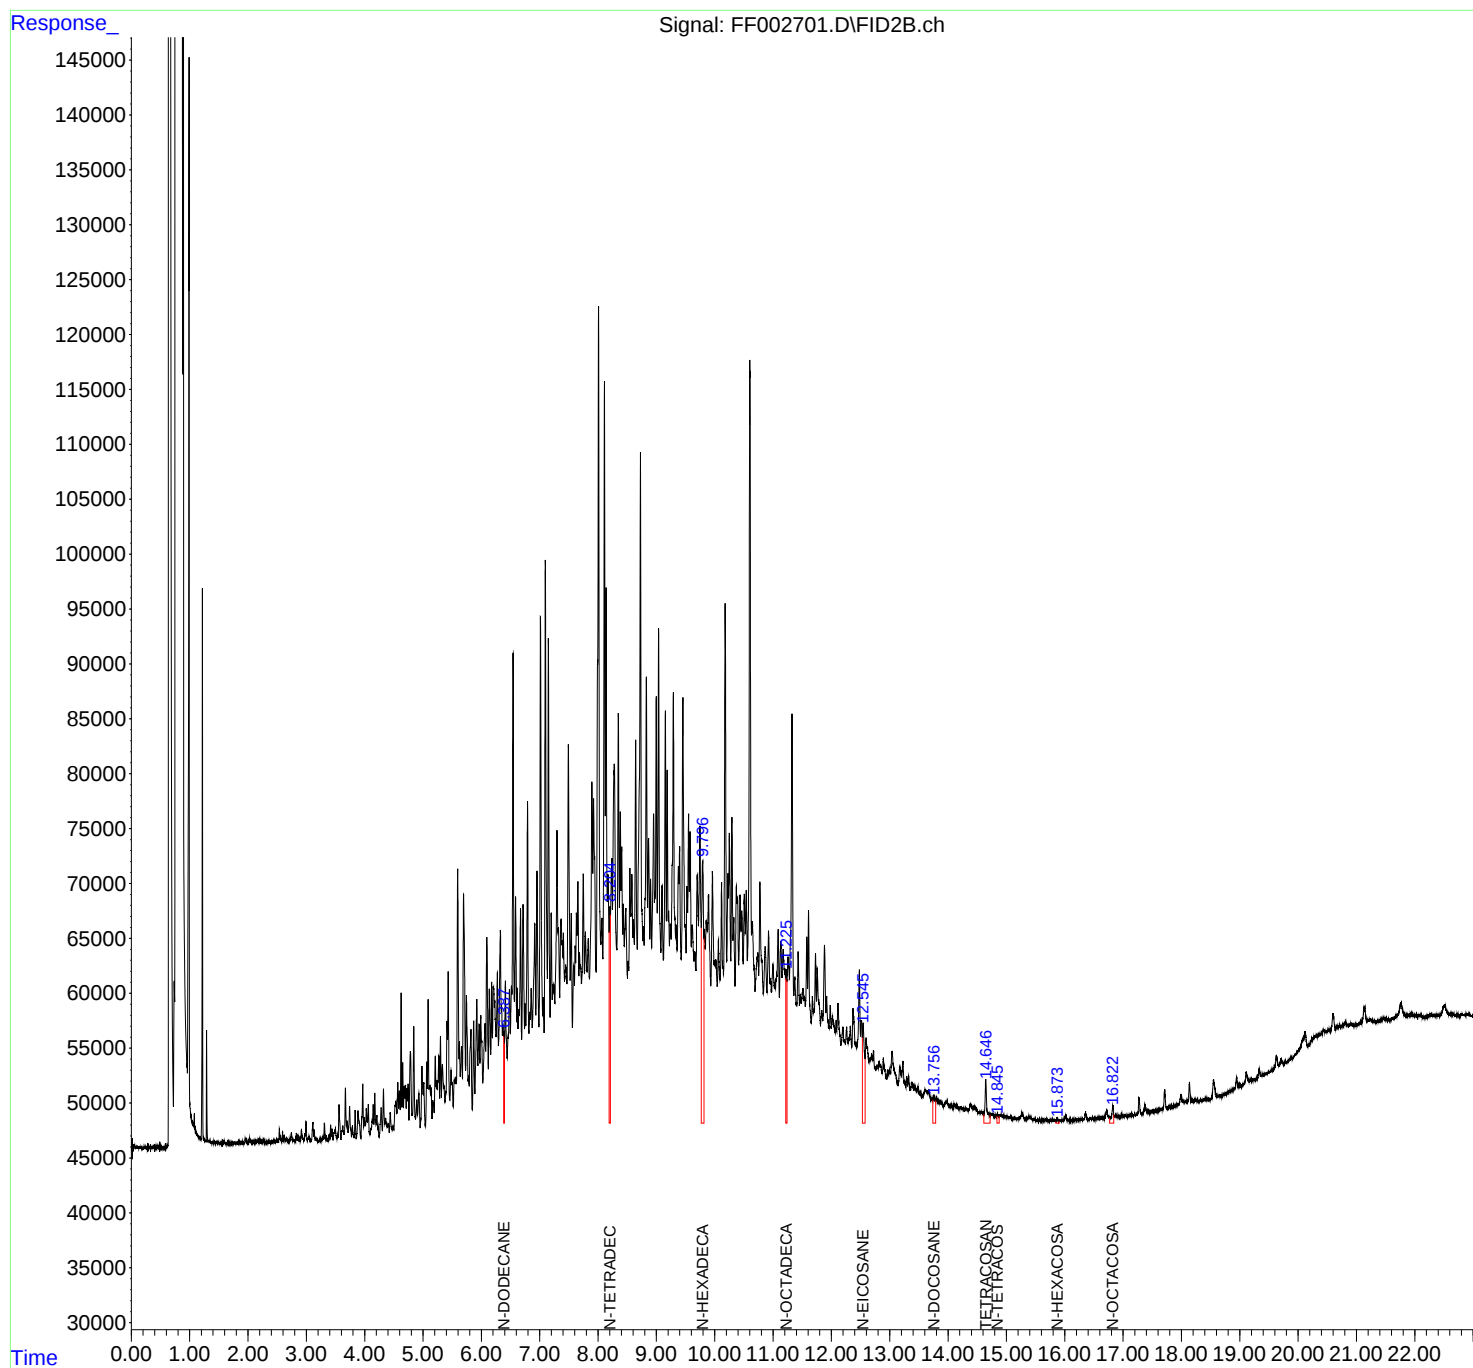

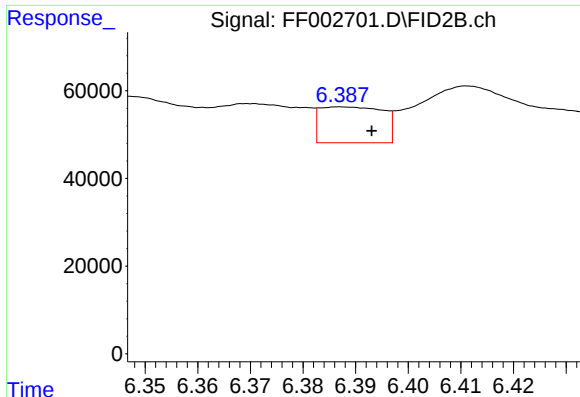


#3 N-DODECANE

R.T.: 6.388 min
Delta R.T.: -0.006 min
Response: 68134
Conc: 0.51 ug/ml

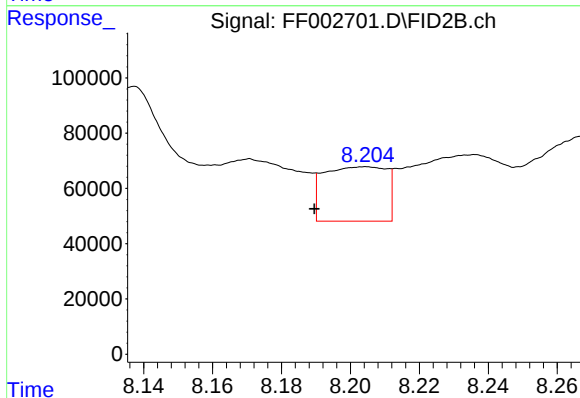


#4 N-TETRADECANE

R.T.: 8.204 min
Delta R.T.: 0.015 min
Response: 247993
Conc: 1.94 ug/ml

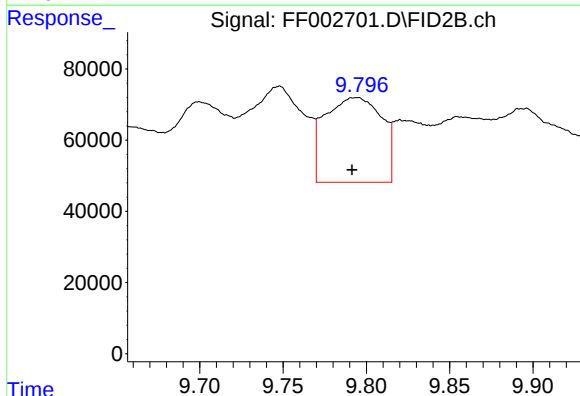


#5 N-HEXADECANE

R.T.: 9.794 min
Delta R.T.: 0.003 min
Response: 564346
Conc: 4.69 ug/ml

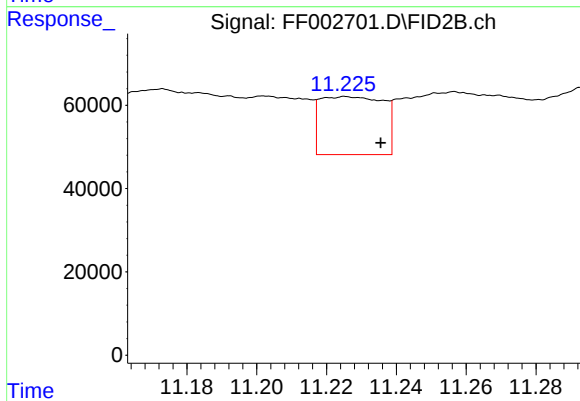


#6 N-OCTADECANE

R.T.: 11.226 min
Delta R.T.: -0.010 min
Response: 175059
Conc: 1.53 ug/ml

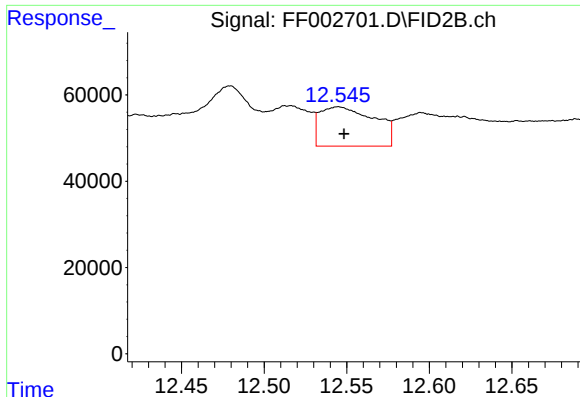


#7 N-EICOSANE

R.T.: 12.545 min
Delta R.T.: -0.003 min
Response: 209149
Conc: 1.98 ug/ml

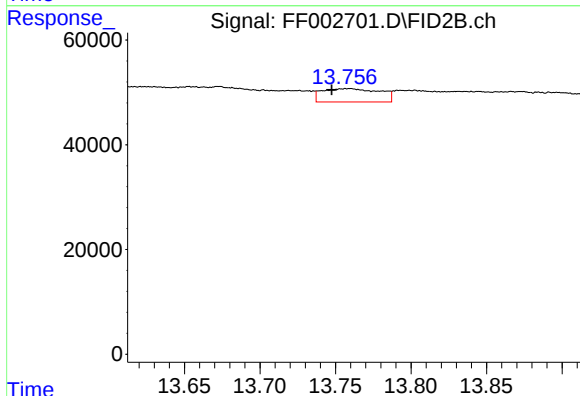


#8 N-DOCOSANE

R.T.: 13.759 min
Delta R.T.: 0.012 min
Response: 67909
Conc: 0.68 ug/ml

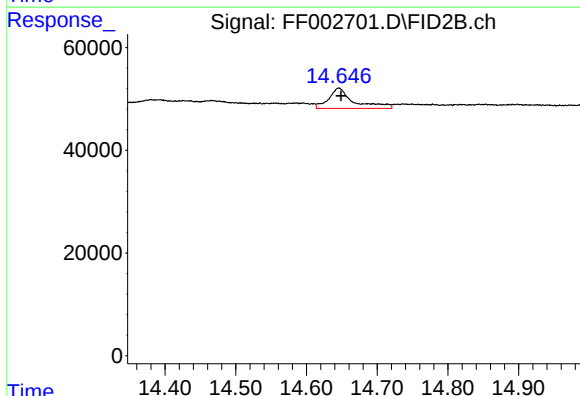


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.646 min
Delta R.T.: -0.003 min
Response: 97366
Conc: 1.15 ug/ml

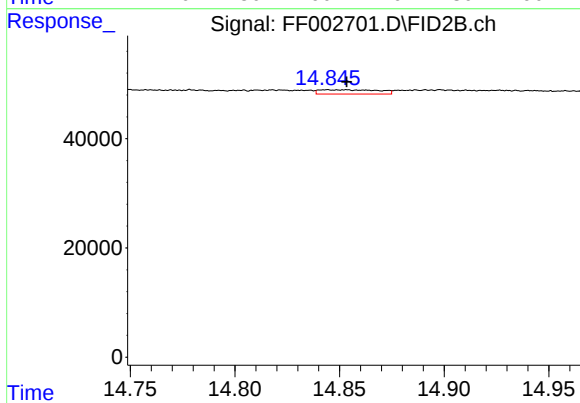


#10 N-TETRACOSANE

R.T.: 14.853 min
Delta R.T.: 0.000 min
Response: 15592
Conc: 0.16 ug/ml

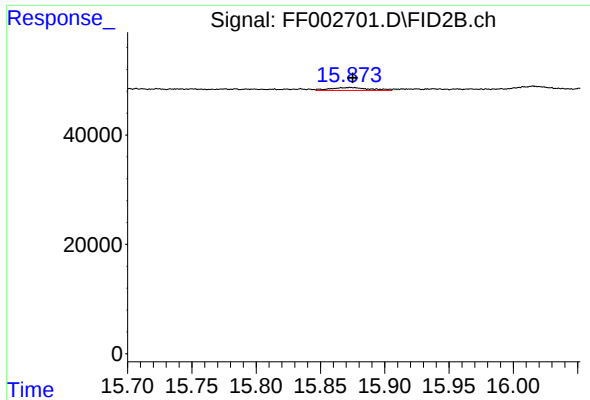

#11 N-HEXACOSANE

R.T.: 15.873 min
Delta R.T.: -0.002 min
Response: 11148
Conc: 0.11 ug/ml

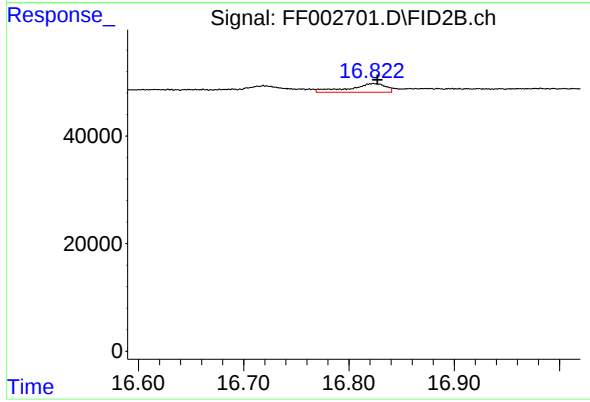

#12 N-OCTACOSANE

R.T.: 16.824 min
Delta R.T.: -0.003 min
Response: 38904
Conc: 0.38 ug/ml