

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111518\
 Data File : FF002704.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2018 15:03
 Operator : AJ\SJ
 Sample : J5950-11
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 16 03:35:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.655	6792094	86.949 ug/ml
Target Compounds				
1)	N-OCTANE	2.262	900622	7.170 ug/ml
2)	N-DECANE	4.364	4248398	34.015 ug/ml
3)	N-DODECANE	6.390	7091985	58.512 ug/ml
4)	N-TETRADECANE	8.194	73613777	637.258 ug/ml
5)	N-HEXADECANE	9.782	50811841	464.719 ug/ml
6)	N-OCTADECANE	11.249	11091700	106.851 ug/ml
7)	N-EICOSANE	12.561	17496228	180.702 ug/ml
8)	N-DOCOSANE	13.744	4610368	50.355 ug/ml
10)	N-TETRACOSANE	14.856	1461839	16.409 ug/ml
12)	N-OCTACOSANE	16.823	159489	1.672 ug/ml
13)	N-TRIACONTANE	17.713	130068	1.312 ug/ml
14)	N-DOTRIACONTANE	18.547	153476	1.550 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111518\
Data File : FF002704.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2018 15:03
Operator : AJ\SJ
Sample : J5950-11
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 16 03:35:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

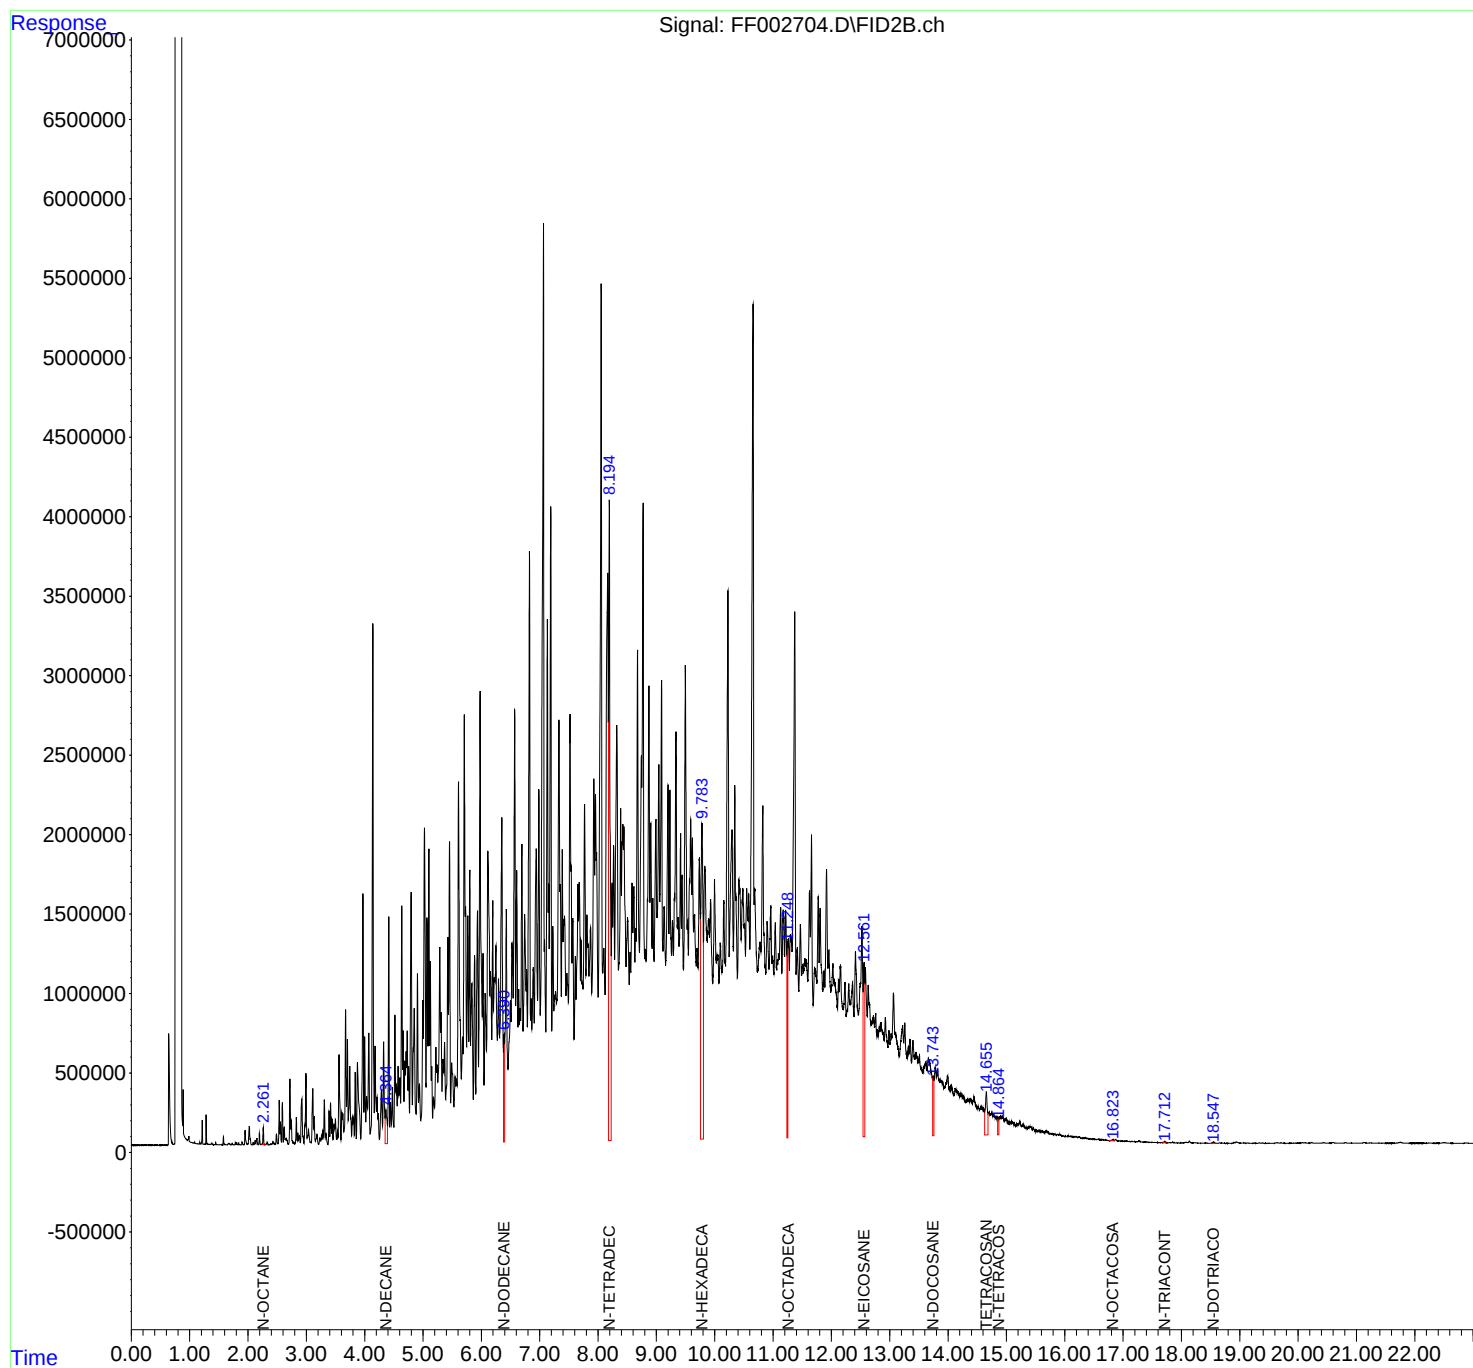

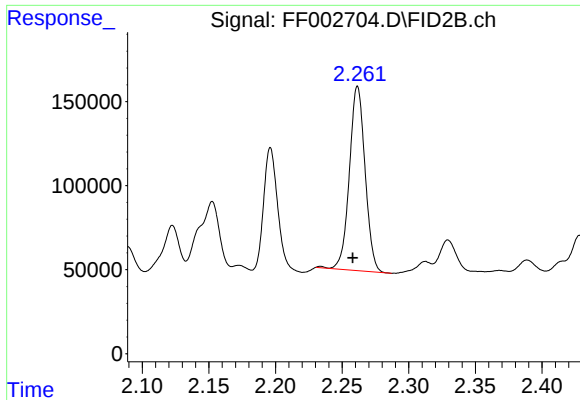


#1 N-OCTANE

R.T.: 2.262 min
Delta R.T.: 0.004 min
Response: 900622
Conc: 7.17 ug/ml

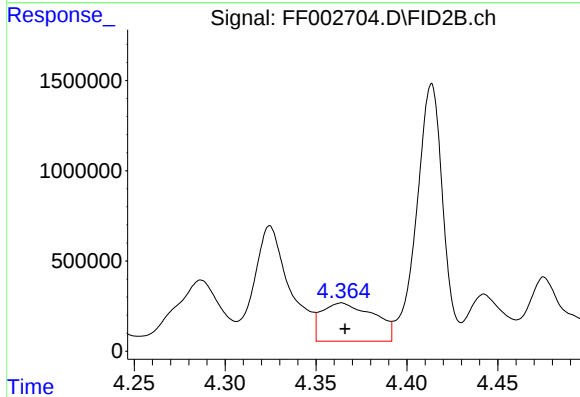


#2 N-DECANE

R.T.: 4.364 min
Delta R.T.: -0.002 min
Response: 4248398
Conc: 34.01 ug/ml

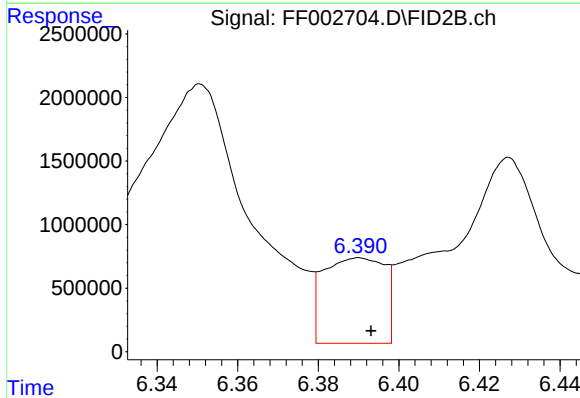


#3 N-DODECANE

R.T.: 6.390 min
Delta R.T.: -0.003 min
Response: 7091985
Conc: 58.51 ug/ml

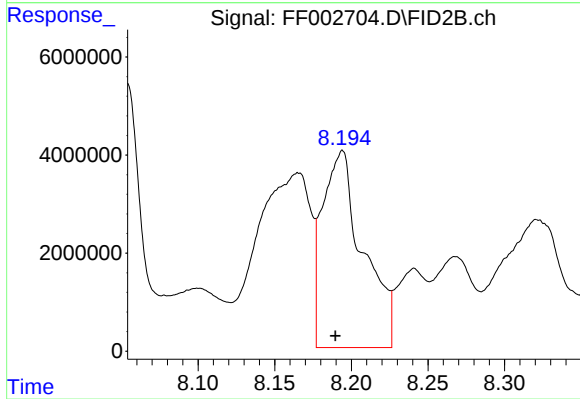


#4 N-TETRADECANE

R.T.: 8.194 min
Delta R.T.: 0.004 min
Response: 73613777
Conc: 637.26 ug/ml

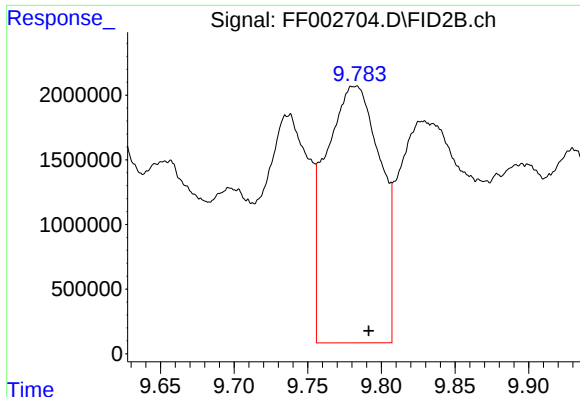


#5 N-HEXADECANE

R.T.: 9.782 min
Delta R.T.: -0.009 min
Response: 50811841
Conc: 464.72 ug/ml

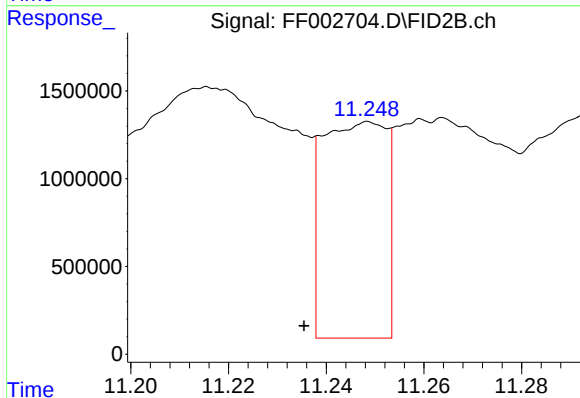


#6 N-OCTADECANE

R.T.: 11.249 min
Delta R.T.: 0.013 min
Response: 11091700
Conc: 106.85 ug/ml

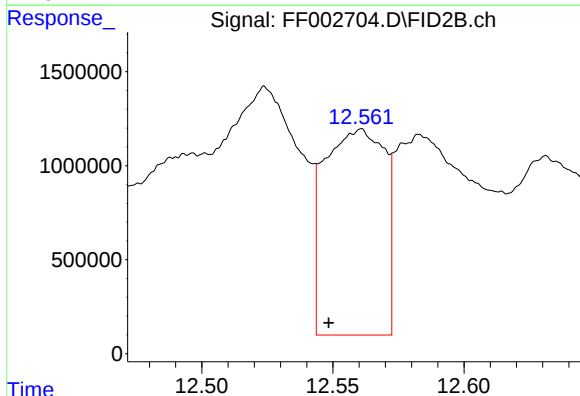


#7 N-EICOSANE

R.T.: 12.561 min
Delta R.T.: 0.012 min
Response: 17496228
Conc: 180.70 ug/ml

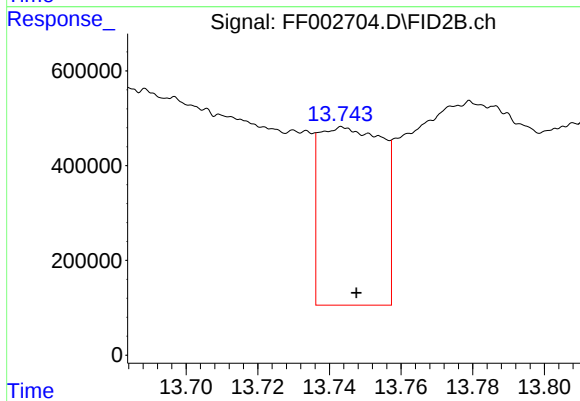


#8 N-DOCOSANE

R.T.: 13.744 min
Delta R.T.: -0.004 min
Response: 4610368
Conc: 50.36 ug/ml

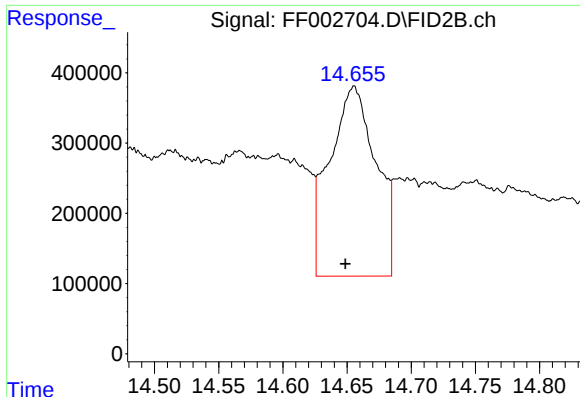


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.655 min
Delta R.T.: 0.007 min
Response: 6792094
Conc: 86.95 ug/ml

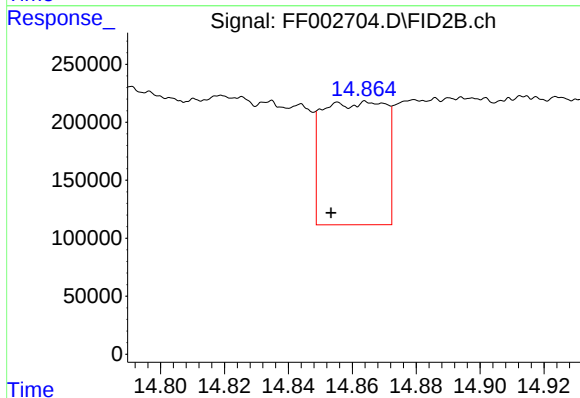


#10 N-TETRACOSANE

R.T.: 14.856 min
Delta R.T.: 0.002 min
Response: 1461839
Conc: 16.41 ug/ml

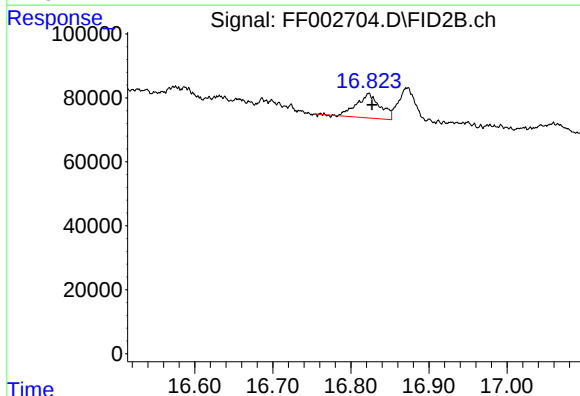


#12 N-OCTACOSANE

R.T.: 16.823 min
Delta R.T.: -0.004 min
Response: 159489
Conc: 1.67 ug/ml

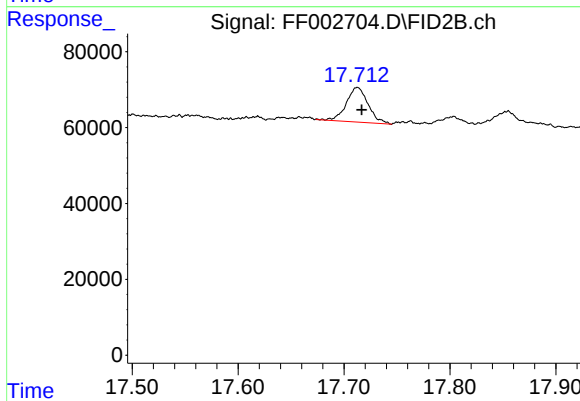

#13 N-TRIACONTANE

R.T.: 17.713 min
Delta R.T.: -0.004 min
Response: 130068
Conc: 1.31 ug/ml

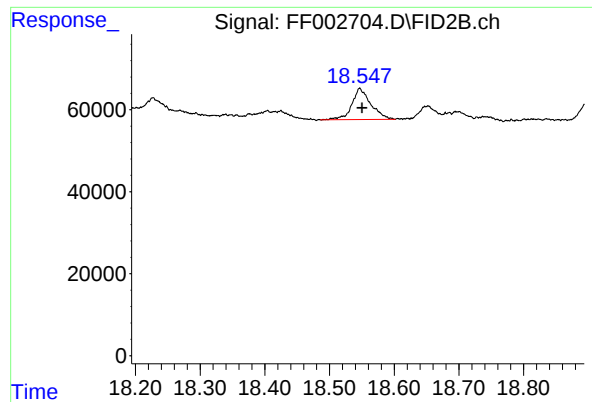

#14 N-DOTRIACONTANE

R.T.: 18.547 min
Delta R.T.: -0.004 min
Response: 153476
Conc: 1.55 ug/ml