

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111518\
 Data File : FG002979.D
 Signal(s) : FID1A.ch
 Acq On : 15 Nov 2018 17:33
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 16 04:00:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.747	6320042	57.507 ug/ml
Target Compounds			
2) N-DECANE	4.459	8067250	63.252 ug/ml
3) N-DODECANE	6.488	8000548	61.382 ug/ml
4) N-TETRADECANE	8.286	7940781	60.055 ug/ml
5) N-HEXADECANE	9.891	7853639	58.978 ug/ml
6) N-OCTADECANE	11.334	7743504	58.535 ug/ml
7) N-EICOSANE	12.647	7554427	58.275 ug/ml
8) N-DOCOSANE	13.847	7335173	57.621 ug/ml
10) N-TETRACOSANE	14.952	7281453	58.286 ug/ml
11) N-HEXACOSANE	15.975	7331975	59.491 ug/ml
12) N-OCTACOSANE	16.925	7400544	60.846 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111518\
Data File : FG002979.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2018 17:33
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 16 04:00:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

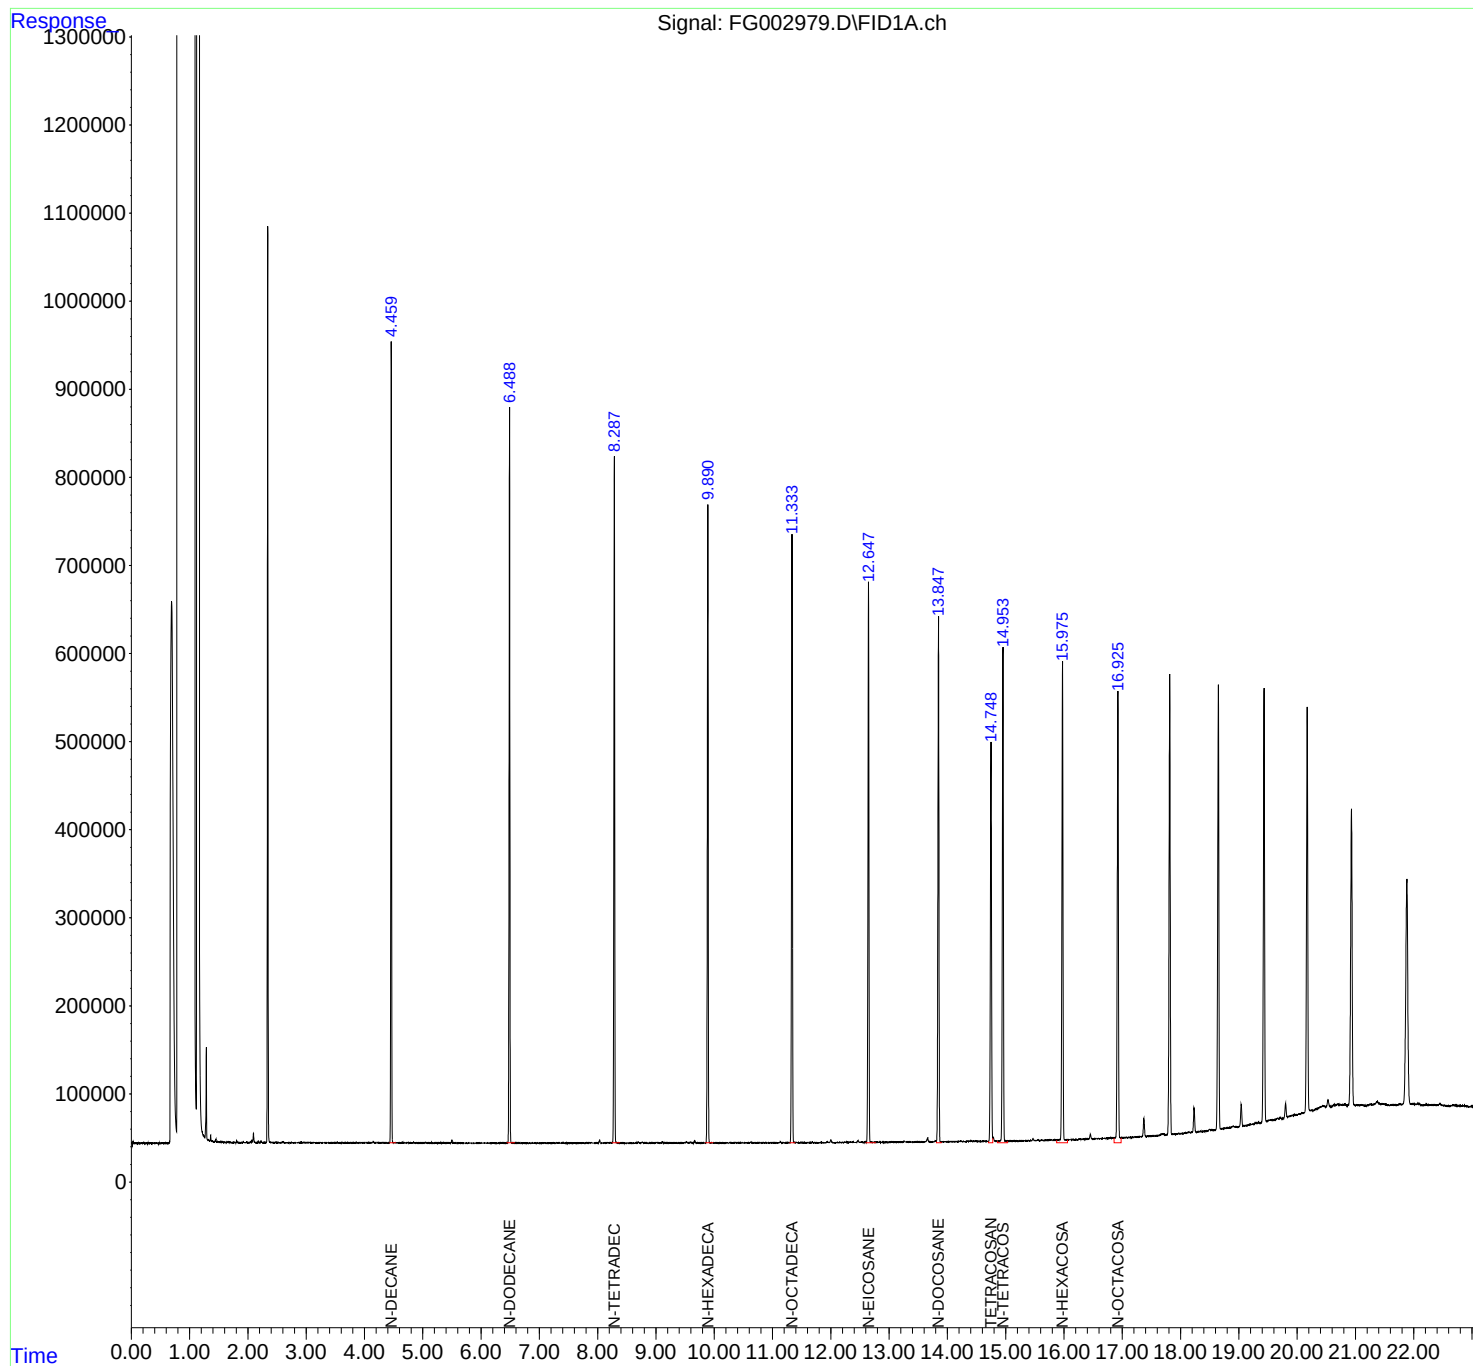

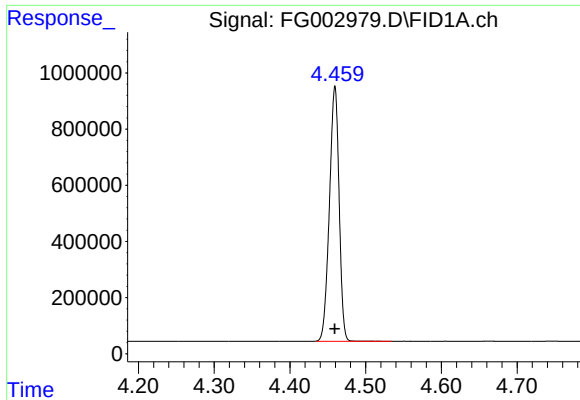


#2 N-DECANE

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 8067250
Conc: 63.25 ug/ml

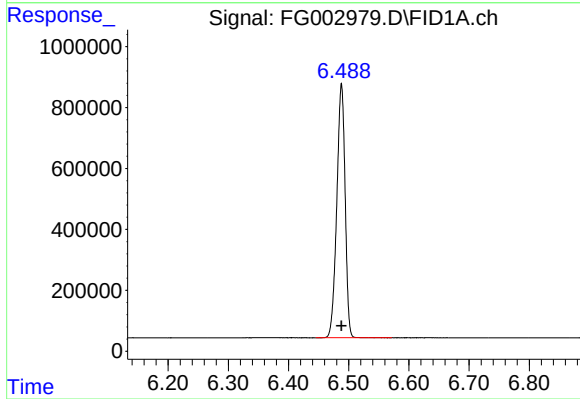


#3 N-DODECANE

R.T.: 6.488 min
Delta R.T.: 0.000 min
Response: 8000548
Conc: 61.38 ug/ml

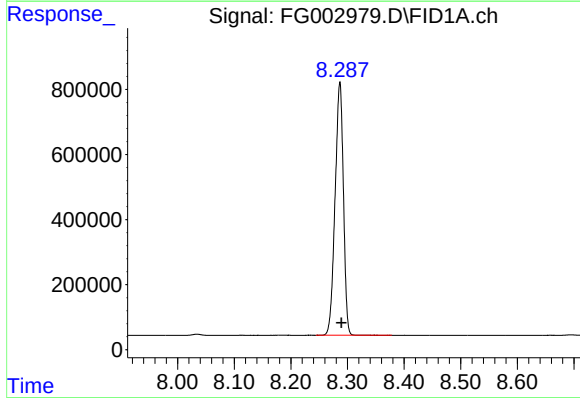


#4 N-TETRADECANE

R.T.: 8.286 min
Delta R.T.: -0.003 min
Response: 7940781
Conc: 60.06 ug/ml

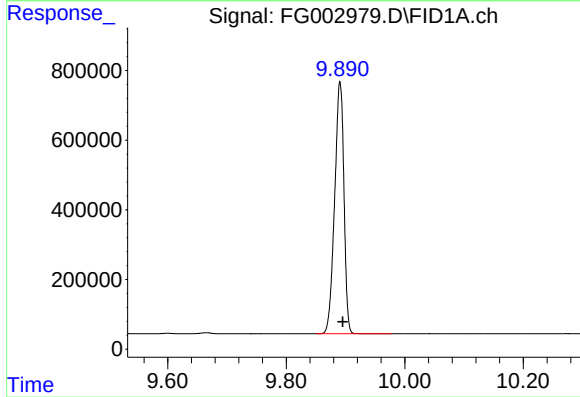


#5 N-HEXADECANE

R.T.: 9.891 min
Delta R.T.: -0.005 min
Response: 7853639
Conc: 58.98 ug/ml

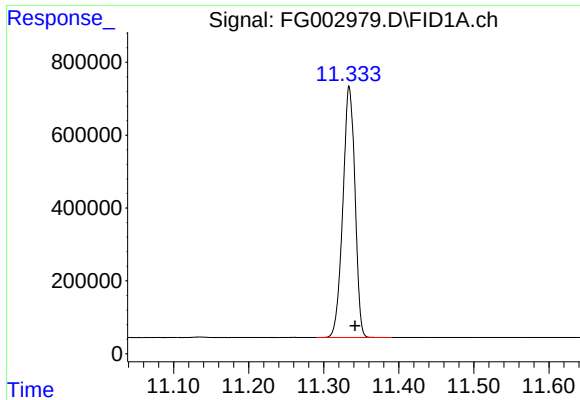


#6 N-OCTADECANE

R.T.: 11.334 min
Delta R.T.: -0.008 min
Response: 7743504
Conc: 58.54 ug/ml

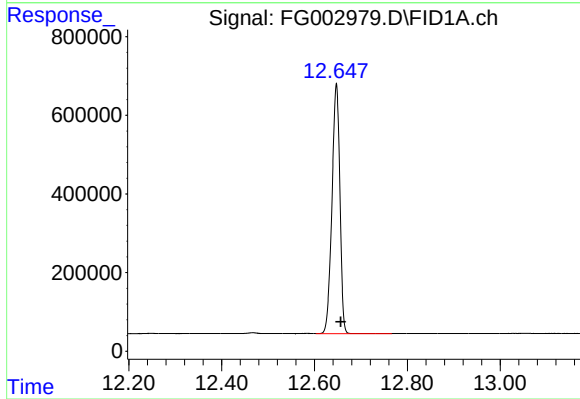


#7 N-EICOSANE

R.T.: 12.647 min
Delta R.T.: -0.009 min
Response: 7554427
Conc: 58.28 ug/ml

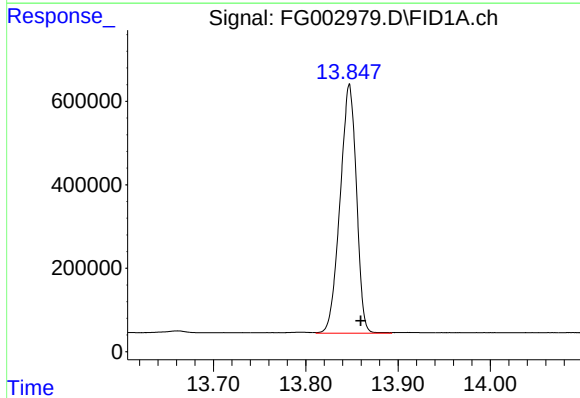


#8 N-DOCOSANE

R.T.: 13.847 min
Delta R.T.: -0.012 min
Response: 7335173
Conc: 57.62 ug/ml

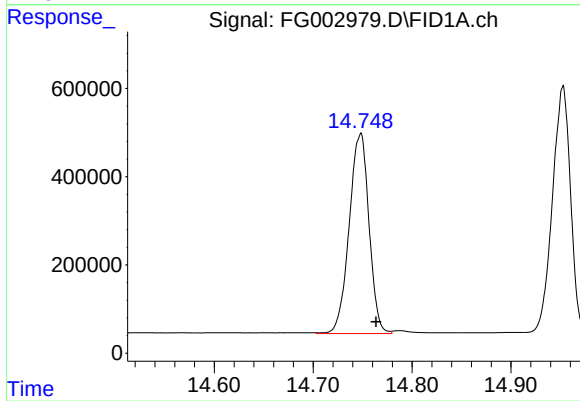


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.747 min
Delta R.T.: -0.016 min
Response: 6320042
Conc: 57.51 ug/ml

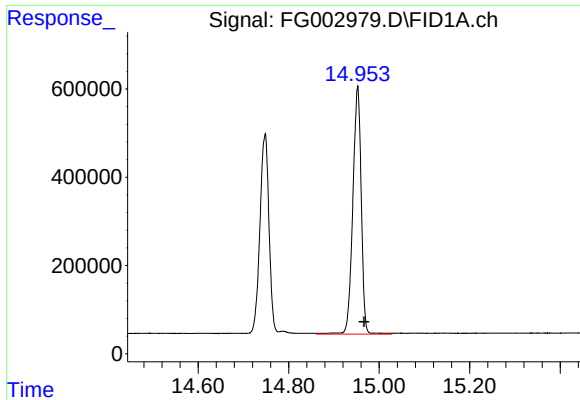


#10 N-TETRACOSANE

R.T.: 14.952 min
Delta R.T.: -0.014 min
Response: 7281453
Conc: 58.29 ug/ml

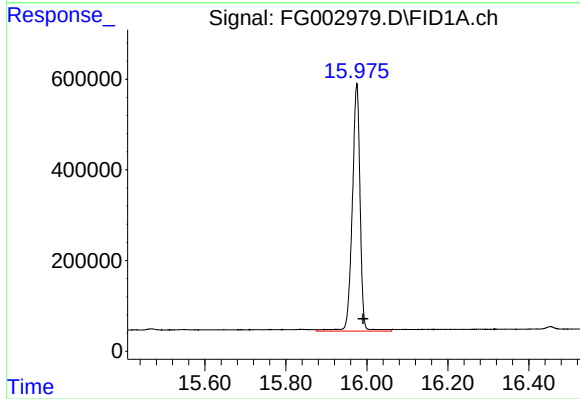

#11 N-HEXACOSANE

R.T.: 15.975 min
Delta R.T.: -0.016 min
Response: 7331975
Conc: 59.49 ug/ml

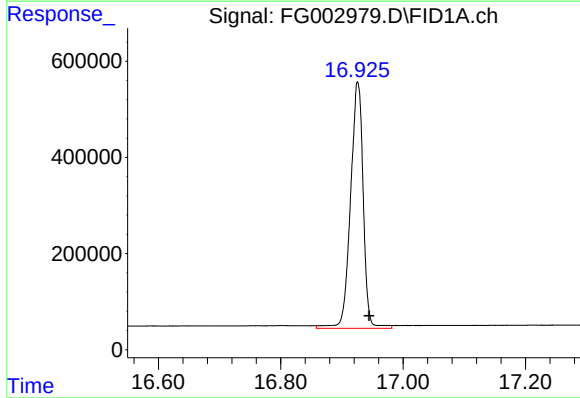

#12 N-OCTACOSANE

R.T.: 16.925 min
Delta R.T.: -0.019 min
Response: 7400544
Conc: 60.85 ug/ml