

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111518\
 Data File : FF002699.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2018 10:18
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 15 12:35:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.648	4139156	48.688 ug/ml
Target Compounds			
2) N-DECANE	4.370	5791533	42.118 ug/ml
3) N-DODECANE	6.396	5648959	42.061 ug/ml
4) N-TETRADECANE	8.190	5552405	43.367 ug/ml
5) N-HEXADECANE	9.792	5354863	44.487 ug/ml
6) N-OCTADECANE	11.235	5167762	45.246 ug/ml
7) N-EICOSANE	12.547	4892279	46.230 ug/ml
8) N-DOCOSANE	13.747	4753829	47.559 ug/ml
10) N-TETRACOSANE	14.852	4717723	48.804 ug/ml
11) N-HEXACOSANE	15.874	4639034	47.343 ug/mlm
12) N-OCTACOSANE	16.826	4789133	46.340 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111518\
Data File : FF002699.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2018 10:18
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 15 12:35:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

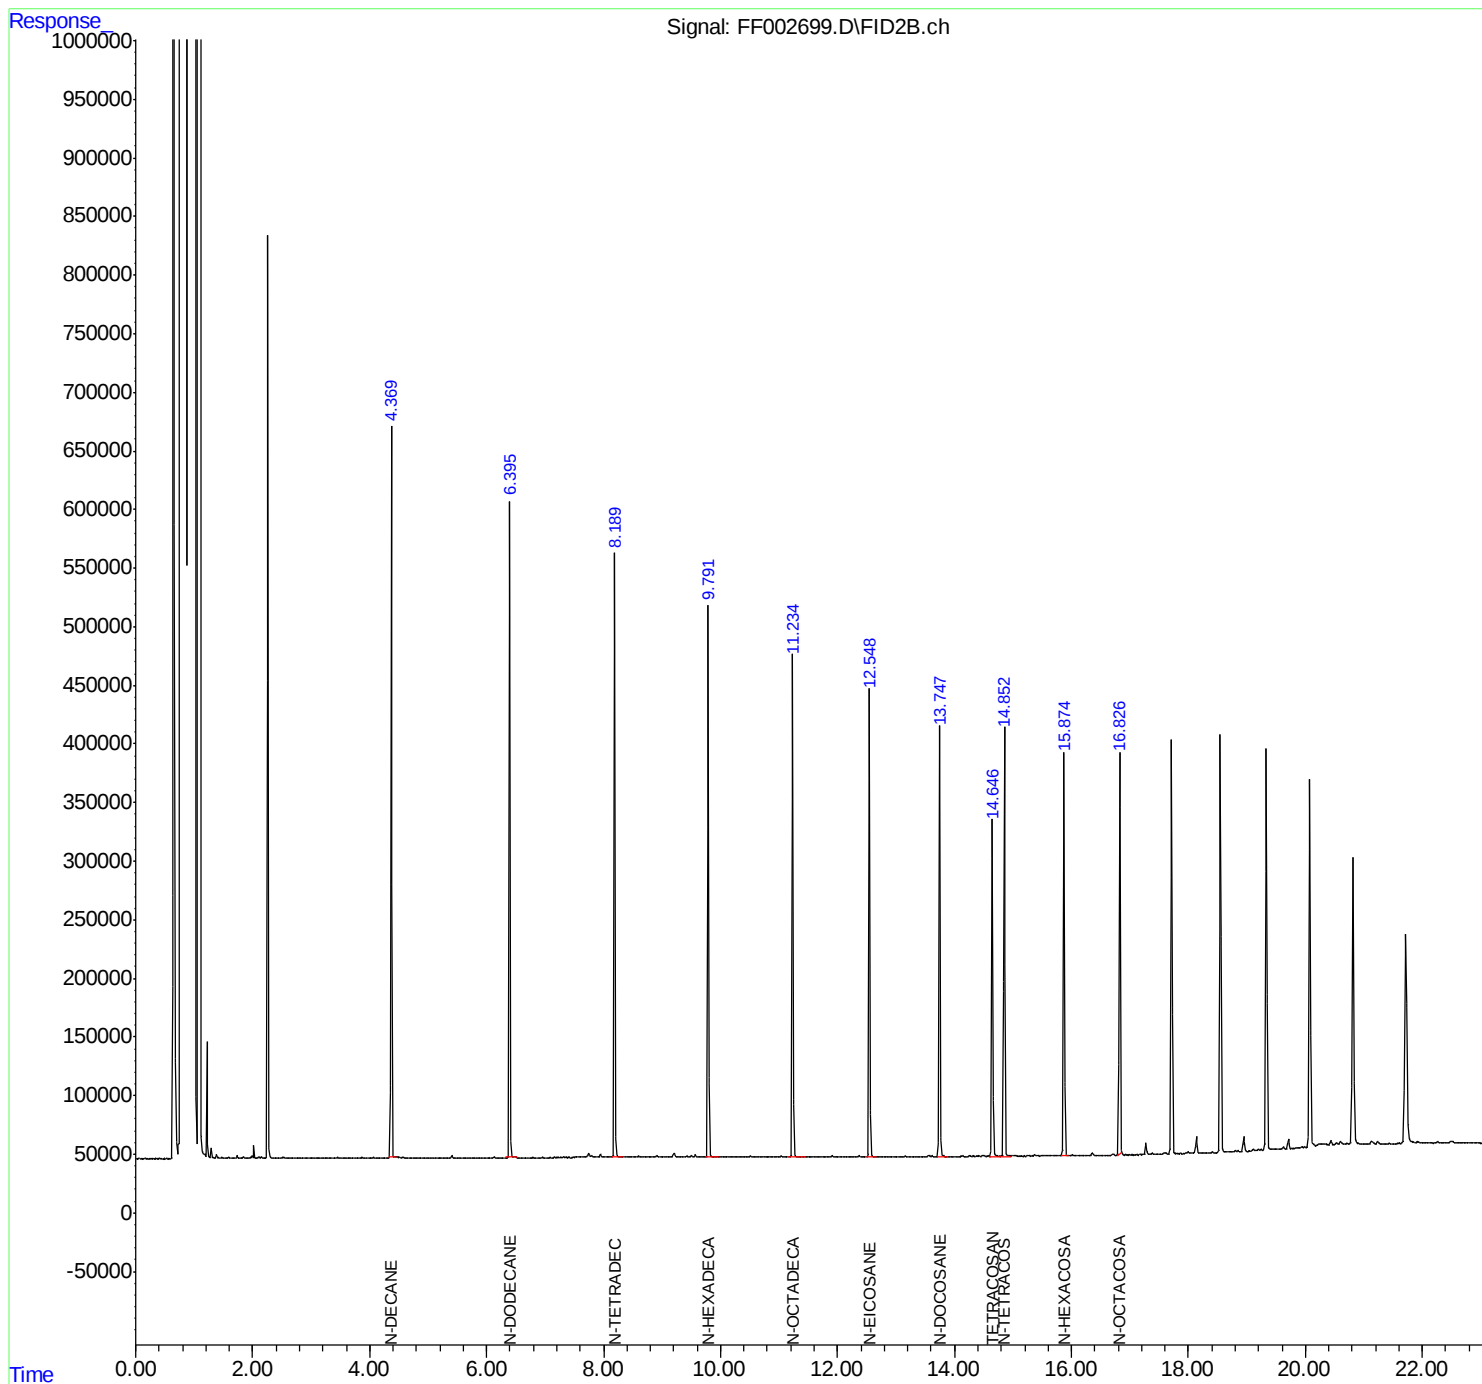

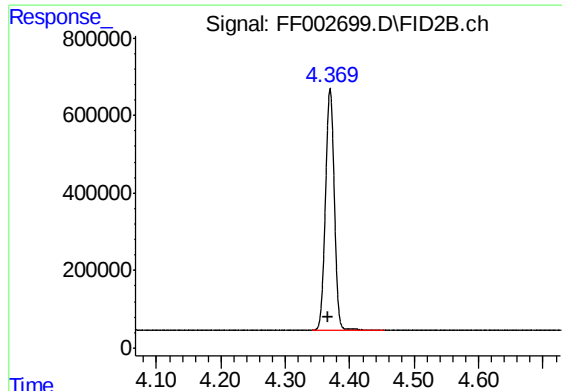


#2 N-DECANE

R.T.: 4.370 min
Delta R.T.: 0.004 min
Response: 5791533
Conc: 42.12 ug/ml

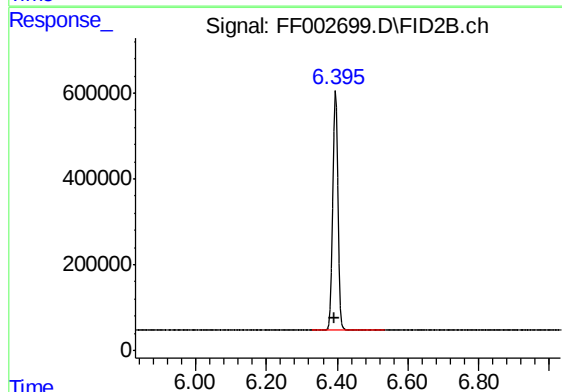


#3 N-DODECANE

R.T.: 6.396 min
Delta R.T.: 0.002 min
Response: 5648959
Conc: 42.06 ug/ml

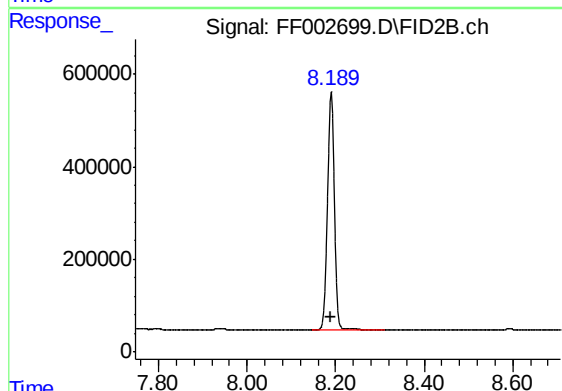


#4 N-TETRADECANE

R.T.: 8.190 min
Delta R.T.: 0.000 min
Response: 5552405
Conc: 43.37 ug/ml

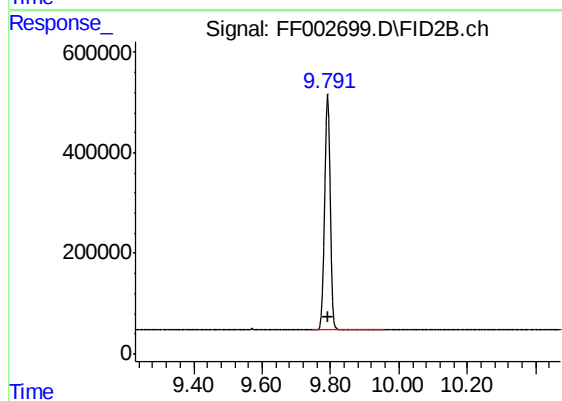


#5 N-HEXADECANE

R.T.: 9.792 min
Delta R.T.: 0.000 min
Response: 5354863
Conc: 44.49 ug/ml

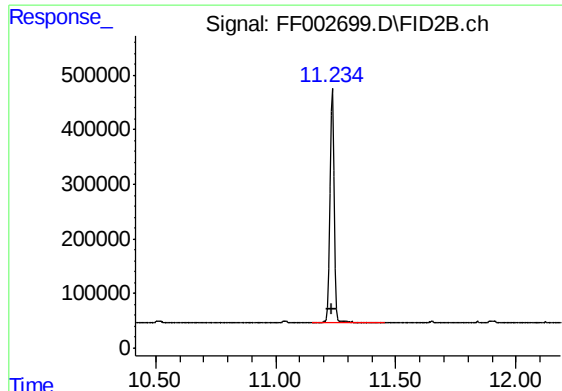


#6 N-OCTADECANE

R.T.: 11.235 min
Delta R.T.: 0.000 min
Response: 5167762
Conc: 45.25 ug/ml

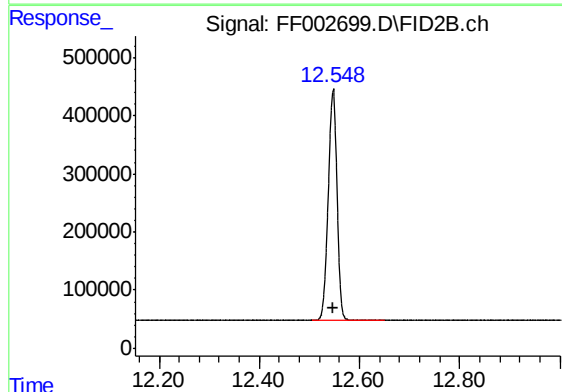


#7 N-EICOSANE

R.T.: 12.547 min
Delta R.T.: -0.001 min
Response: 4892279
Conc: 46.23 ug/ml

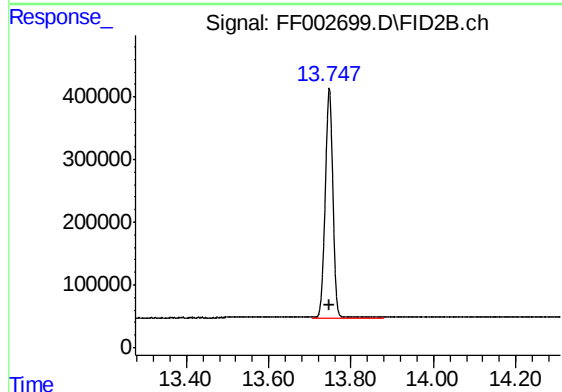


#8 N-DOCOSANE

R.T.: 13.747 min
Delta R.T.: 0.000 min
Response: 4753829
Conc: 47.56 ug/ml

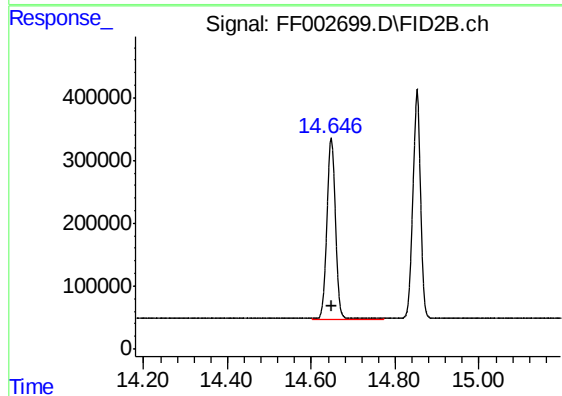


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.648 min
Delta R.T.: -0.001 min
Response: 4139156
Conc: 48.69 ug/ml

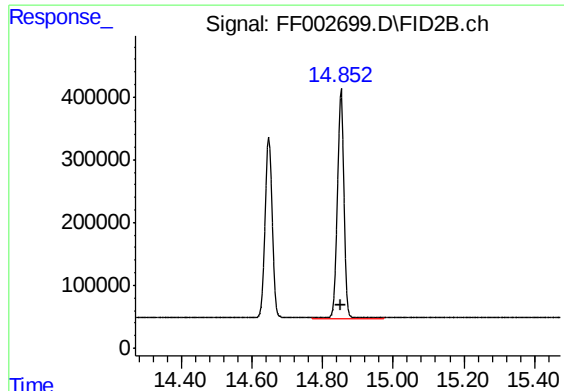


#10 N-TETRACOSANE

R.T.: 14.852 min
Delta R.T.: -0.001 min
Response: 4717723
Conc: 48.80 ug/ml

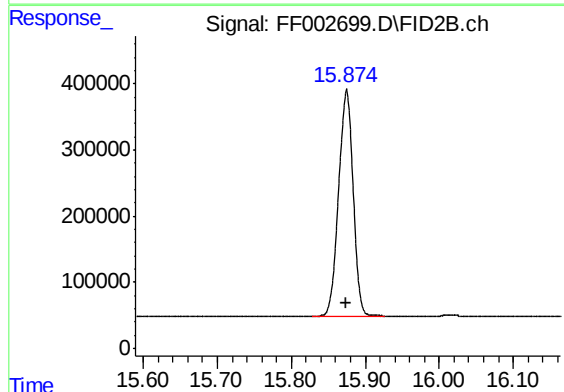

#11 N-HEXACOSANE

R.T.: 15.874 min
Delta R.T.: 0.000 min
Response: 4639034
Conc: 47.34 ug/ml m

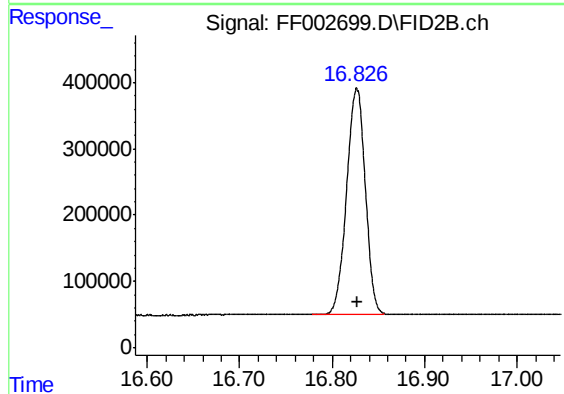

#12 N-OCTACOSANE

R.T.: 16.826 min
Delta R.T.: 0.000 min
Response: 4789133
Conc: 46.34 ug/ml m