

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
 Data File : FF011731.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2022 11:08
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 16 04:33:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.775	3630647	27.013 ug/ml
12) N-OCTACOSANE	17.231	3192357	24.097 ug/ml
13) N-TRIACONTANE	18.116	113107	0.858 ug/ml
14) N-DOTRIACONTANE	18.948	160675	1.194 ug/ml
15) N-TETRATRIACONTANE	19.732	160106	1.216 ug/ml
16) N-HEXATRIACONTANE	20.473	65172	0.529 ug/ml
17) N-OCTATRIACONTANE	21.215	99190	0.852 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
Data File : FF011731.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2022 11:08
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 04:33:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

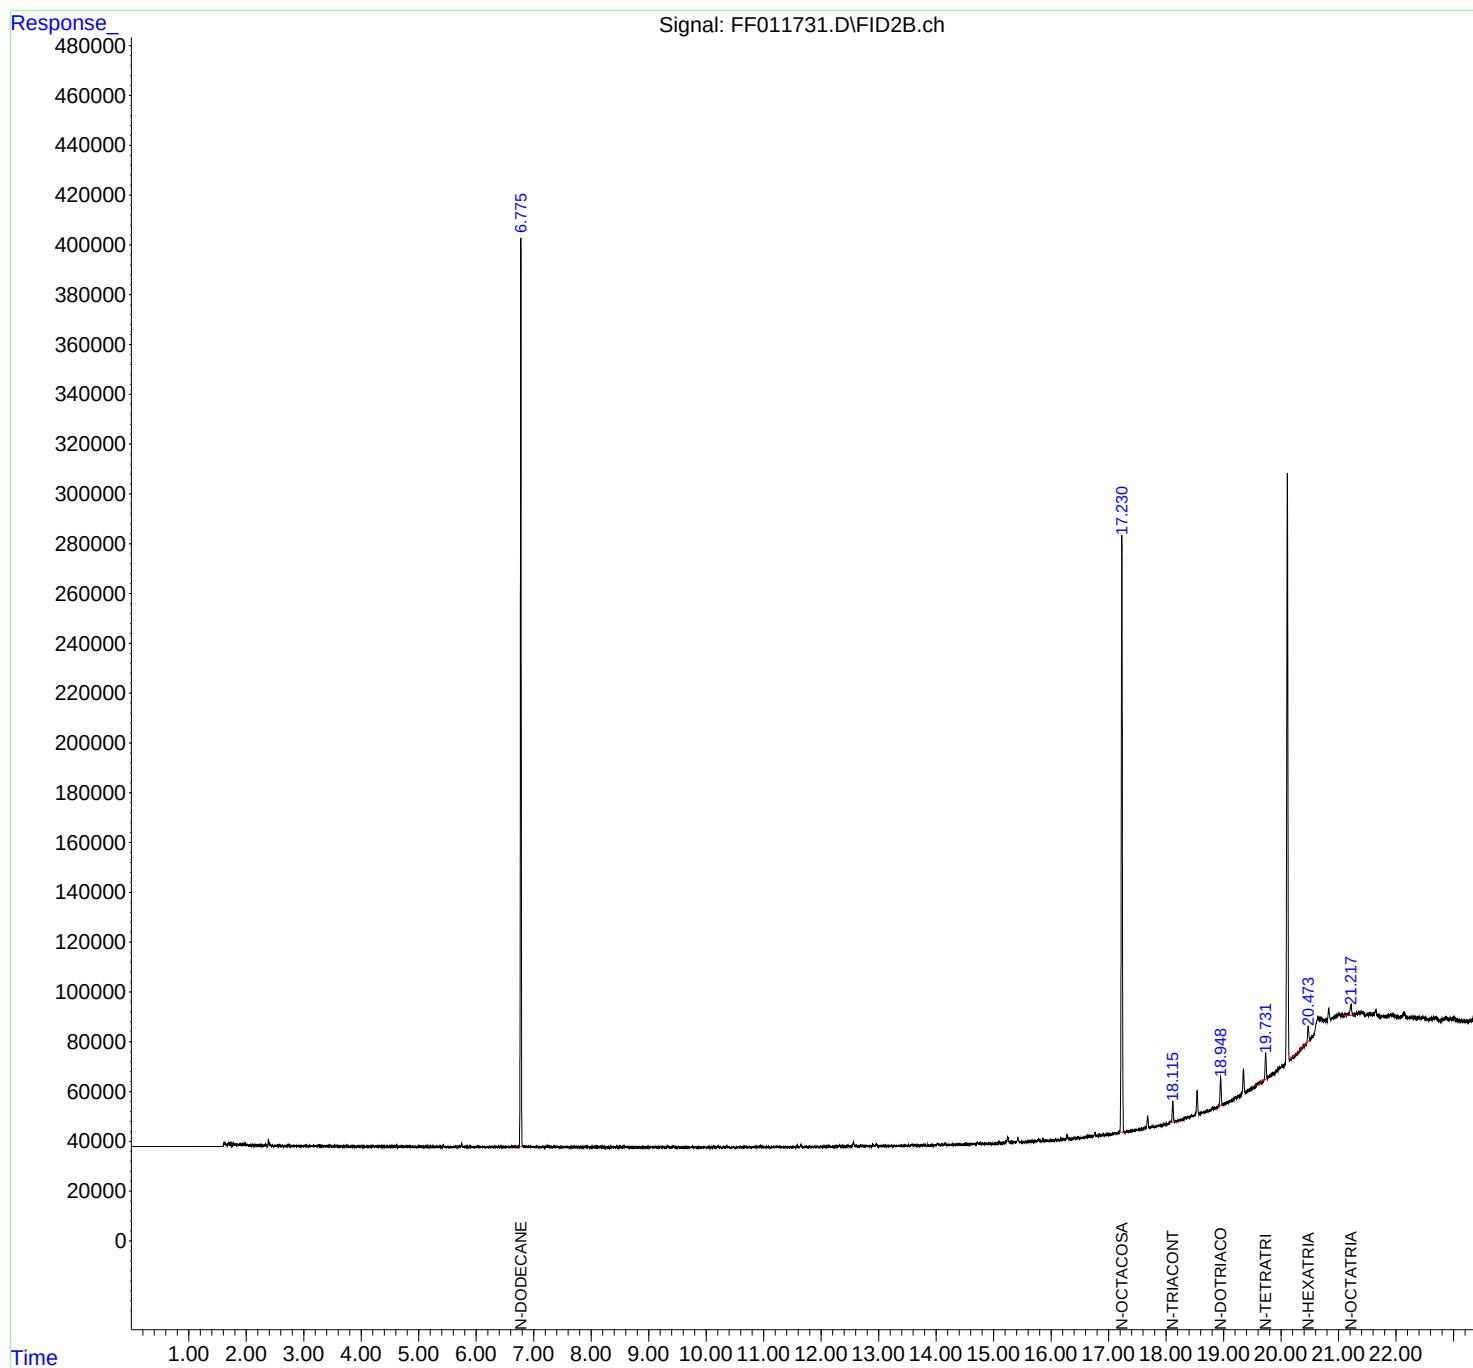


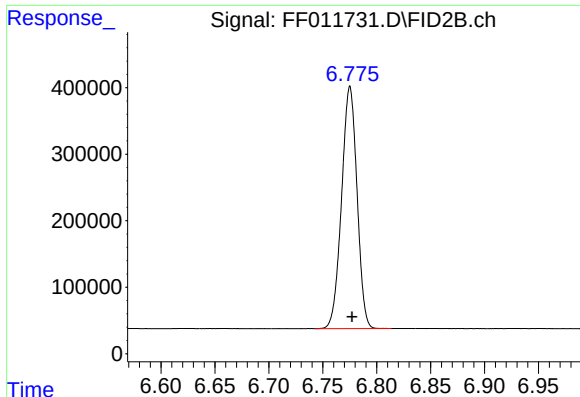

#3 N-DODECANE


R.T.: 6.775 min
Delta R.T.: -0.002 min
Response: 3630647
Conc: 27.01 ug/ml

Instrument :
FID_F
ClientSampleId :

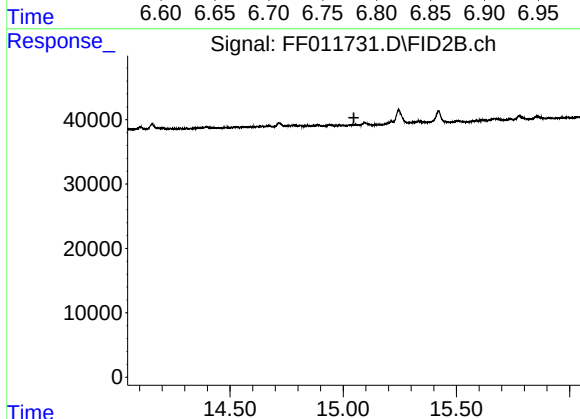


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.047 min
Response: 0
Conc: N.D.

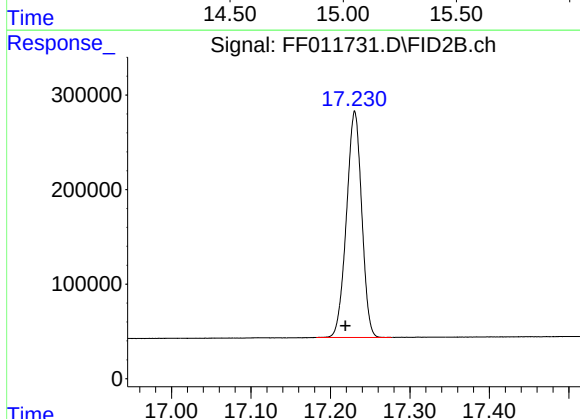


#12 N-OCTACOSANE

R.T.: 17.231 min
Delta R.T.: 0.012 min
Response: 3192357
Conc: 24.10 ug/ml

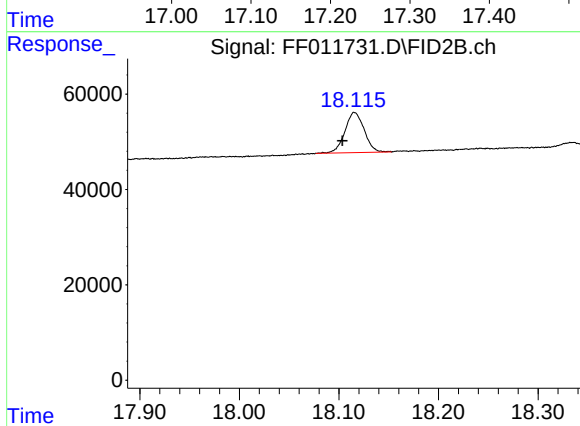

#13 N-TRIACONTANE


R.T.: 18.116 min
Delta R.T.: 0.012 min
Response: 113107
Conc: 0.86 ug/ml

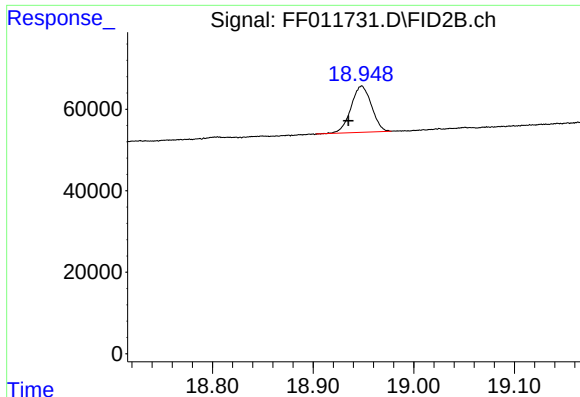

#14 N-DOTRIACONTANE


R.T.: 18.948 min
Delta R.T.: 0.013 min
Response: 160675
Conc: 1.19 ug/ml

Instrument :
FID_F
ClientSampleId :

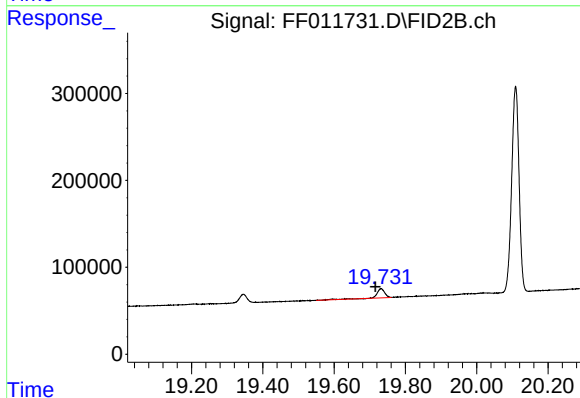


#15 N-TETRATRIACONTANE

R.T.: 19.732 min
Delta R.T.: 0.016 min
Response: 160106
Conc: 1.22 ug/ml

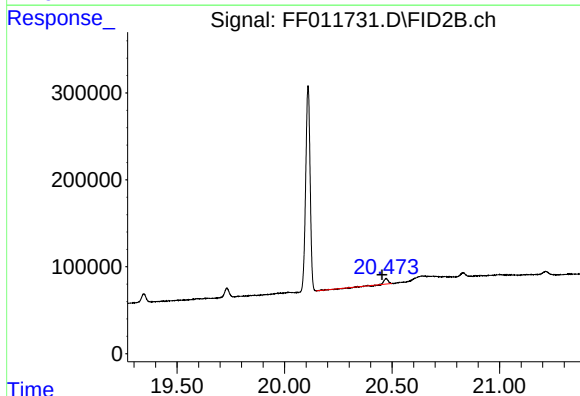

#16 N-HEXATRIACONTANE

R.T.: 20.473 min
Delta R.T.: 0.019 min
Response: 65172
Conc: 0.53 ug/ml

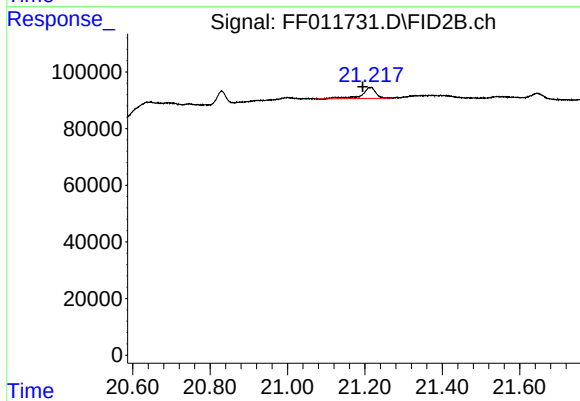

#17 N-OCTATRIACONTANE

R.T.: 21.215 min
Delta R.T.: 0.021 min
Response: 99190
Conc: 0.85 ug/ml