

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
 Data File : FF011733.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2022 12:13
 Operator : YP\AJ
 Sample : PB148156BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 16 04:34:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.055	2211544	18.640 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.228	50854	0.384 ug/ml
13) N-TRIACONTANE	18.116	64735	0.491 ug/ml
14) N-DOTRIACONTANE	18.950	71175	0.529 ug/ml
15) N-TETRATRIACONTANE	19.733	50779	0.386 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
Data File : FF011733.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2022 12:13
Operator : YP\AJ
Sample : PB148156BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 04:34:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

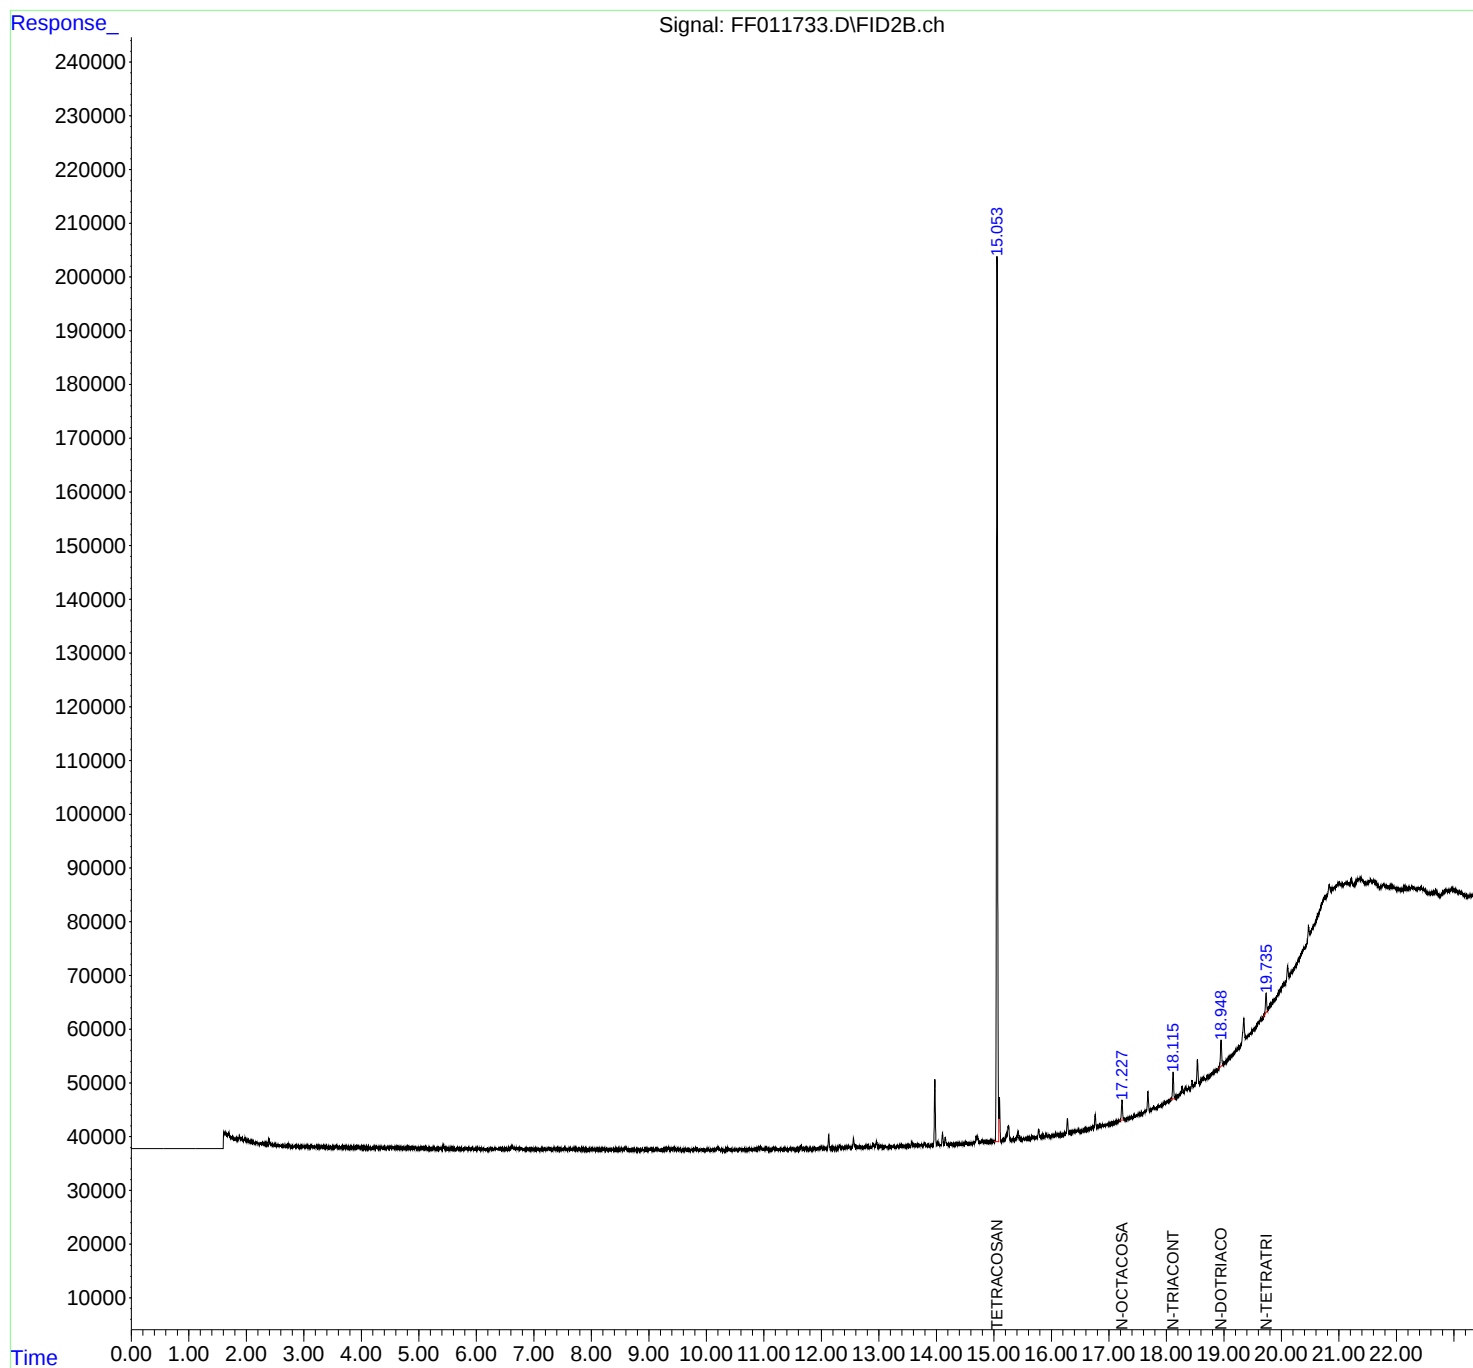


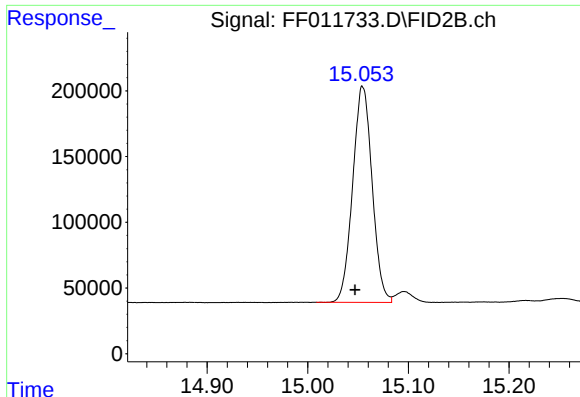

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.055 min
Delta R.T.: 0.008 min
Response: 2211544
Conc: 18.64 ug/ml

Instrument :
FID_F
ClientSampleId :

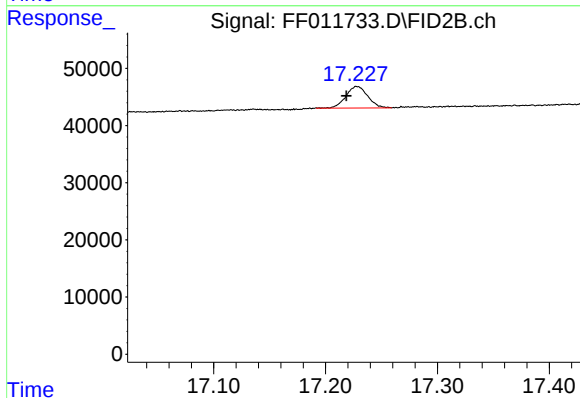


#12 N-OCTACOSANE

R.T.: 17.228 min
Delta R.T.: 0.009 min
Response: 50854
Conc: 0.38 ug/ml

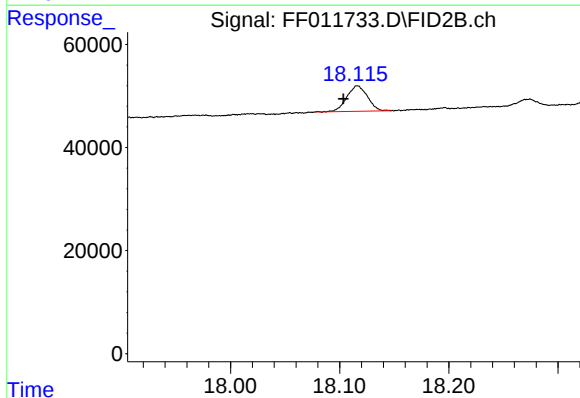


#13 N-TRIACONTANE

R.T.: 18.116 min
Delta R.T.: 0.013 min
Response: 64735
Conc: 0.49 ug/ml

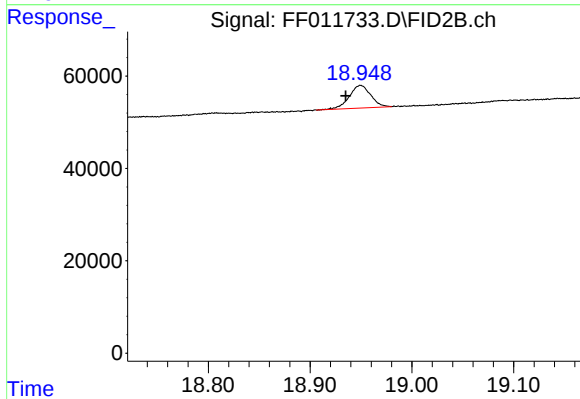

#14 N-DOTRIACONTANE

R.T.: 18.950 min
Delta R.T.: 0.015 min
Response: 71175
Conc: 0.53 ug/ml

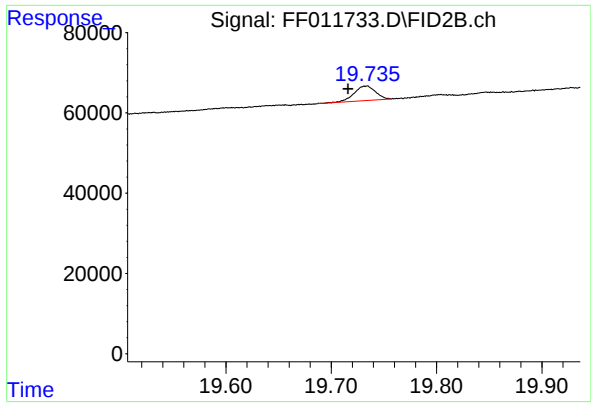

#15 N-TETRATRIACONTANE

R.T.: 19.733 min
Delta R.T.: 0.017 min
Response: 50779
Conc: 0.39 ug/ml

Instrument :
FID_F
ClientSampleId :