

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
 Data File : FF011740.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2022 16:08
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 16 04:35:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.774	2907408	21.632 ug/ml
12)	N-OCTACOSANE	17.228	2589906	19.549 ug/ml
13)	N-TRIACONTANE	18.115	125076	0.948 ug/ml
14)	N-DOTRIACONTANE	18.947	185497	1.378 ug/ml
15)	N-TETRATRIACONTANE	19.731	181964	1.382 ug/ml
16)	N-HEXATRIACONTANE	20.470	115255	0.936 ug/ml
17)	N-OCTATRIACONTANE	21.213	76995	0.661 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
Data File : FF011740.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2022 16:08
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 04:35:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

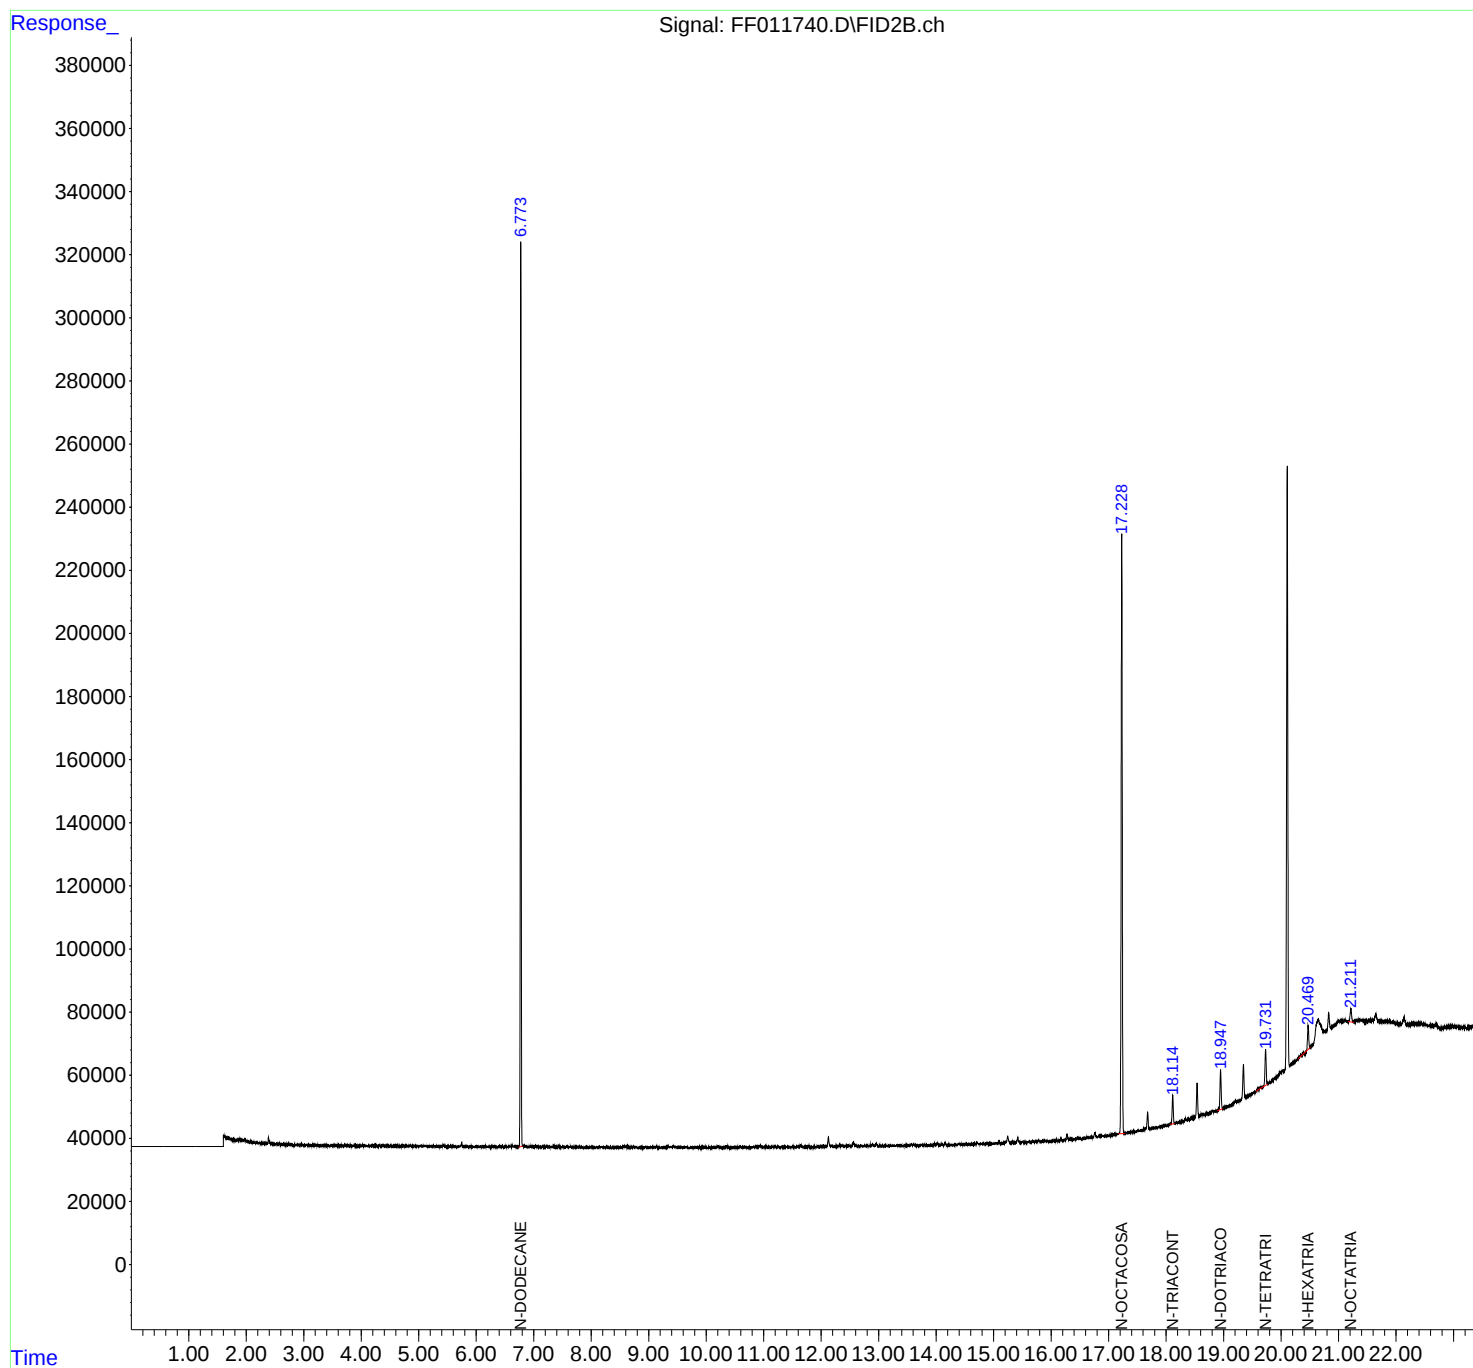


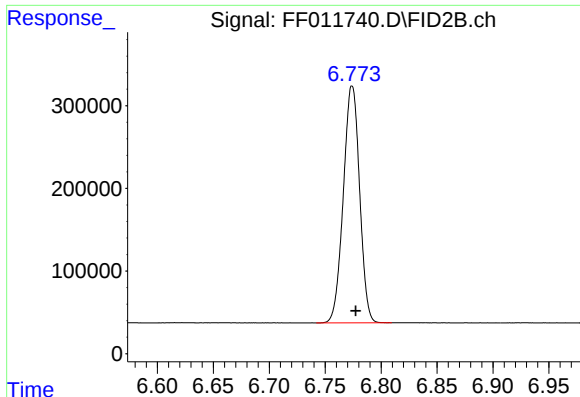

#3 N-DODECANE


R.T.: 6.774 min
Delta R.T.: -0.003 min
Response: 2907408
Conc: 21.63 ug/ml

Instrument :
FID_F
ClientSampleId :

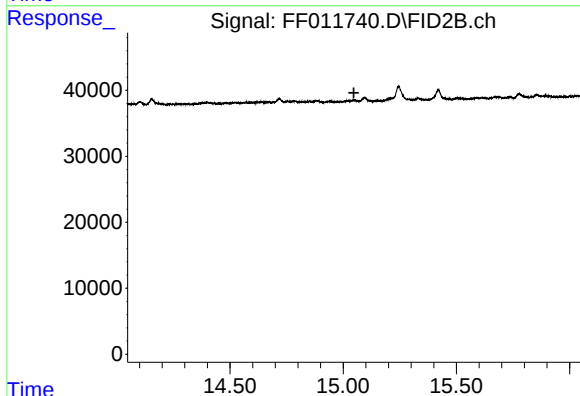


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.047 min
Response: 0
Conc: N.D.

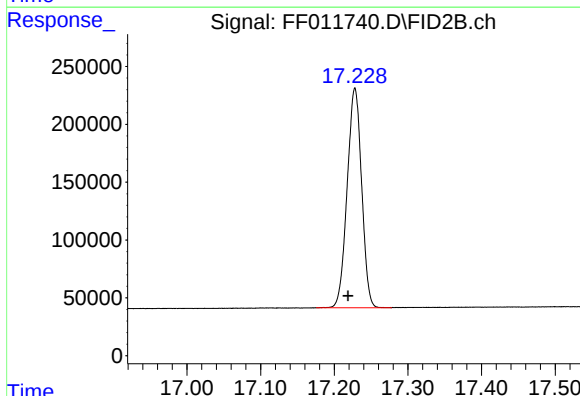


#12 N-OCTACOSANE

R.T.: 17.228 min
Delta R.T.: 0.009 min
Response: 2589906
Conc: 19.55 ug/ml

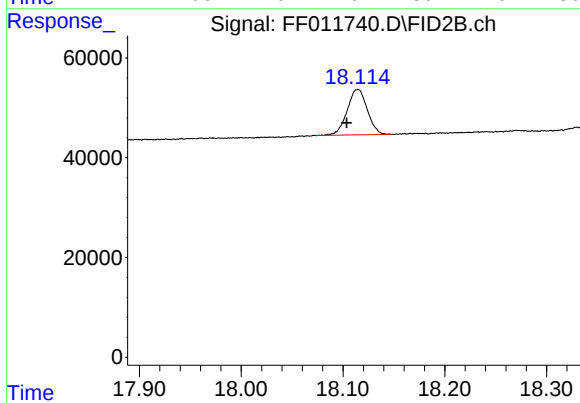

#13 N-TRIACONTANE


R.T.: 18.115 min
Delta R.T.: 0.011 min
Response: 125076
Conc: 0.95 ug/ml

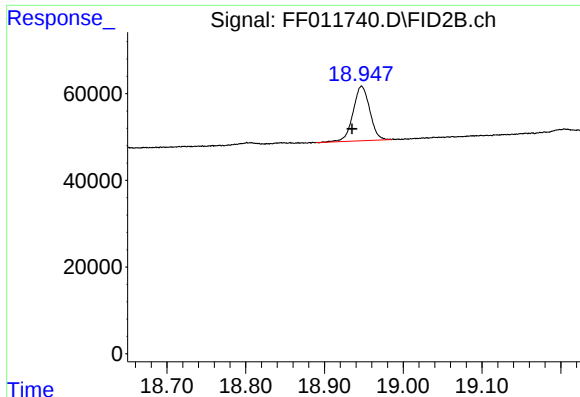

#14 N-DOTRIACONTANE


R.T.: 18.947 min
Delta R.T.: 0.012 min
Response: 185497
Conc: 1.38 ug/ml

Instrument :
FID_F
ClientSampleId :

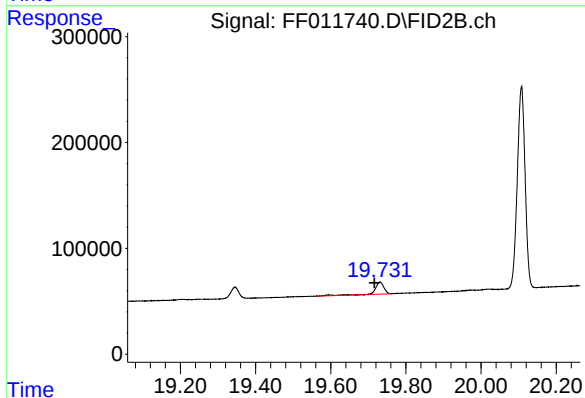


#15 N-TETRATRIACONTANE

R.T.: 19.731 min
Delta R.T.: 0.015 min
Response: 181964
Conc: 1.38 ug/ml

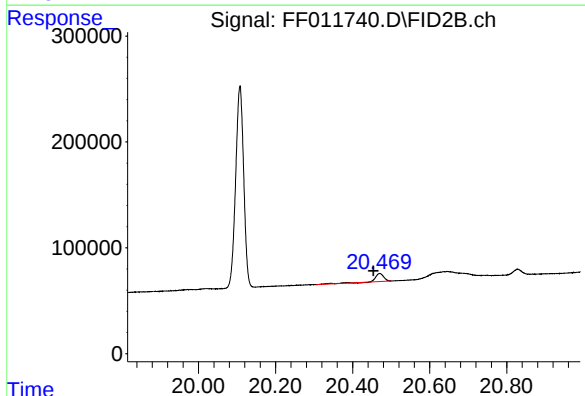

#16 N-HEXATRIACONTANE

R.T.: 20.470 min
Delta R.T.: 0.016 min
Response: 115255
Conc: 0.94 ug/ml

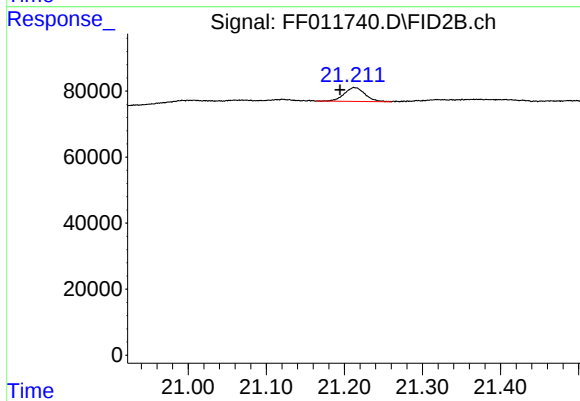

#17 N-OCTATRIACONTANE

R.T.: 21.213 min
Delta R.T.: 0.018 min
Response: 76995
Conc: 0.66 ug/ml