

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
 Data File : FF011741.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2022 16:37
 Operator : YP\AJ
 Sample : N5607-02 2X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 16 04:36:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	812916	6.852 ug/ml
Target Compounds			
6) N-OCTADECANE	11.659	154671	1.118 ug/ml
7) N-EICOSANE	12.950	212615	1.537 ug/ml
8) N-DOCOSANE	14.155	88817	0.658 ug/ml
10) N-TETRACOSANE	15.240	706952	5.213 ug/ml
11) N-HEXACOSANE	16.281	162505	1.216 ug/ml
12) N-OCTACOSANE	17.235	333148	2.515 ug/ml
13) N-TRIACONTANE	18.116	488714	3.706 ug/ml
14) N-DOTRIACONTANE	18.950	302426	2.247 ug/ml
15) N-TETRATRIACONTANE	19.735	154796	1.175 ug/ml
16) N-HEXATRIACONTANE	20.435	65725	0.534 ug/ml
17) N-OCTATRIACONTANE	21.216	121113	1.040 ug/ml
18) N-TETRACONTANE	22.141	127082	1.169 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
Data File : FF011741.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2022 16:37
Operator : YP\AJ
Sample : N5607-02 2X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 04:36:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

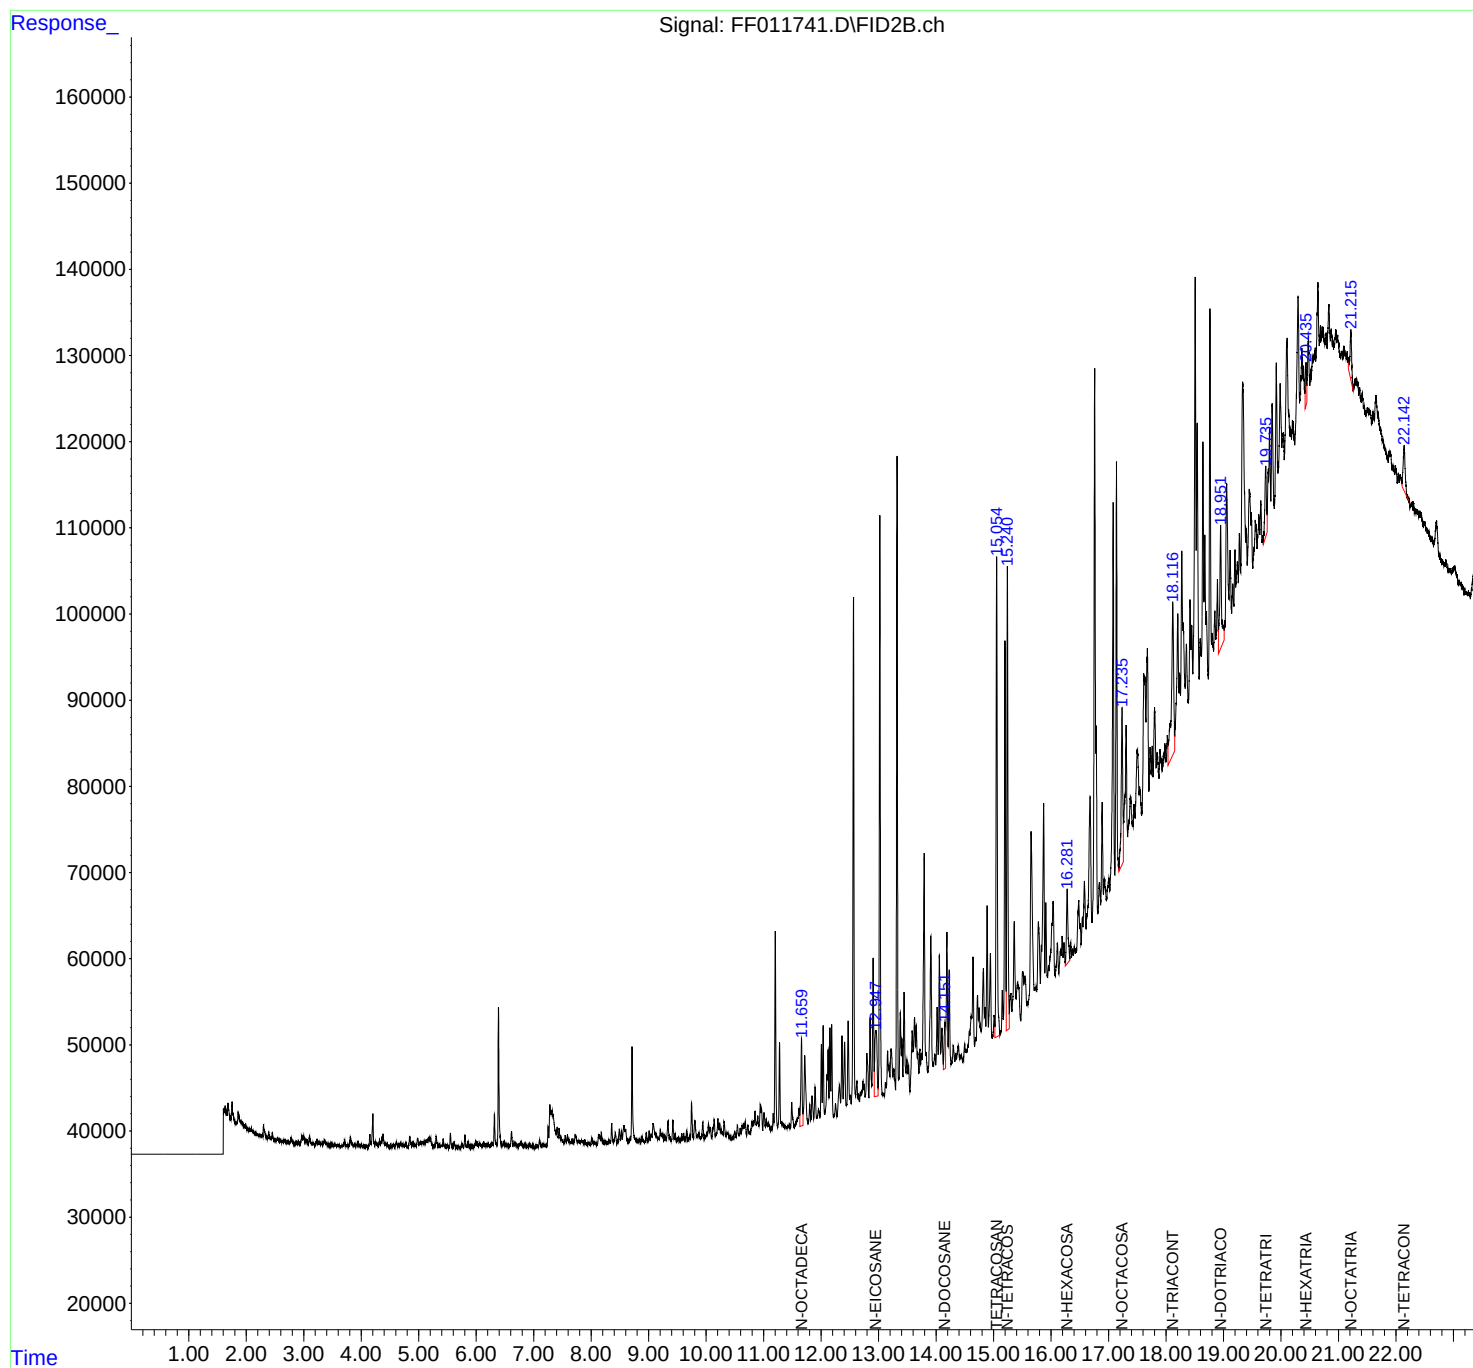


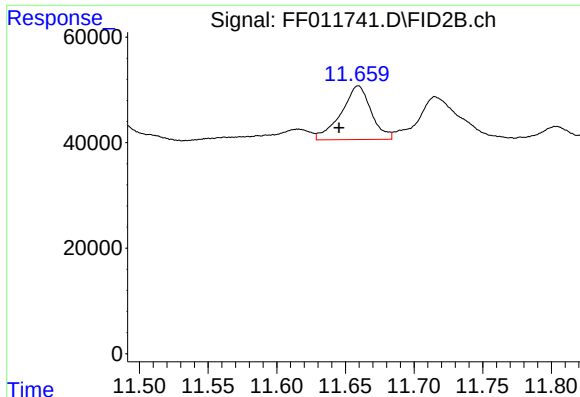

#6 N-OCTADECANE


R.T.: 11.659 min
Delta R.T.: 0.014 min
Response: 154671
Conc: 1.12 ug/ml

Instrument :
FID_F
ClientSampleId :

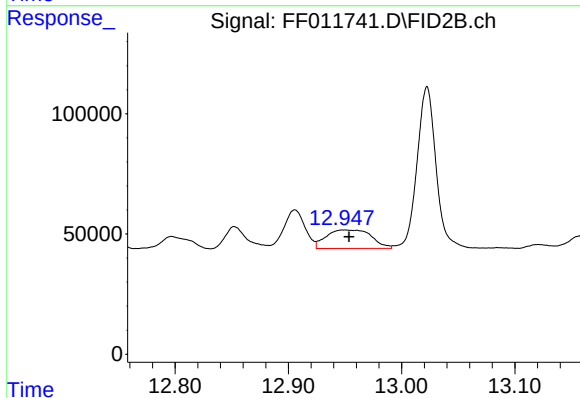


#7 N-EICOSANE

R.T.: 12.950 min
Delta R.T.: -0.004 min
Response: 212615
Conc: 1.54 ug/ml

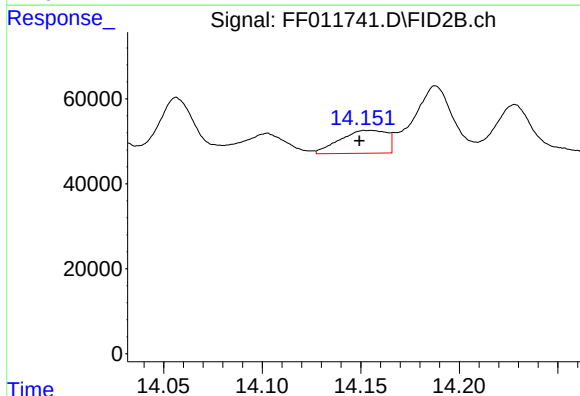


#8 N-DOCOSANE

R.T.: 14.155 min
Delta R.T.: 0.005 min
Response: 88817
Conc: 0.66 ug/ml

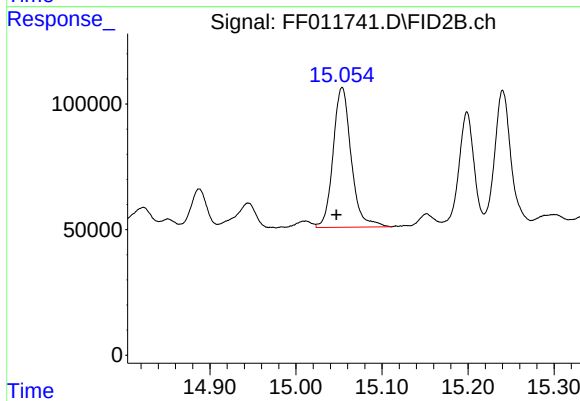

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.054 min
Delta R.T.: 0.007 min
Response: 812916
Conc: 6.85 ug/ml

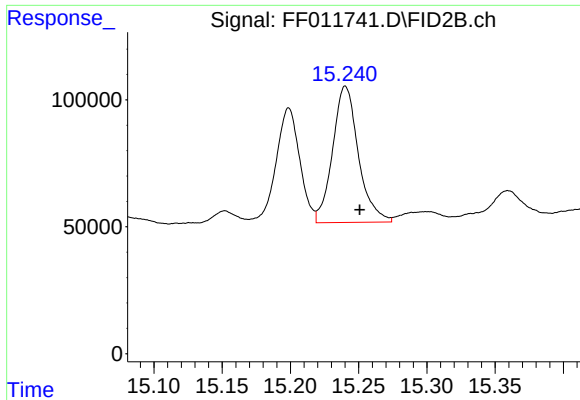

#10 N-TETRACOSANE


R.T.: 15.240 min
Delta R.T.: -0.011 min
Response: 706952
Conc: 5.21 ug/ml

Instrument :
FID_F
ClientSampleId :

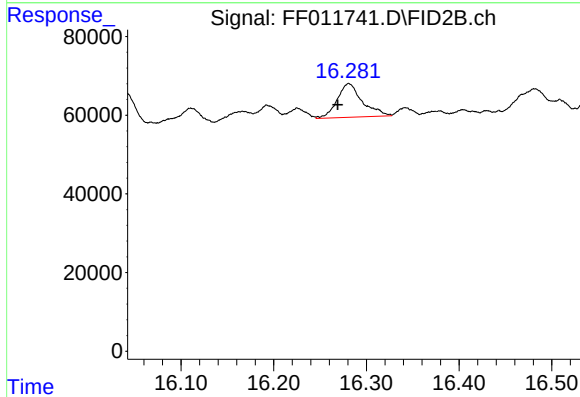


#11 N-HEXACOSANE

R.T.: 16.281 min
Delta R.T.: 0.012 min
Response: 162505
Conc: 1.22 ug/ml

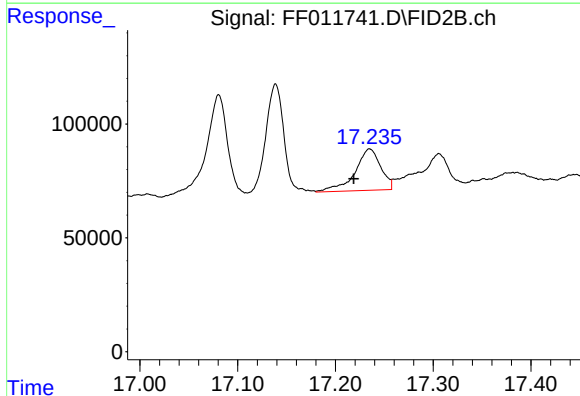


#12 N-OCTACOSANE

R.T.: 17.235 min
Delta R.T.: 0.016 min
Response: 333148
Conc: 2.51 ug/ml

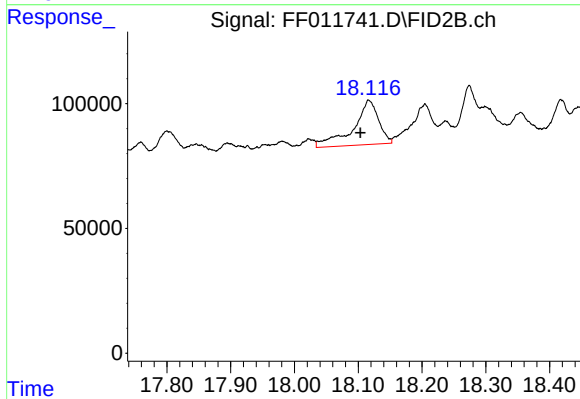

#13 N-TRIACONTANE


R.T.: 18.116 min
Delta R.T.: 0.013 min
Response: 488714
Conc: 3.71 ug/ml

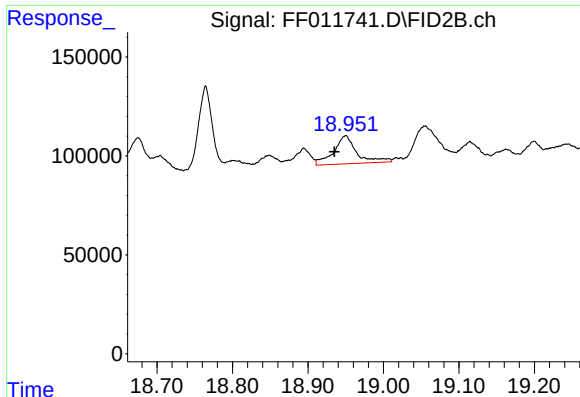

#14 N-DOTRIACONTANE


R.T.: 18.950 min
Delta R.T.: 0.015 min
Response: 302426
Conc: 2.25 ug/ml

Instrument :
FID_F
ClientSampleId :

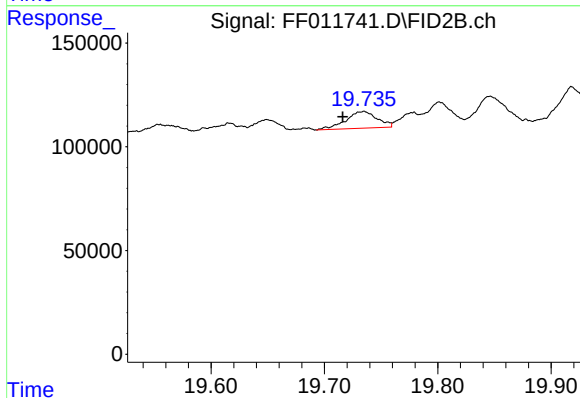


#15 N-TETRATRIACONTANE

R.T.: 19.735 min
Delta R.T.: 0.019 min
Response: 154796
Conc: 1.18 ug/ml

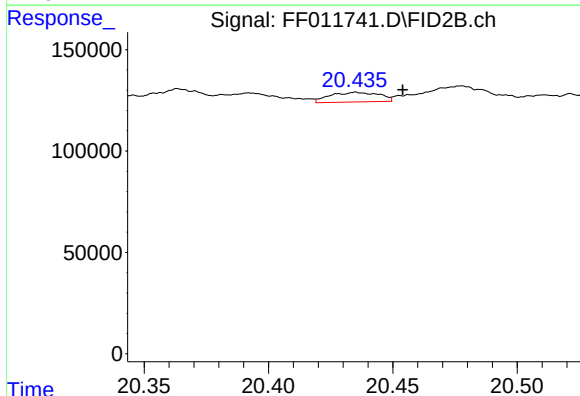


#16 N-HEXATRIACONTANE

R.T.: 20.435 min
Delta R.T.: -0.019 min
Response: 65725
Conc: 0.53 ug/ml

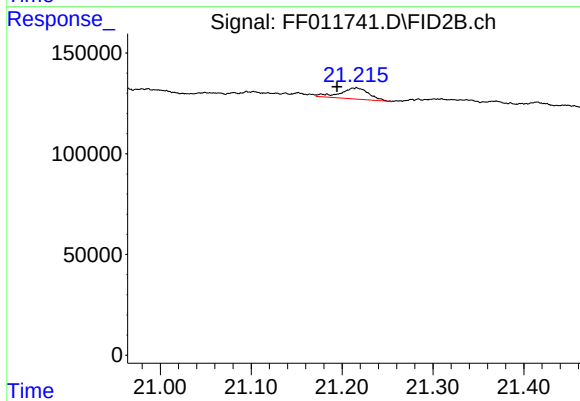

#17 N-OCTATRIACONTANE

R.T.: 21.216 min
Delta R.T.: 0.022 min
Response: 121113
Conc: 1.04 ug/ml

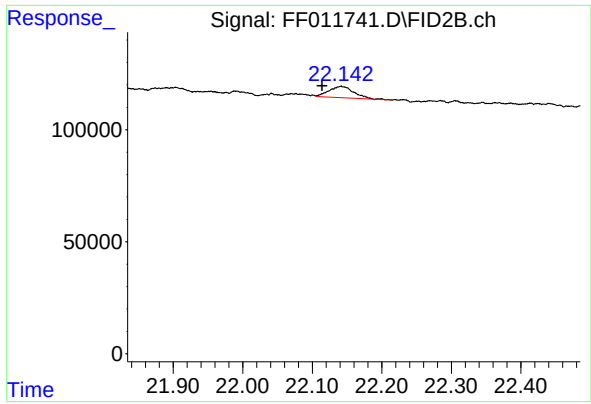

#18 N-TETRACONTANE

R.T.: 22.141 min
Delta R.T.: 0.027 min
Response: 127082
Conc: 1.17 ug/ml

Instrument :
FID_F
ClientSampleId :