

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
 Data File : FF011742.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2022 17:07
 Operator : YP\AJ
 Sample : N5607-04 5X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 16 04:36:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	564492	4.758 ug/ml
Target Compounds			
6) N-OCTADECANE	11.657	48312	0.349 ug/ml
7) N-EICOSANE	12.944	127104	0.919 ug/ml
8) N-DOCOSANE	14.188	287591	2.131 ug/ml
10) N-TETRACOSANE	15.241	627361	4.626 ug/ml
11) N-HEXACOSANE	16.282	117815	0.882 ug/ml
12) N-OCTACOSANE	17.235	285372	2.154 ug/ml
13) N-TRIACONTANE	18.114	229165	1.738 ug/ml
14) N-DOTRIACONTANE	18.949	260261	1.934 ug/ml
15) N-TETRATRIACONTANE	19.731	107996	0.820 ug/ml
16) N-HEXATRIACONTANE	20.437	149717	1.216 ug/ml
18) N-TETRACONTANE	22.143	131329	1.208 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
Data File : FF011742.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2022 17:07
Operator : YP\AJ
Sample : N5607-04 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 04:36:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

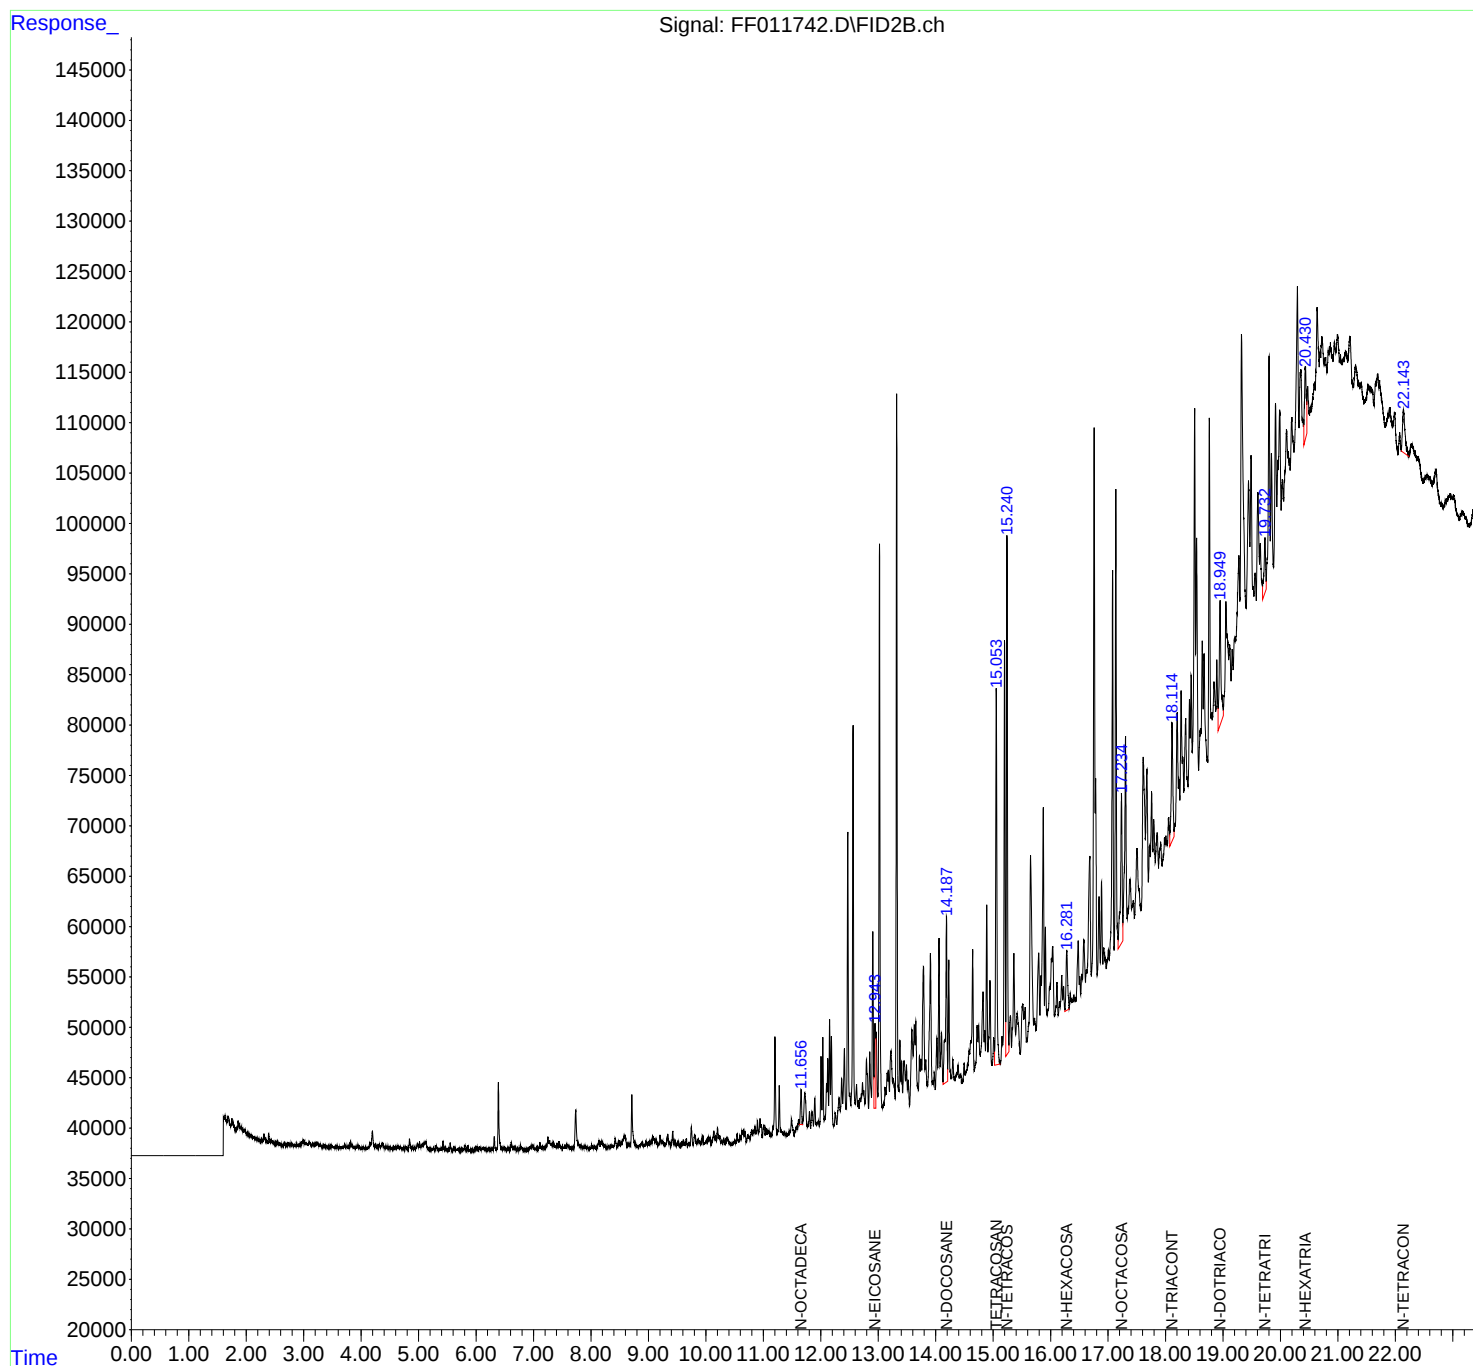


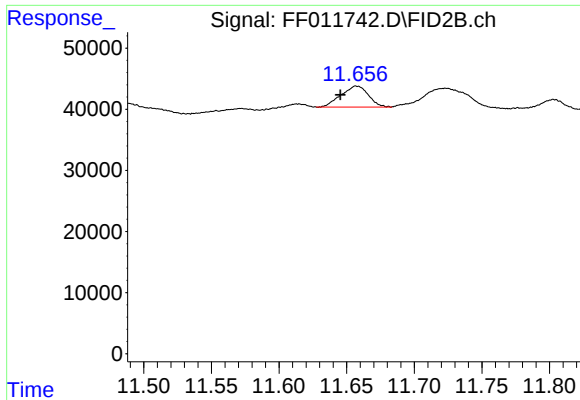

#6 N-OCTADECANE


R.T.: 11.657 min
Delta R.T.: 0.012 min
Response: 48312
Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :

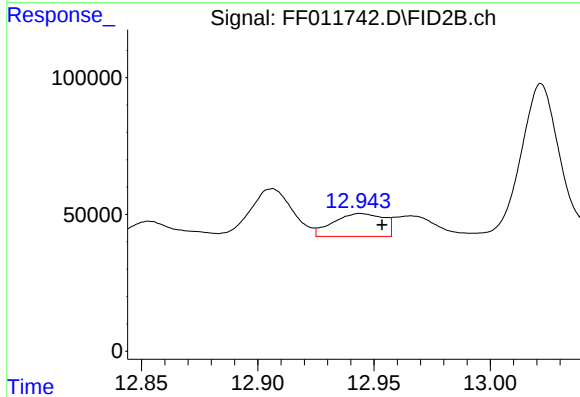


#7 N-EICOSANE

R.T.: 12.944 min
Delta R.T.: -0.009 min
Response: 127104
Conc: 0.92 ug/ml

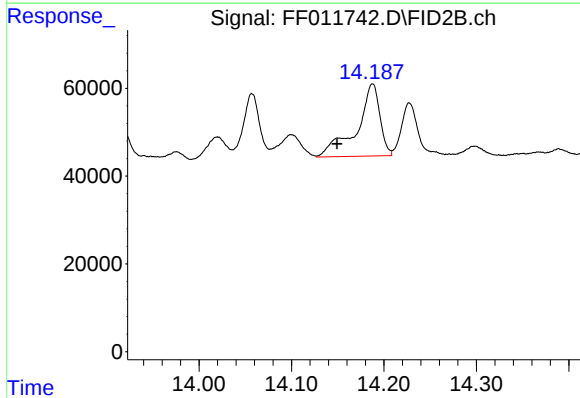


#8 N-DOCOSANE

R.T.: 14.188 min
Delta R.T.: 0.038 min
Response: 287591
Conc: 2.13 ug/ml

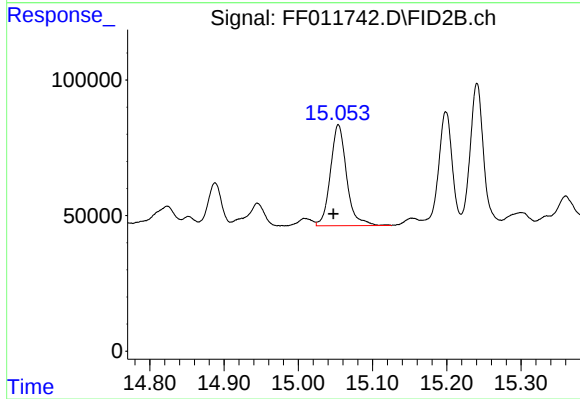

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.054 min
Delta R.T.: 0.007 min
Response: 564492
Conc: 4.76 ug/ml

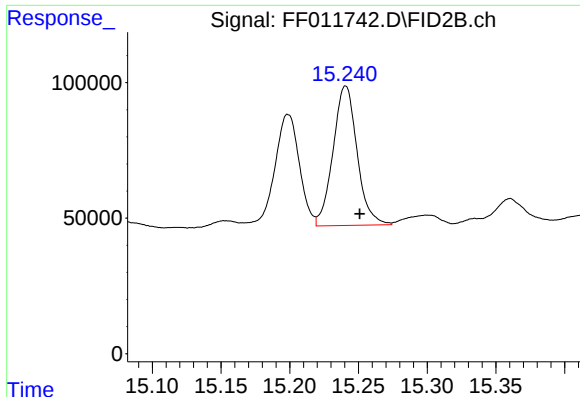

#10 N-TETRACOSANE


R.T.: 15.241 min
Delta R.T.: -0.010 min
Response: 627361
Conc: 4.63 ug/ml

Instrument :
FID_F
ClientSampleId :

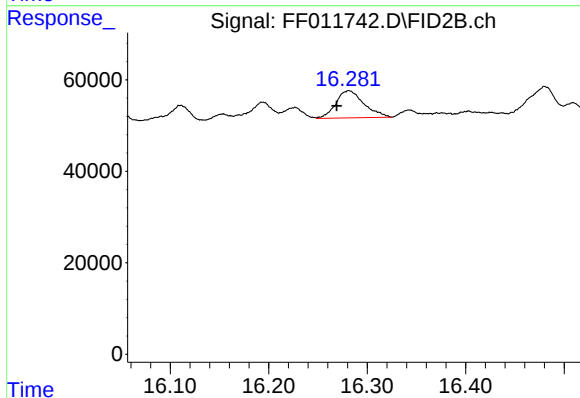


#11 N-HEXACOSANE

R.T.: 16.282 min
Delta R.T.: 0.013 min
Response: 117815
Conc: 0.88 ug/ml

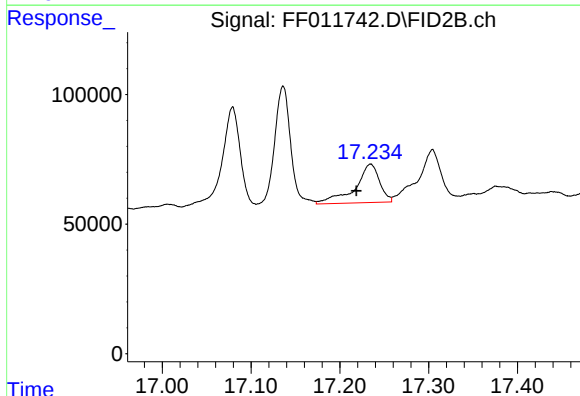


#12 N-OCTACOSANE

R.T.: 17.235 min
Delta R.T.: 0.016 min
Response: 285372
Conc: 2.15 ug/ml

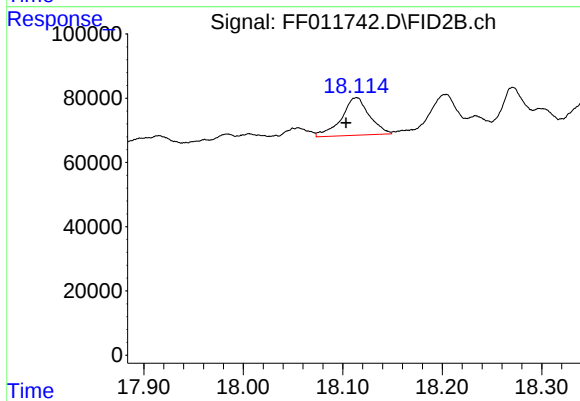

#13 N-TRIACONTANE


R.T.: 18.114 min
Delta R.T.: 0.010 min
Response: 229165
Conc: 1.74 ug/ml

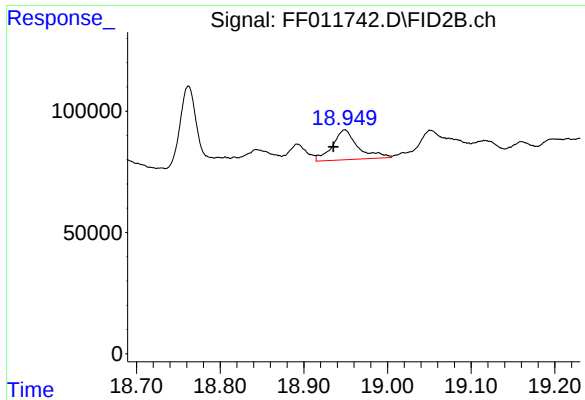

#14 N-DOTRIACONTANE


R.T.: 18.949 min
Delta R.T.: 0.014 min
Response: 260261
Conc: 1.93 ug/ml

Instrument :
FID_F
ClientSampleId :

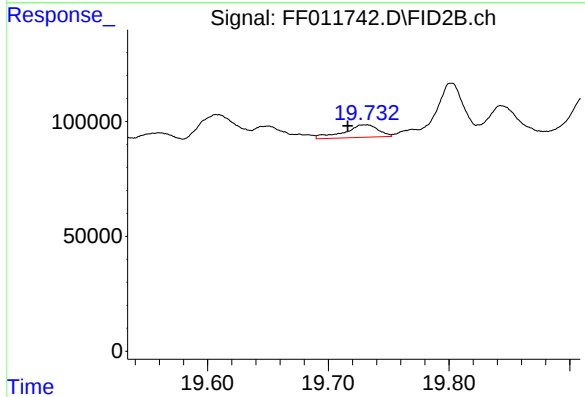


#15 N-TETRATRIACONTANE

R.T.: 19.731 min
Delta R.T.: 0.015 min
Response: 107996
Conc: 0.82 ug/ml

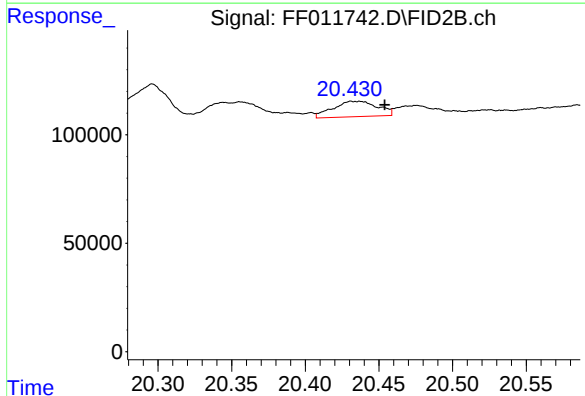

#16 N-HEXATRIACONTANE

R.T.: 20.437 min
Delta R.T.: -0.017 min
Response: 149717
Conc: 1.22 ug/ml

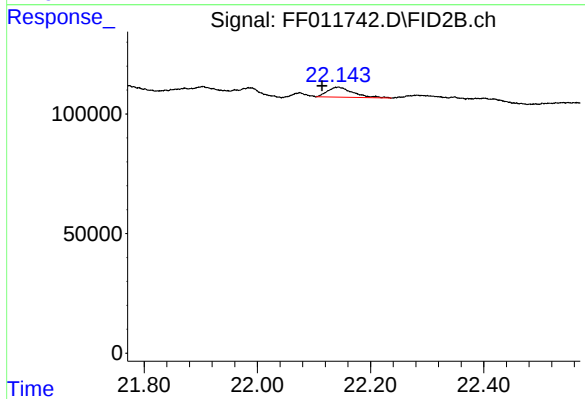

#18 N-TETRACONTANE

R.T.: 22.143 min
Delta R.T.: 0.029 min
Response: 131329
Conc: 1.21 ug/ml