

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
 Data File : FF011743.D
 Signal(s) : FID2B.ch
 Acq On : 15 Nov 2022 17:36
 Operator : YP\AJ
 Sample : N5607-06 5X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 16 04:36:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.052	467822	3.943 ug/ml
Target Compounds			
7) N-EICOSANE	12.943	150806	1.090 ug/ml
8) N-DOCOSANE	14.188	309431	2.292 ug/ml
10) N-TETRACOSANE	15.240	822885	6.068 ug/ml
11) N-HEXACOSANE	16.283	96632	0.723 ug/ml
12) N-OCTACOSANE	17.237	260405	1.966 ug/ml
13) N-TRIACONTANE	18.115	212571	1.612 ug/ml
14) N-DOTRIACONTANE	18.949	123624	0.918 ug/ml
15) N-TETRATRIACONTANE	19.732	60867	0.462 ug/ml
16) N-HEXATRIACONTANE	20.441	132576	1.076 ug/ml
18) N-TETRACONTANE	22.141	123801	1.138 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111522\
Data File : FF011743.D
Signal(s) : FID2B.ch
Acq On : 15 Nov 2022 17:36
Operator : YP\AJ
Sample : N5607-06 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 04:36:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

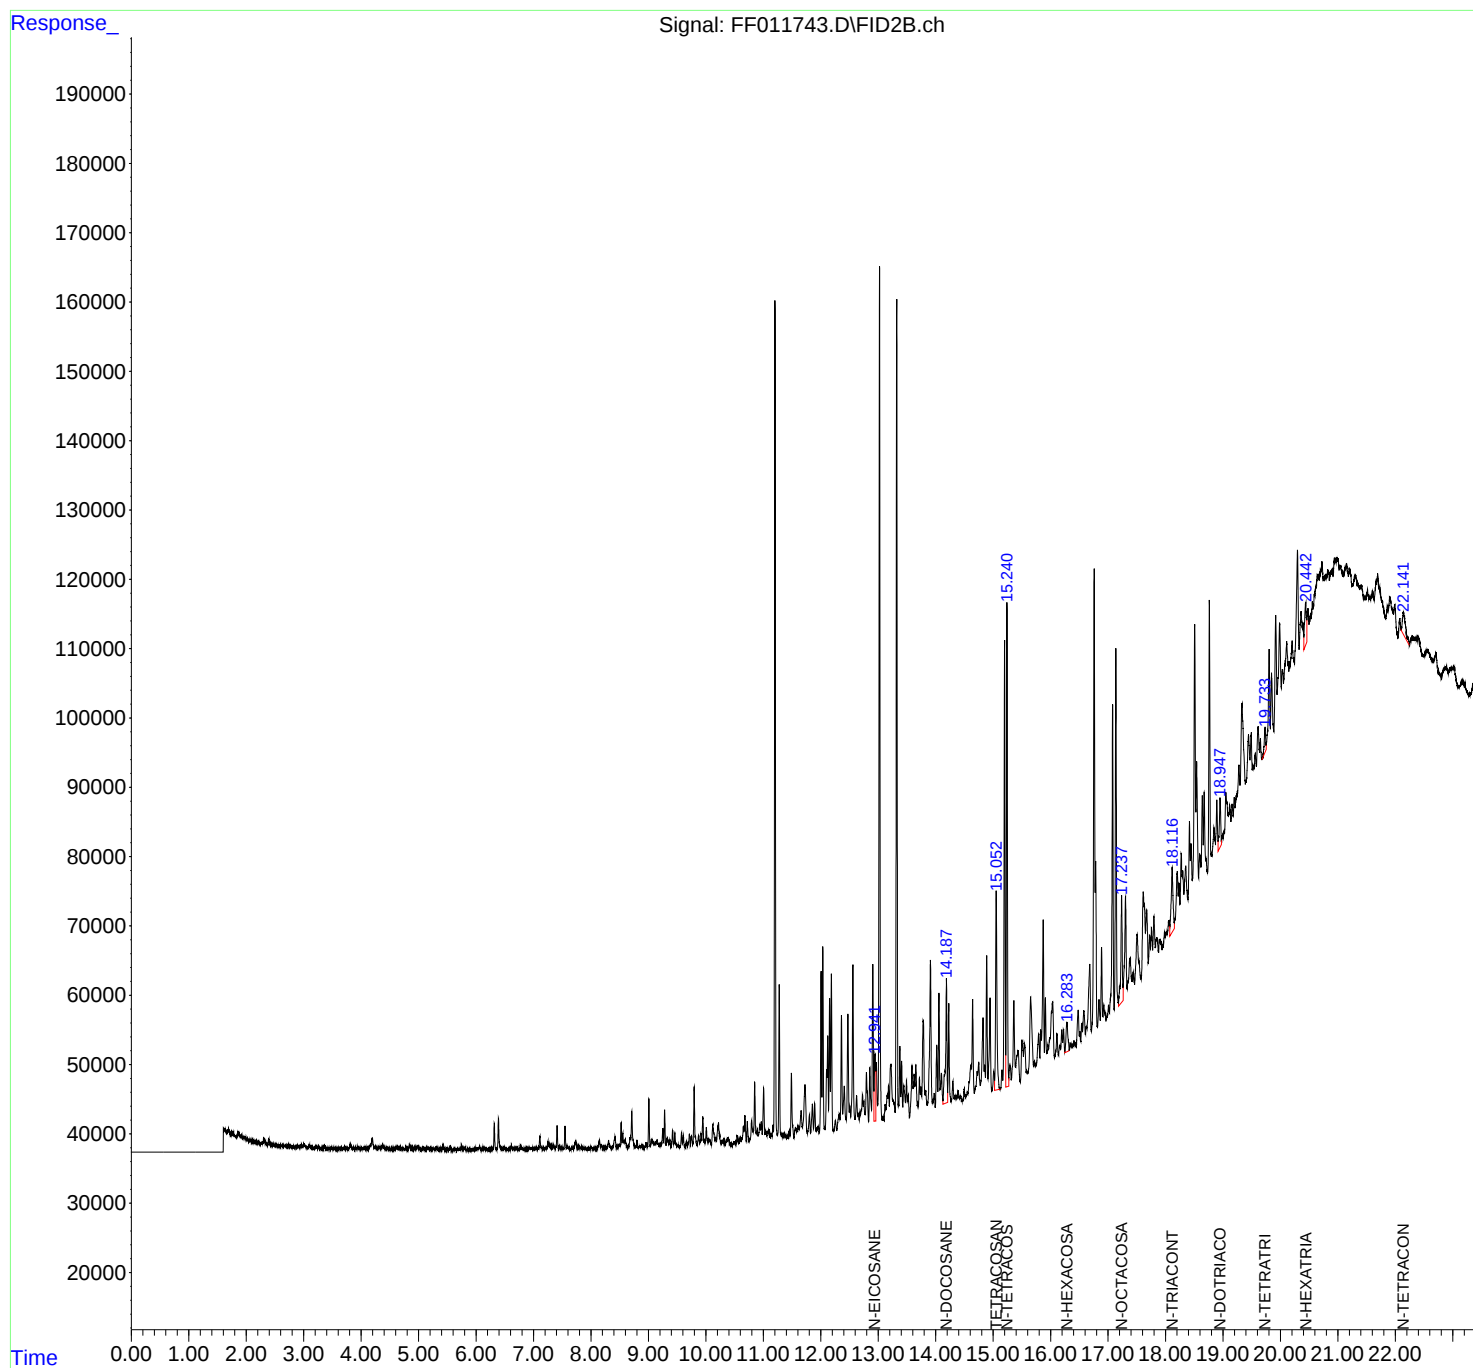


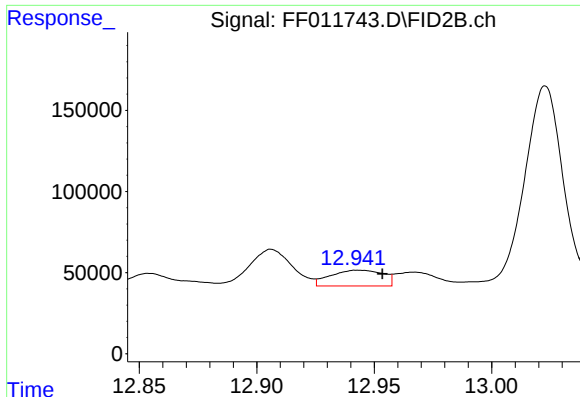

#7 N-EICOSANE


R.T.: 12.943 min
Delta R.T.: -0.010 min
Response: 150806
Conc: 1.09 ug/ml

Instrument :
FID_F
ClientSampleId :

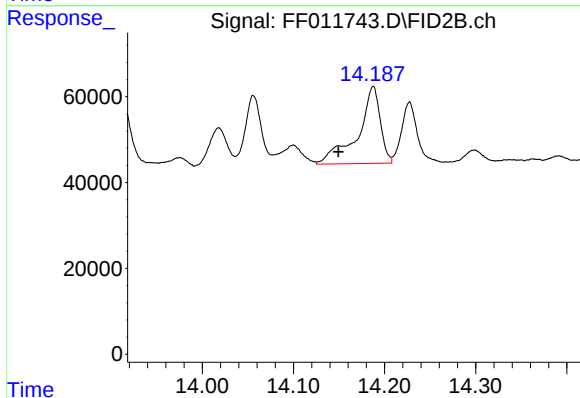


#8 N-DOCOSANE

R.T.: 14.188 min
Delta R.T.: 0.038 min
Response: 309431
Conc: 2.29 ug/ml

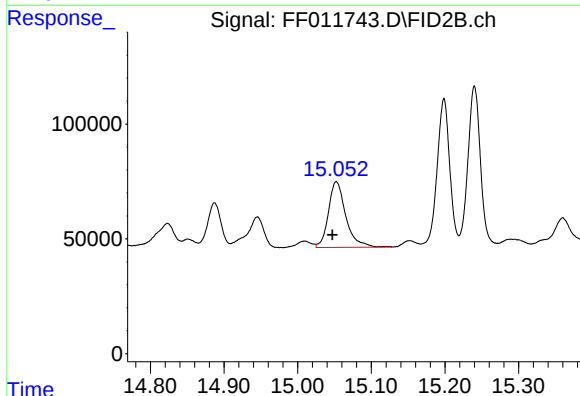


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.052 min
Delta R.T.: 0.005 min
Response: 467822
Conc: 3.94 ug/ml

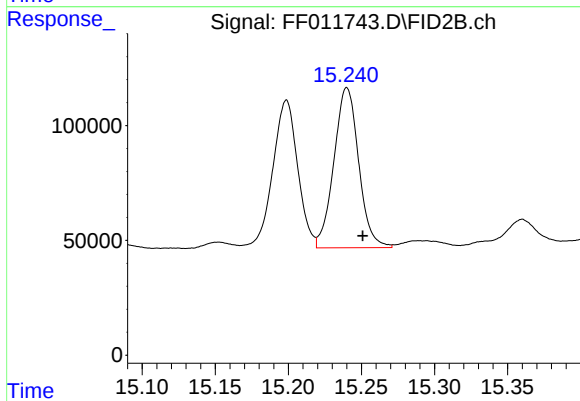

#10 N-TETRACOSANE


R.T.: 15.240 min
Delta R.T.: -0.011 min
Response: 822885
Conc: 6.07 ug/ml

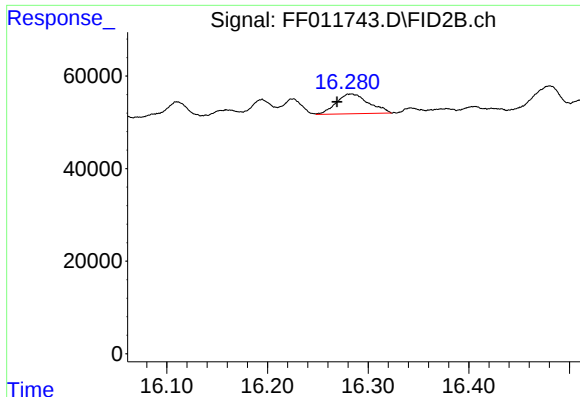

#11 N-HEXACOSANE


R.T.: 16.283 min
Delta R.T.: 0.014 min
Response: 96632
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

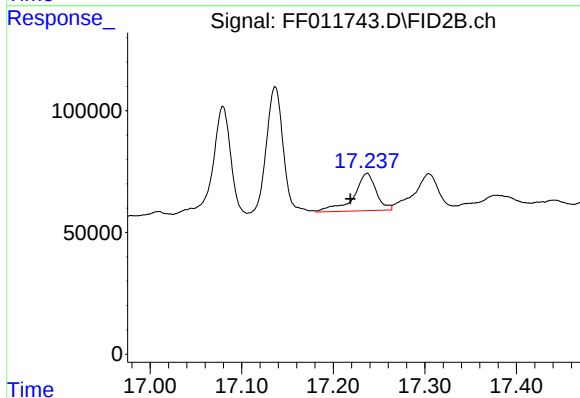


#12 N-OCTACOSANE

R.T.: 17.237 min
Delta R.T.: 0.018 min
Response: 260405
Conc: 1.97 ug/ml

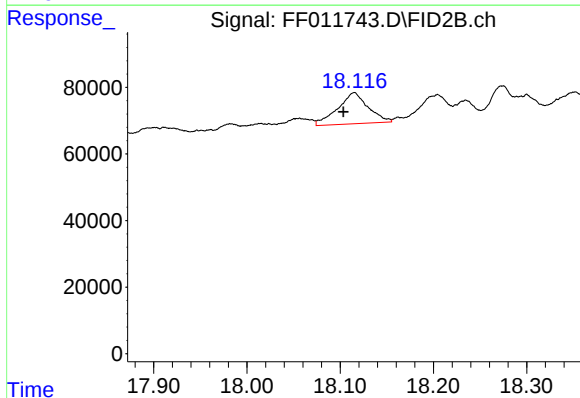


#13 N-TRIACONTANE

R.T.: 18.115 min
Delta R.T.: 0.012 min
Response: 212571
Conc: 1.61 ug/ml

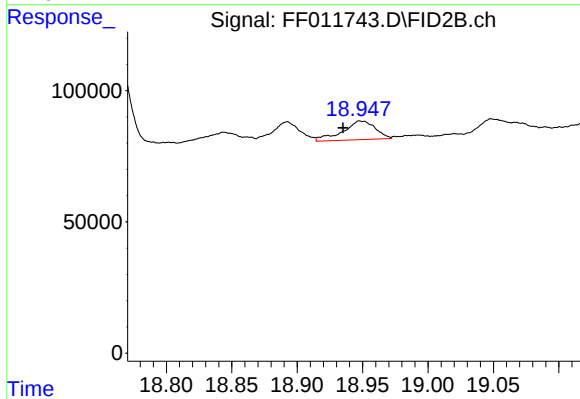

#14 N-DOTRIACONTANE


R.T.: 18.949 min
Delta R.T.: 0.013 min
Response: 123624
Conc: 0.92 ug/ml

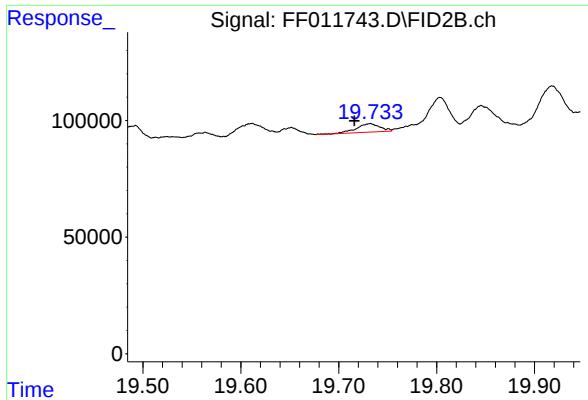

#15 N-TETRATRIACONTANE


R.T.: 19.732 min
Delta R.T.: 0.016 min
Response: 60867
Conc: 0.46 ug/ml

Instrument :
FID_F
ClientSampleId :

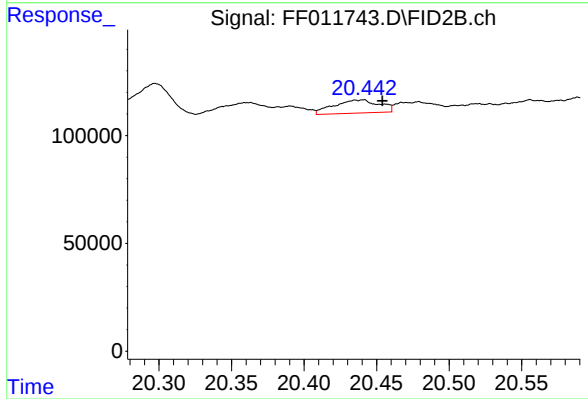

#16 N-HEXATRIACONTANE

R.T.: 20.441 min
Delta R.T.: -0.013 min
Response: 132576
Conc: 1.08 ug/ml

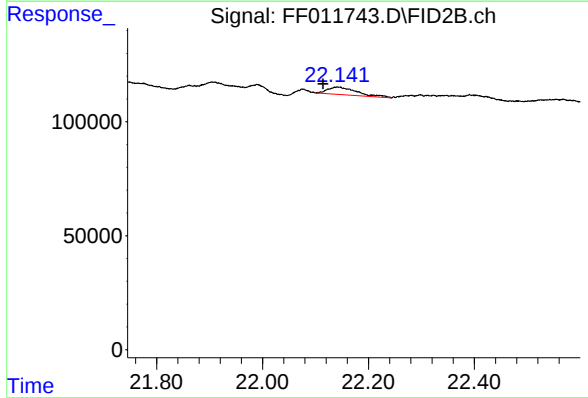

#18 N-TETRACONTANE

R.T.: 22.141 min
Delta R.T.: 0.027 min
Response: 123801
Conc: 1.14 ug/ml