

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF111522\  
 Data File : FF011745.D  
 Signal(s) : FID2B.ch  
 Acq On : 15 Nov 2022 19:05  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Nov 16 04:37:02 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF110422.M  
 Quant Title :  
 QLast Update : Fri Nov 04 14:11:34 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.054 | 1961286  | 16.531 ug/ml |
| Target Compounds              |        |          |              |
| 13) N-TRIACONTANE             | 18.115 | 64992    | 0.493 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.948 | 91270    | 0.678 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.732 | 84351    | 0.640 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.471 | 146267   | 1.188 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF111522\  
Data File : FF011745.D  
Signal(s) : FID2B.ch  
Acq On : 15 Nov 2022 19:05  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Nov 16 04:37:02 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF110422.M  
Quant Title :  
QLast Update : Fri Nov 04 14:11:34 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

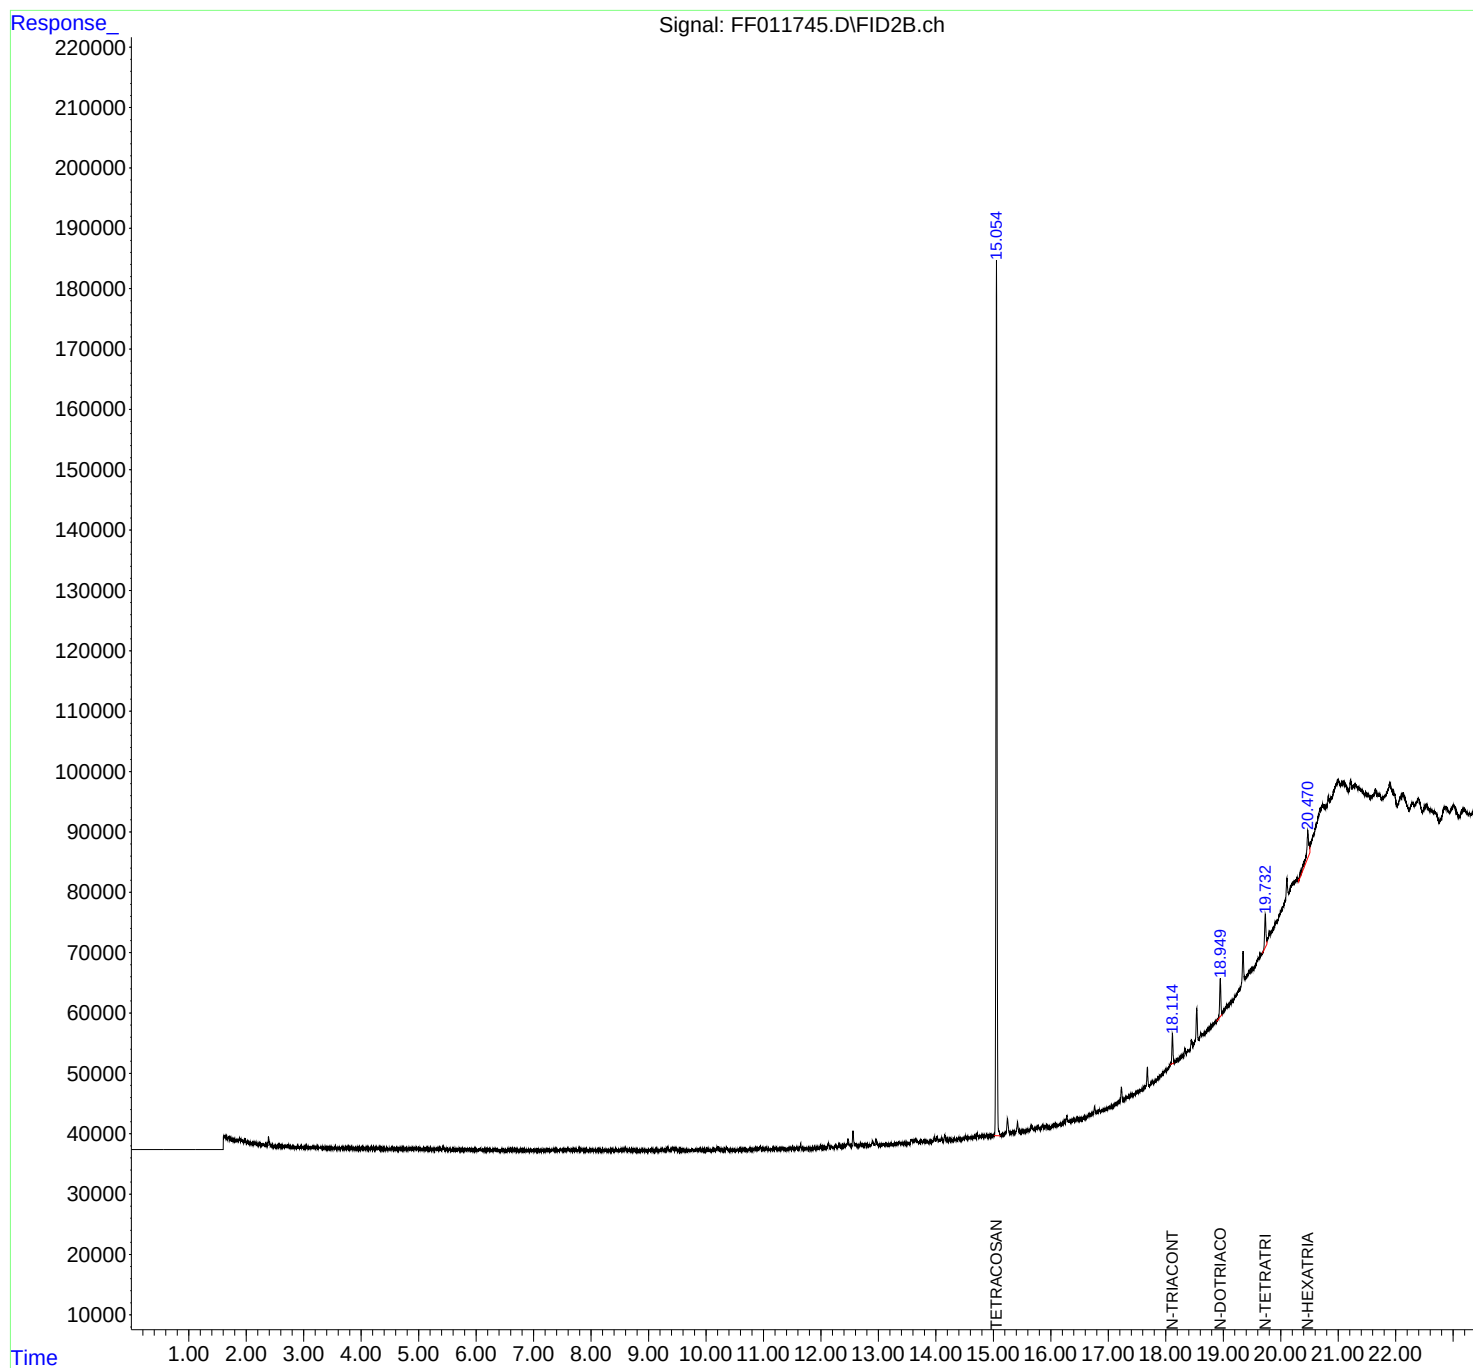


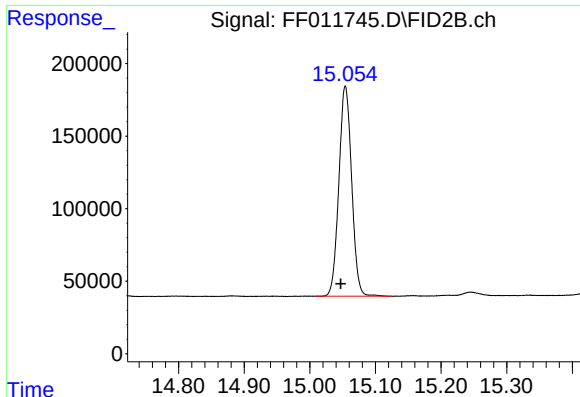

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.054 min  
Delta R.T.: 0.007 min  
Response: 1961286  
Conc: 16.53 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

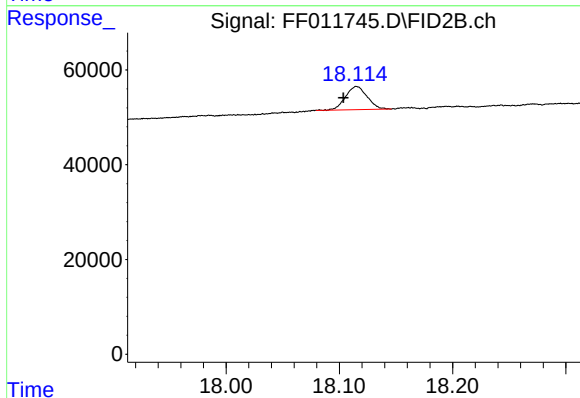


#13 N-TRIACONTANE

R.T.: 18.115 min  
Delta R.T.: 0.012 min  
Response: 64992  
Conc: 0.49 ug/ml

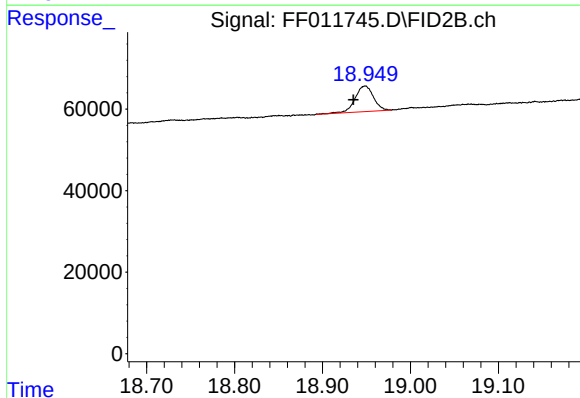


#14 N-DOTRIACONTANE

R.T.: 18.948 min  
Delta R.T.: 0.013 min  
Response: 91270  
Conc: 0.68 ug/ml

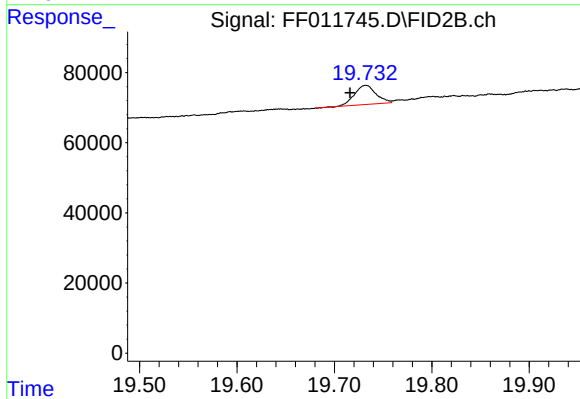

#15 N-TETRATRIACONTANE

R.T.: 19.732 min  
Delta R.T.: 0.016 min  
Response: 84351  
Conc: 0.64 ug/ml

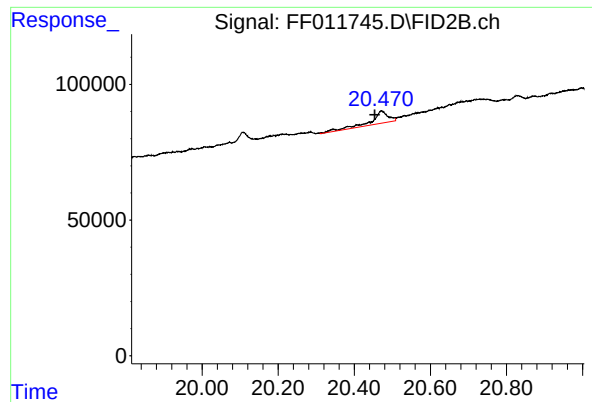

#16 N-HEXATRIACONTANE

R.T.: 20.471 min  
Delta R.T.: 0.017 min  
Response: 146267  
Conc: 1.19 ug/ml

Instrument :

FID\_F

ClientSampleId :