

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111820\
Data File : FF007891.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2020 11:21
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 19 00:16:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.455	3489130	25.207 ug/ml
12)	N-OCTACOSANE	16.892	3103517	22.881 ug/ml
13)	N-TRIACONTANE	17.781	97580	0.754 ug/ml
14)	N-DOTRIACONTANE	18.617	155406	1.341 ug/ml
15)	N-TETRATRIACONTANE	19.404	103556	1.103 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111820\
Data File : FF007891.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2020 11:21
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 19 00:16:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

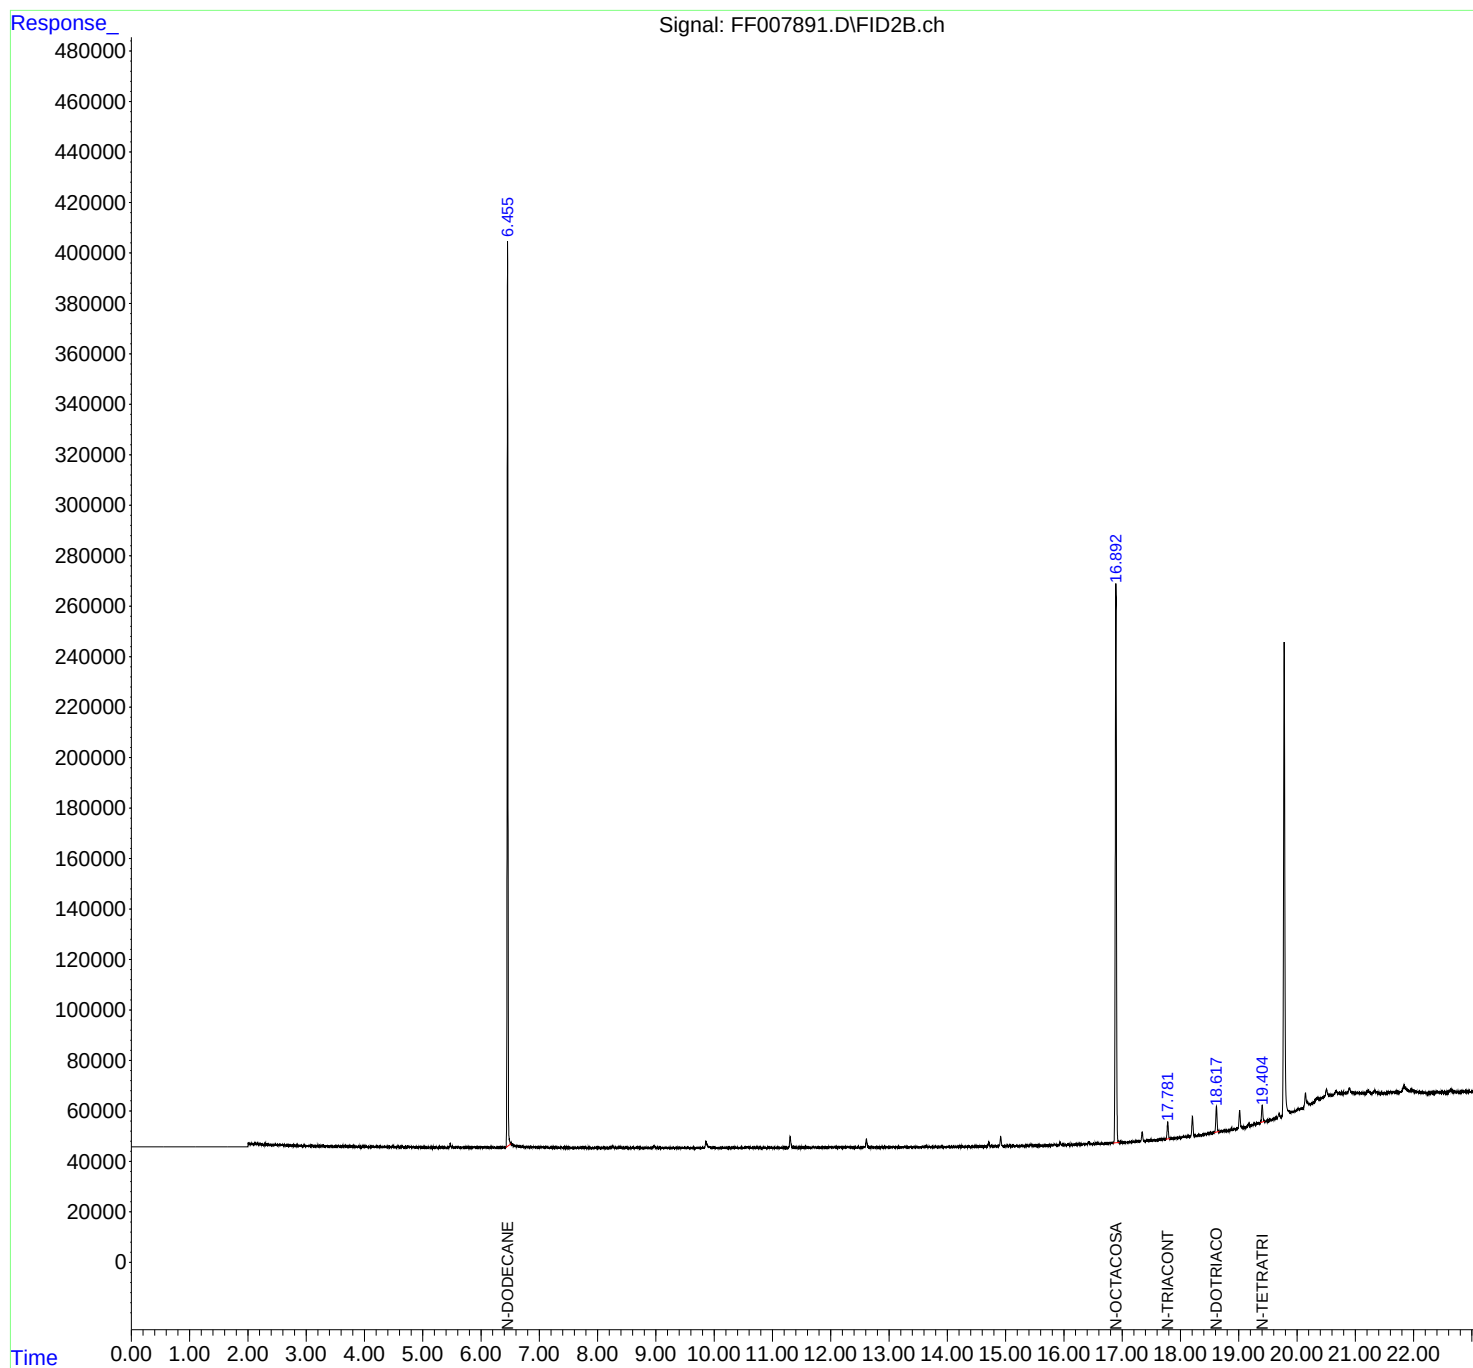


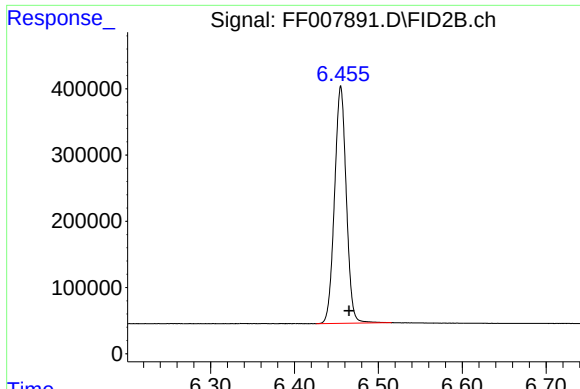

#3 N-DODECANE


R.T.: 6.455 min
Delta R.T.: -0.010 min
Response: 3489130
Conc: 25.21 ug/ml

Instrument :
FID_F
ClientSampleId :

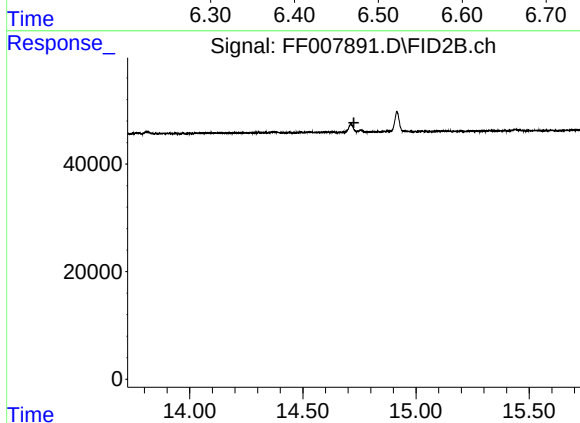


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.726 min
Response: 0
Conc: N.D.

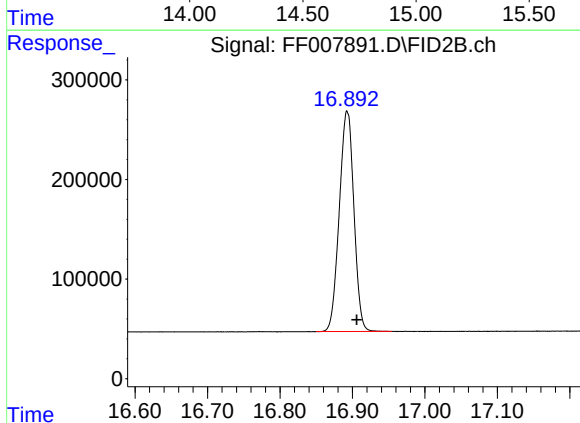


#12 N-OCTACOSANE

R.T.: 16.892 min
Delta R.T.: -0.014 min
Response: 3103517
Conc: 22.88 ug/ml

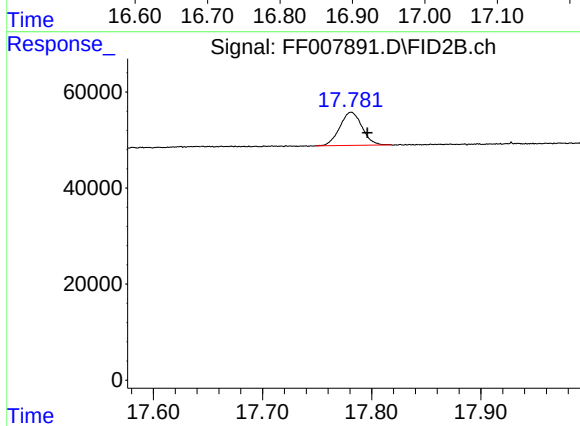

#13 N-TRIACONTANE


R.T.: 17.781 min
Delta R.T.: -0.015 min
Response: 97580
Conc: 0.75 ug/ml

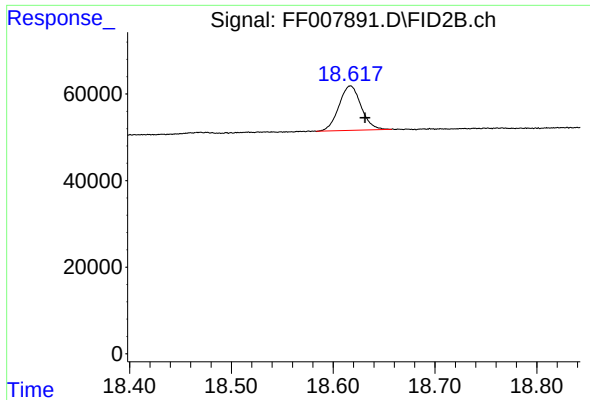

#14 N-DOTRIACONTANE

R.T.: 18.617 min
Delta R.T.: -0.014 min
Response: 155406
Conc: 1.34 ug/ml

Instrument :
FID_F
ClientSampleId :

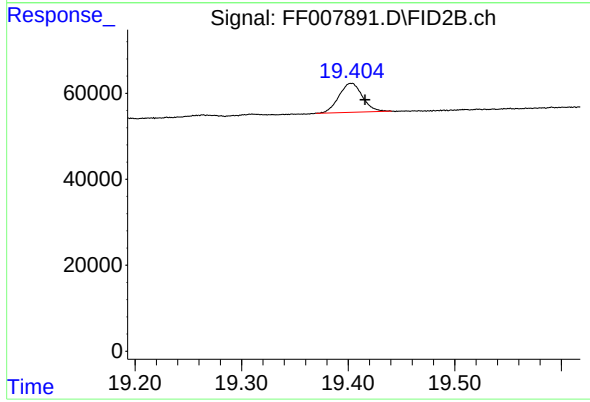

#15 N-TETRATRIACONTANE

R.T.: 19.404 min
Delta R.T.: -0.012 min
Response: 103556
Conc: 1.10 ug/ml